
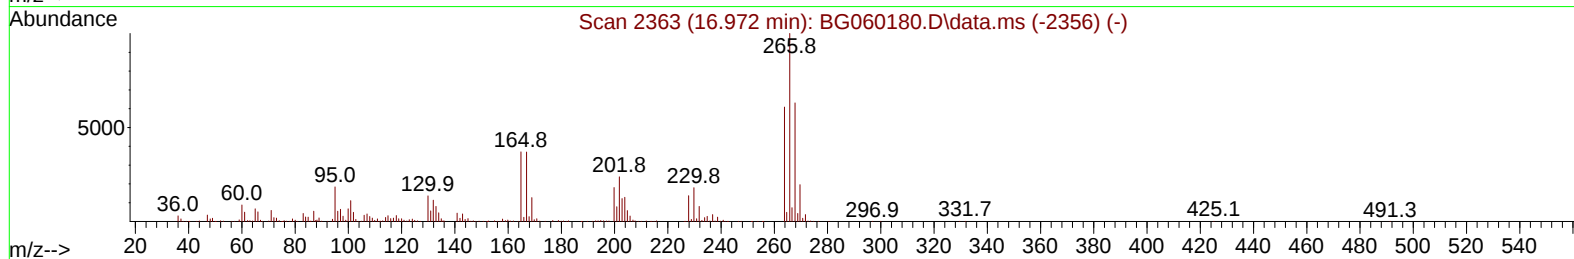
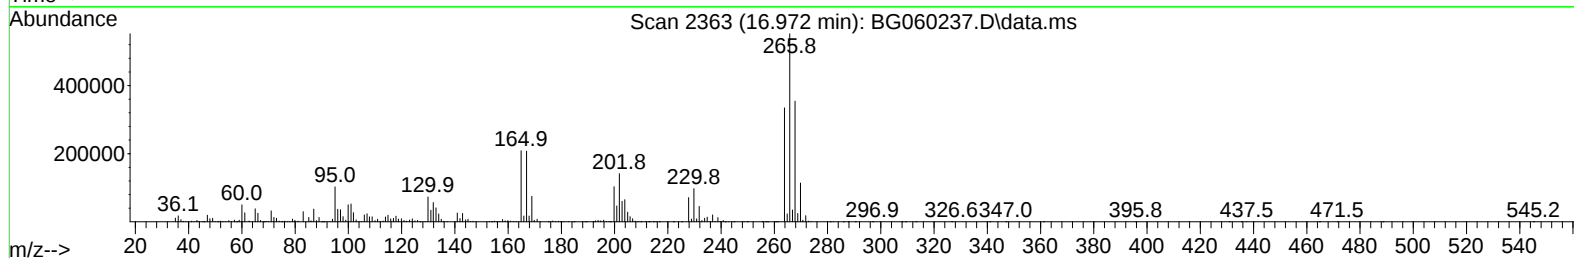


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010424\
Data File : BG060237.D
Acq On : 4 Jan 2024 9:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 11:19:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

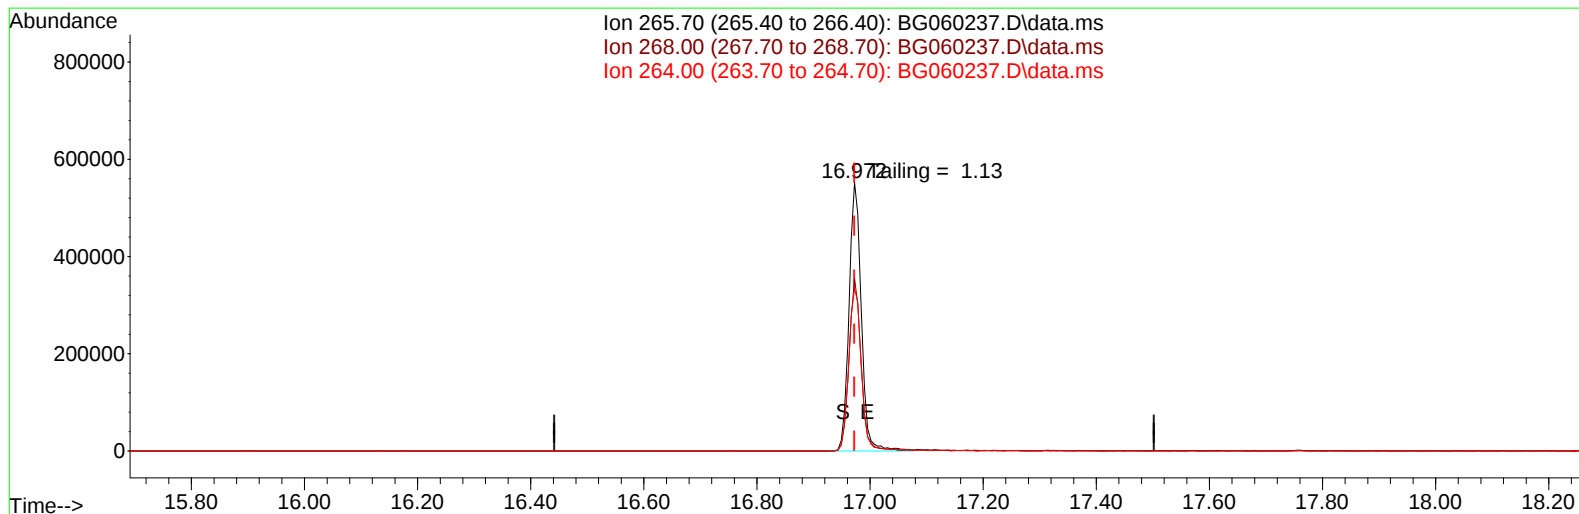

TIC: BG060237.D\data.ms

(70) Pentachlorophenol (C)




16.972min (+ 0.001) 1132366.21 ng

response 835129

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.16
264.00	65.80	60.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010424\
Data File : BG060237.D
Acq On : 4 Jan 2024 9:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 11:19:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

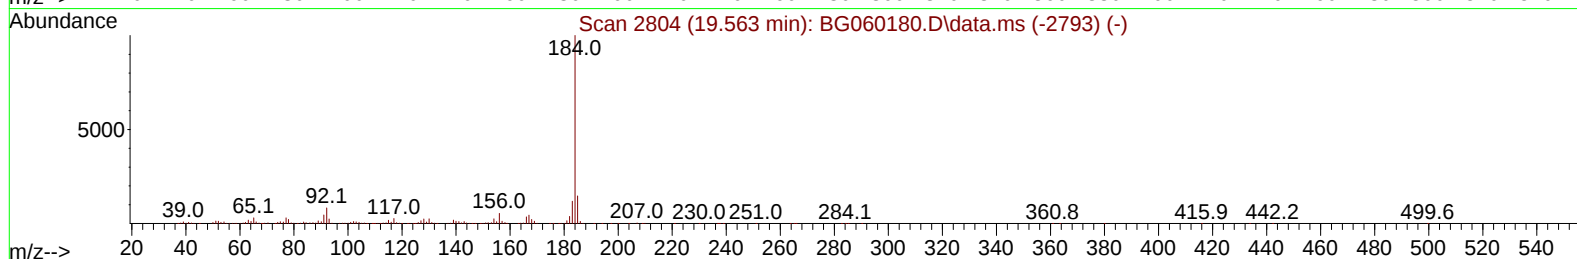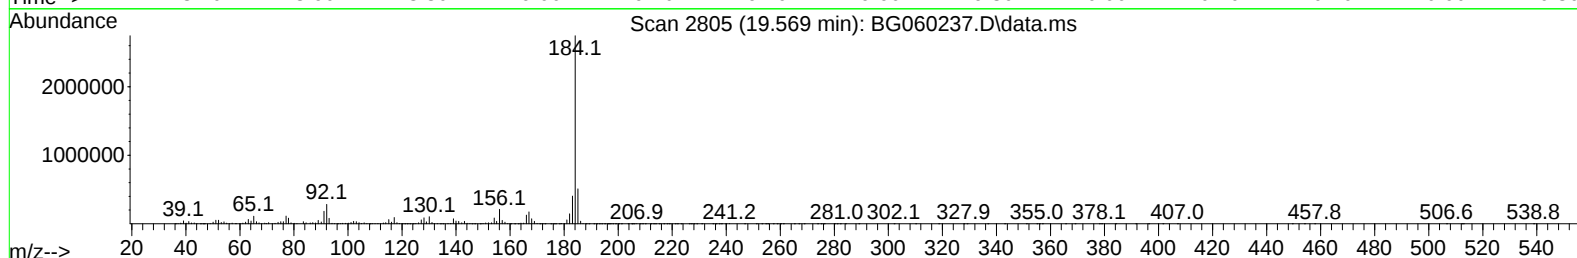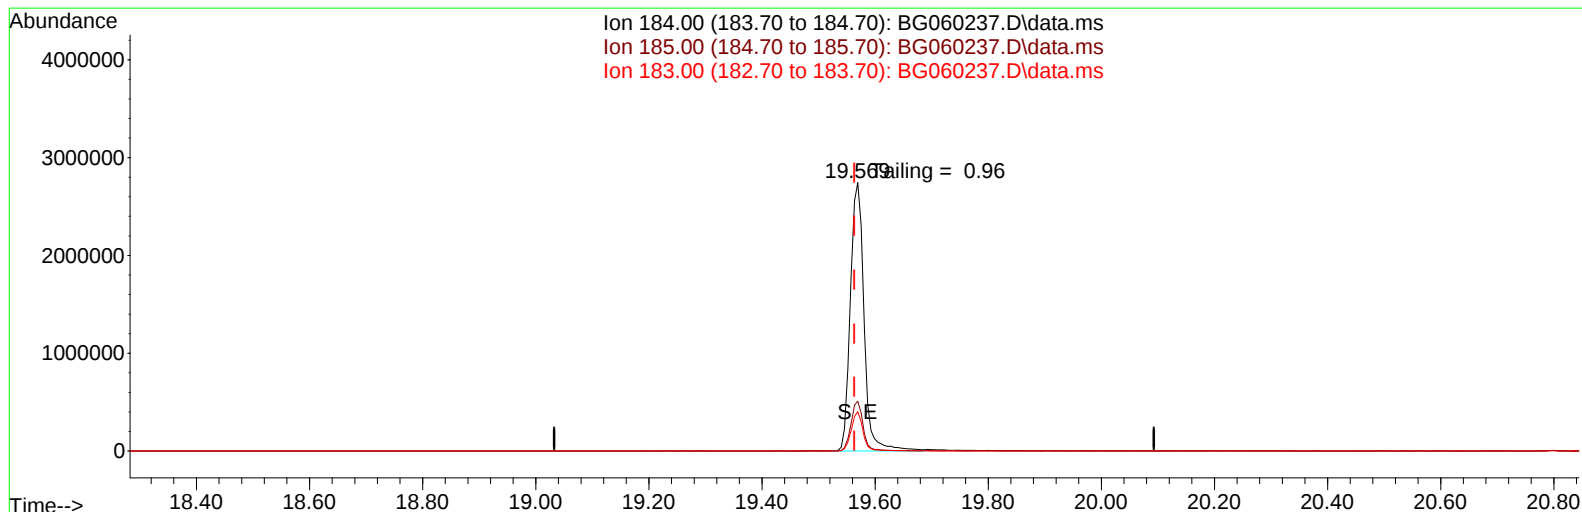

TIC: BG060237.D\data.ms

(77) Benzidine**19.569min (+ 0.006) 623628.53 ng****response 4625662**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	18.59#
183.00	11.80	14.71#
0.00	0.00	0.00