
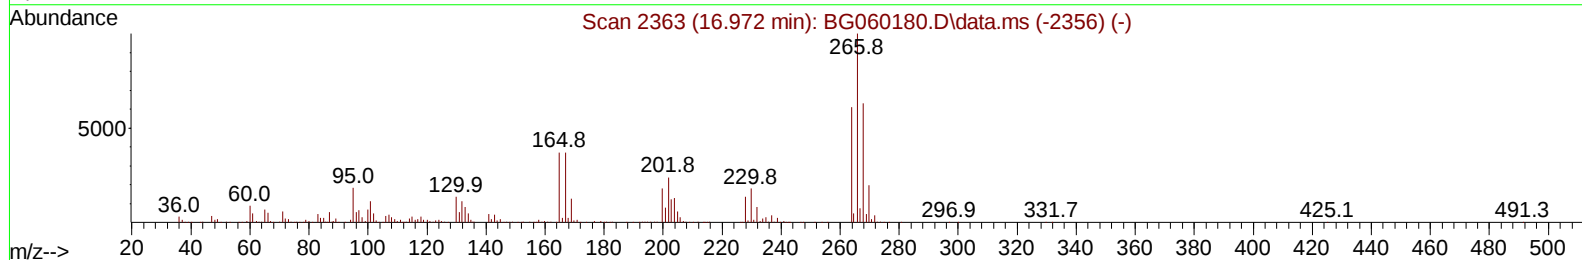
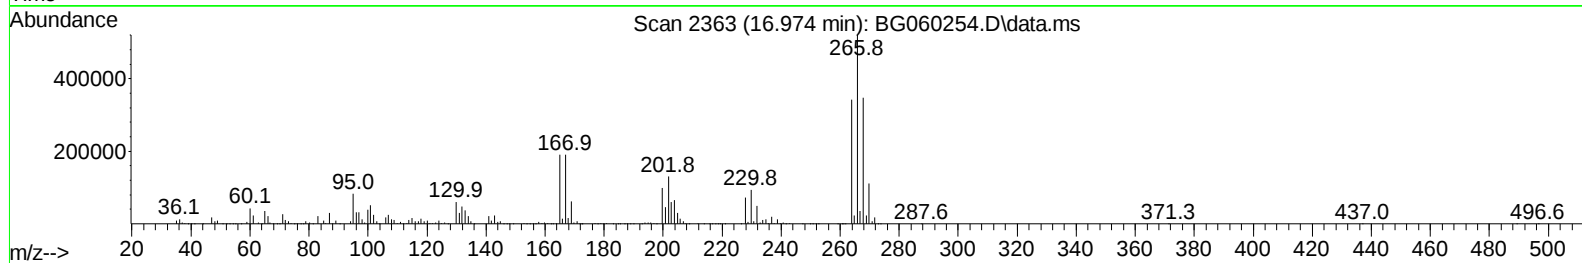


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010424\
Data File : BG060254.D
Acq On : 4 Jan 2024 21:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 02:10:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

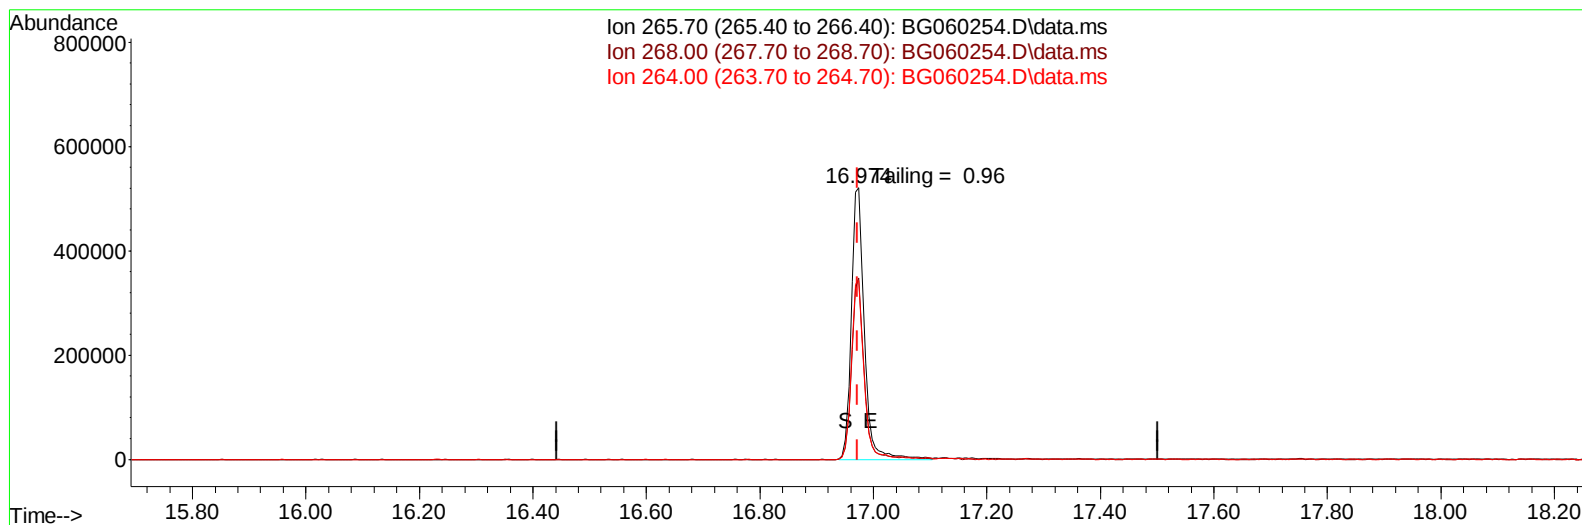




TIC: BG060254.D\data.ms

(70) Pentachlorophenol (C)**16.974min (+ 0.002) 527690.19 ng****response 836007**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	66.81
264.00	65.80	65.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010424\
Data File : BG060254.D
Acq On : 4 Jan 2024 21:43
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 02:10:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

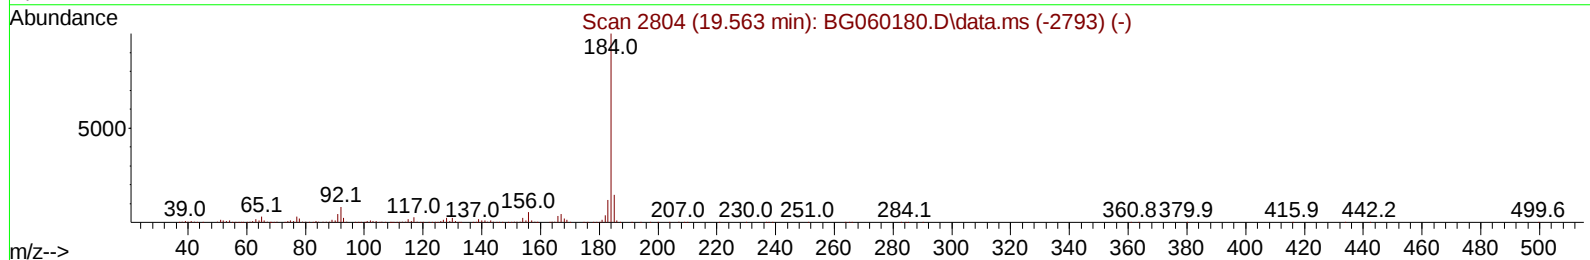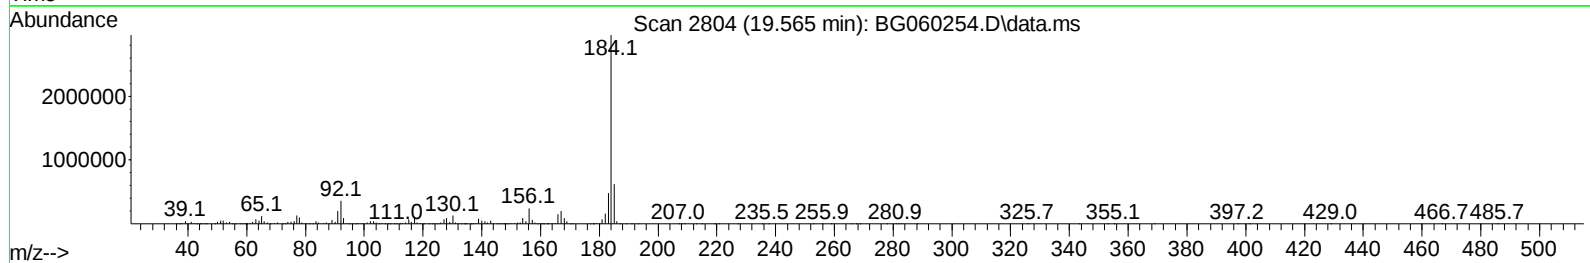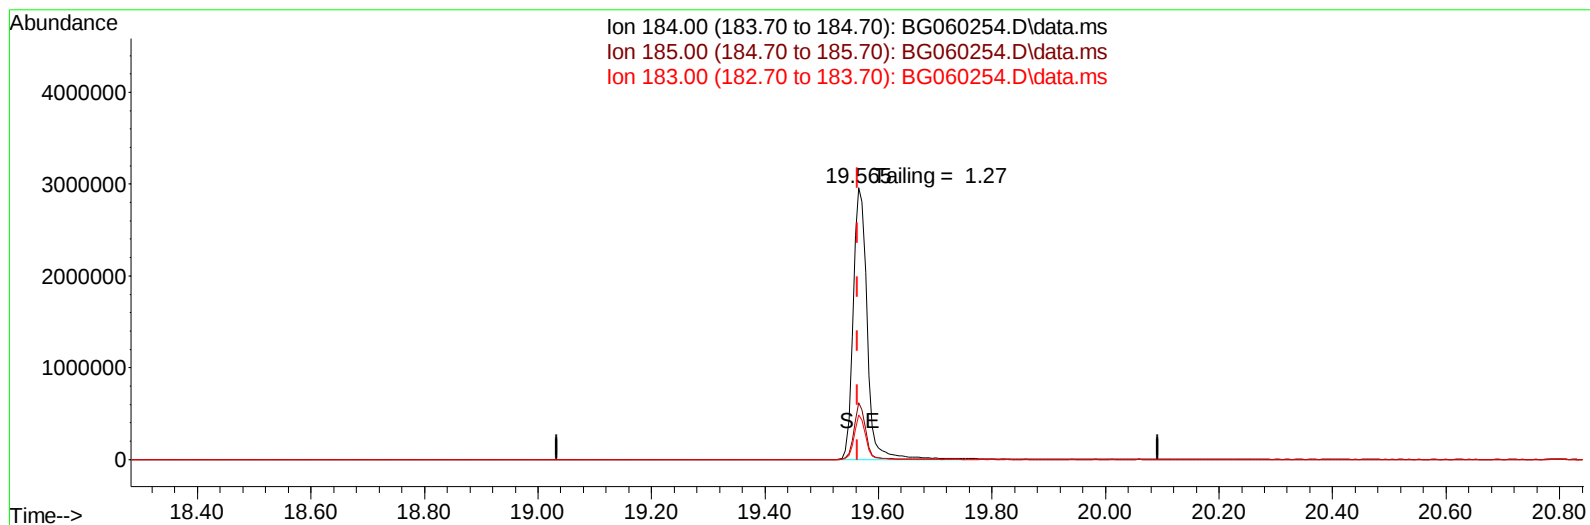

TIC: BG060254.D\data.ms

(77) Benzidine**19.565min (+ 0.002) 61383.74 ng****response 5072900**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	20.87#
183.00	11.80	16.35#
0.00	0.00	0.00