

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010424\  
 Data File : BG060241.D  
 Acq On : 4 Jan 2024 12:16  
 Operator : MA/JU  
 Sample : PB158174BL  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB158174BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060241.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.512       | 405           | 412         | 425          | rBV      | 5008631        | 7861476       | 35.96%          | 8.726%        |
| 2         | 7.104       | 675           | 683         | 695          | rBV      | 5000376        | 8478219       | 38.78%          | 9.411%        |
| 3         | 7.938       | 818           | 825         | 837          | rBV      | 754624         | 1294896       | 5.92%           | 1.437%        |
| 4         | 9.102       | 1013          | 1023        | 1034         | rBV      | 2877441        | 5111512       | 23.38%          | 5.674%        |
| 5         | 10.741      | 1295          | 1302        | 1313         | rBV      | 1055922        | 1908897       | 8.73%           | 2.119%        |
| 6         | 13.197      | 1710          | 1720        | 1736         | rBV      | 7952908        | 12991088      | 59.42%          | 14.420%       |
| 7         | 14.572      | 1947          | 1954        | 1962         | rBV      | 1984823        | 3184274       | 14.56%          | 3.535%        |
| 8         | 16.064      | 2199          | 2208        | 2229         | rBV      | 7087850        | 10741211      | 49.13%          | 11.923%       |
| 9         | 17.321      | 2416          | 2422        | 2436         | rBV      | 2994164        | 4570423       | 20.90%          | 5.073%        |
| 10        | 19.948      | 2862          | 2869        | 2886         | rBV      | 15503142       | 21864304      | 100.00%         | 24.269%       |
| 11        | 21.587      | 3141          | 3148        | 3163         | rBV      | 3026930        | 5103606       | 23.34%          | 5.665%        |
| 12        | 23.855      | 3528          | 3534        | 3540         | rVB3     | 130760         | 275412        | 1.26%           | 0.306%        |
| 13        | 24.772      | 3679          | 3690        | 3705         | rBV      | 1929196        | 5713084       | 26.13%          | 6.342%        |
| 14        | 25.911      | 3874          | 3884        | 3894         | rBV6     | 157960         | 476499        | 2.18%           | 0.529%        |
| 15        | 27.239      | 4101          | 4110        | 4125         | rVB4     | 137852         | 515467        | 2.36%           | 0.572%        |




Sum of corrected areas: 90090368

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010424\  
Data File : BG060241.D  
Acq On : 4 Jan 2024 12:16  
Operator : MA/JU  
Sample : PB158174BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB158174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

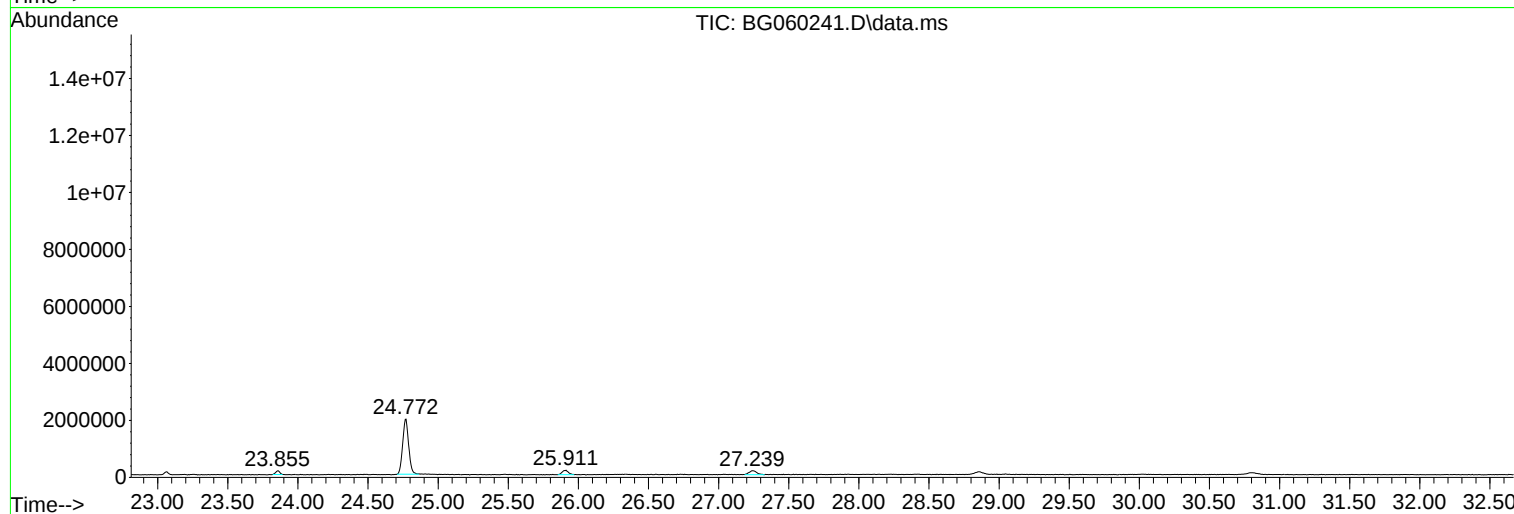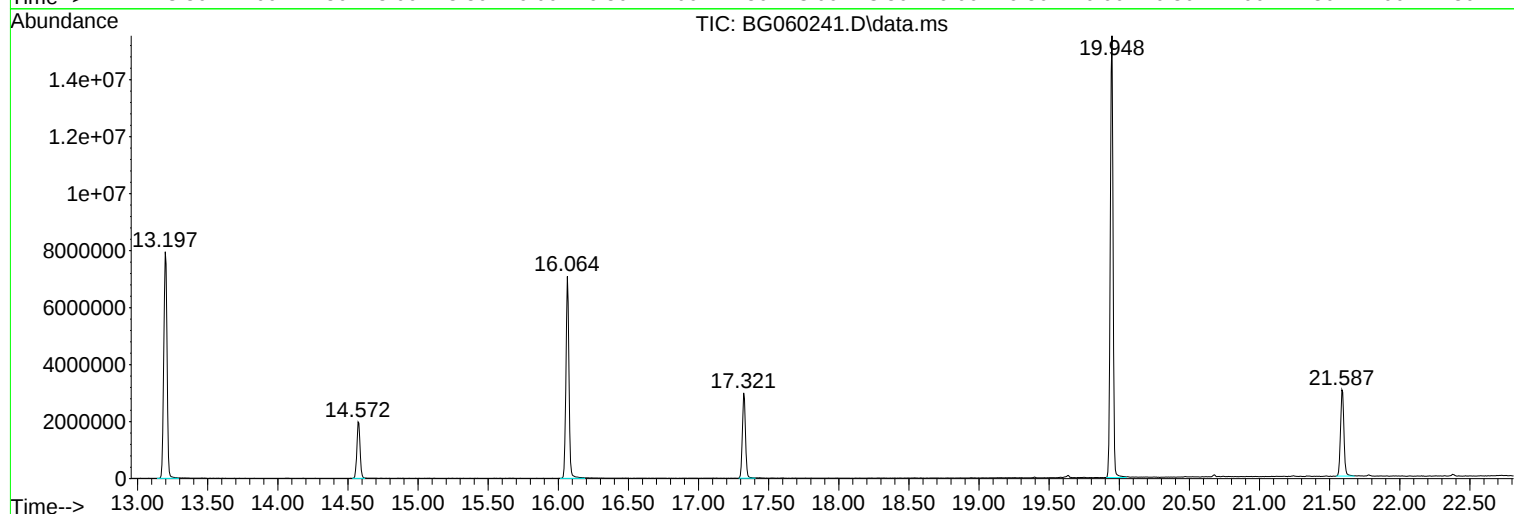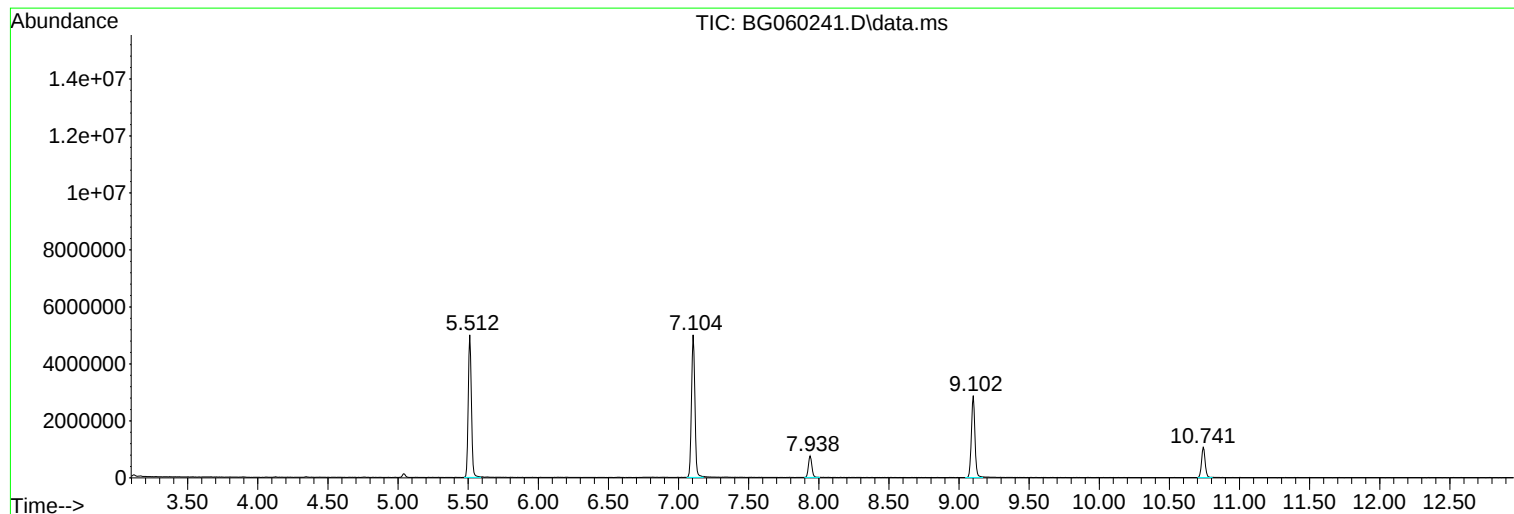

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010424\  
Data File : BG060241.D  
Acq On : 4 Jan 2024 12:16  
Operator : MA/JU  
Sample : PB158174BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB158174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010424\  
Data File : BG060241.D  
Acq On : 4 Jan 2024 12:16  
Operator : MA/JU  
Sample : PB158174BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB158174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|