

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010424\  
Data File : BG060244.D  
Acq On : 4 Jan 2024 14:18  
Operator : MA/JU  
Sample : PB158159BL  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB158159BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060244.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.514       | 406           | 413         | 430          | rBV      | 4876447        | 7800468       | 35.51%          | 8.538%        |
| 2         | 7.106       | 675           | 684         | 698          | rBV      | 4900621        | 8605717       | 39.17%          | 9.420%        |
| 3         | 7.935       | 817           | 825         | 841          | rBV      | 707055         | 1247252       | 5.68%           | 1.365%        |
| 4         | 9.098       | 1015          | 1023        | 1037         | rBV      | 2740352        | 5068793       | 23.07%          | 5.548%        |
| 5         | 10.743      | 1294          | 1303        | 1312         | rBV      | 1057108        | 1931500       | 8.79%           | 2.114%        |
| 6         | 13.199      | 1712          | 1721        | 1733         | rBV      | 8324780        | 13243871      | 60.29%          | 14.496%       |
| 7         | 14.574      | 1948          | 1955        | 1967         | rBV      | 2054017        | 3275844       | 14.91%          | 3.586%        |
| 8         | 16.066      | 2202          | 2209        | 2223         | rBV      | 7085288        | 10889041      | 49.57%          | 11.919%       |
| 9         | 17.324      | 2415          | 2423        | 2437         | rBV      | 2949537        | 4632816       | 21.09%          | 5.071%        |
| 10        | 19.944      | 2863          | 2869        | 2884         | rBV      | 15359887       | 21967713      | 100.00%         | 24.045%       |
| 11        | 21.589      | 3142          | 3149        | 3163         | rBV      | 3200417        | 5193047       | 23.64%          | 5.684%        |
| 12        | 23.851      | 3528          | 3534        | 3545         | rVB4     | 136422         | 313435        | 1.43%           | 0.343%        |
| 13        | 24.768      | 3678          | 3690        | 3705         | rBV      | 1992810        | 5950425       | 27.09%          | 6.513%        |
| 14        | 25.902      | 3875          | 3883        | 3894         | rBV4     | 165171         | 480488        | 2.19%           | 0.526%        |
| 15        | 27.247      | 4101          | 4112        | 4120         | rBV4     | 129650         | 451930        | 2.06%           | 0.495%        |
| 16        | 28.851      | 4377          | 4385        | 4396         | rVB7     | 81960          | 308184        | 1.40%           | 0.337%        |




Sum of corrected areas: 91360524

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010424\  
Data File : BG060244.D  
Acq On : 4 Jan 2024 14:18  
Operator : MA/JU  
Sample : PB158159BL  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB158159BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

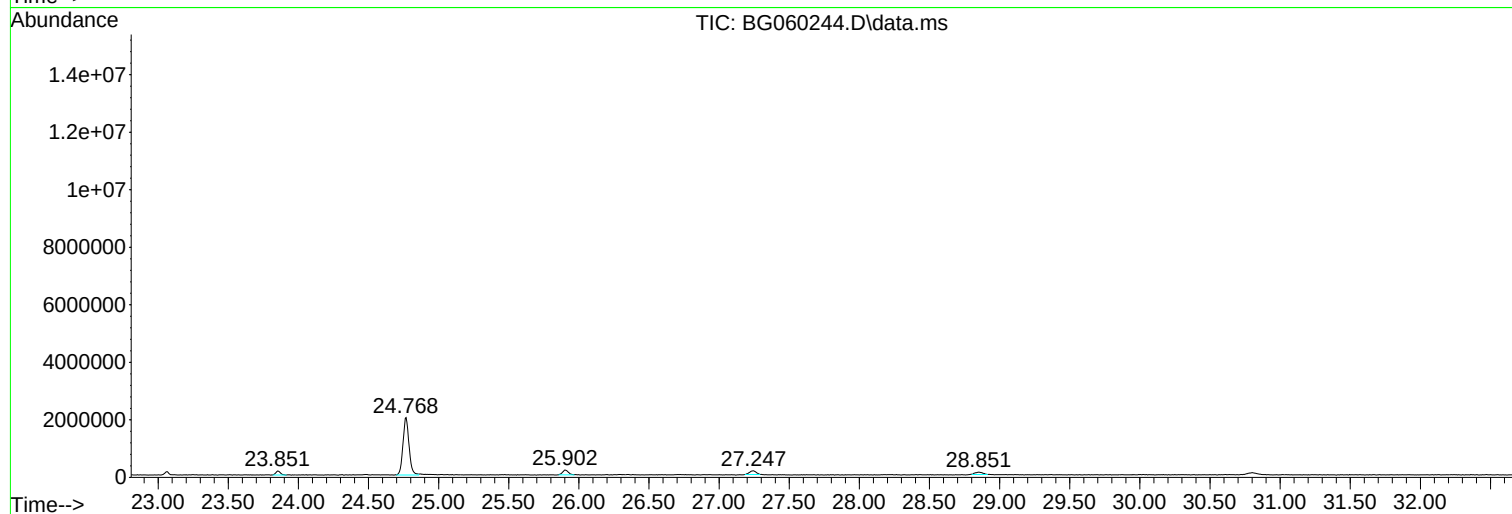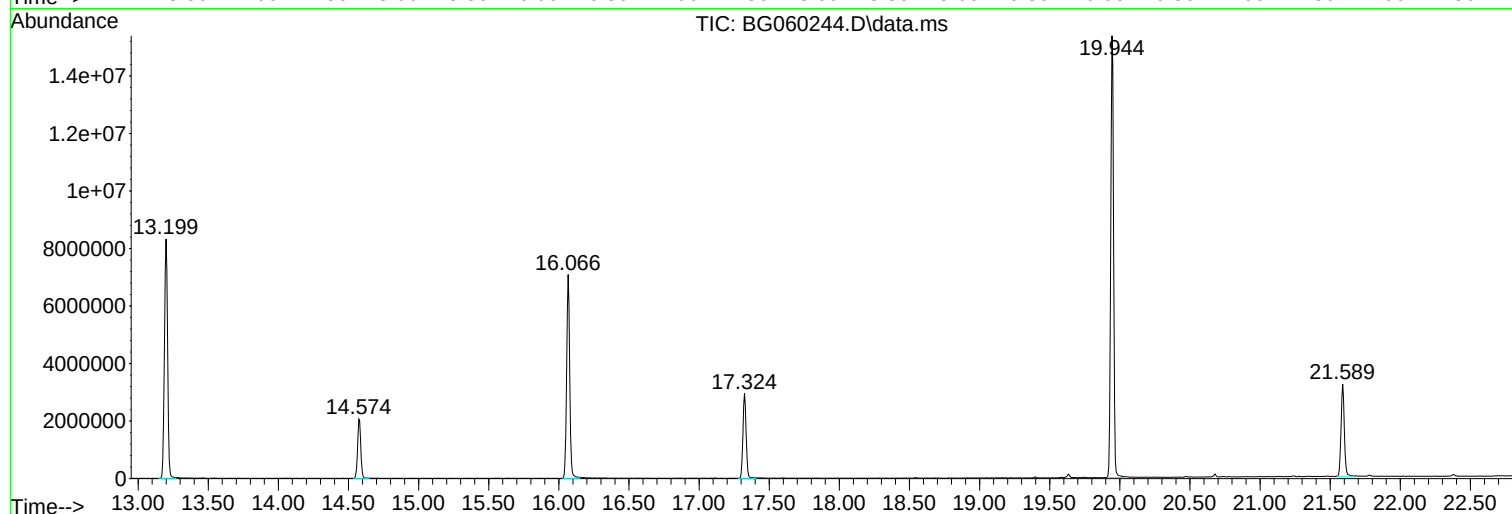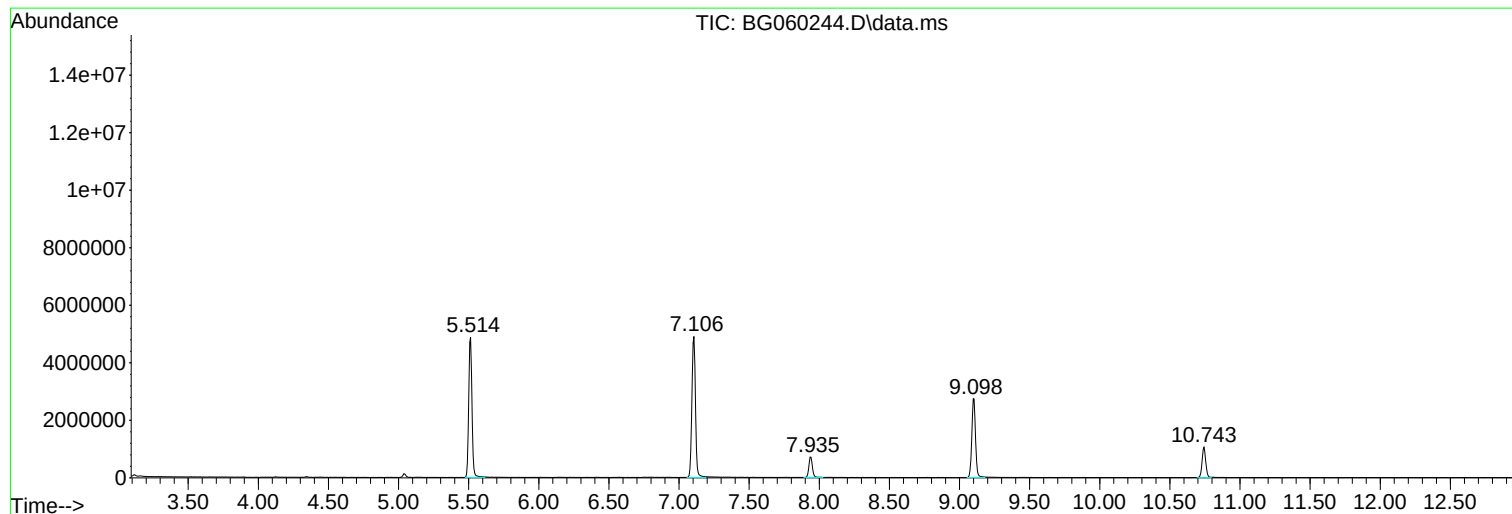

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010424\  
Data File : BG060244.D  
Acq On : 4 Jan 2024 14:18  
Operator : MA/JU  
Sample : PB158159BL  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB158159BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010424\  
Data File : BG060244.D  
Acq On : 4 Jan 2024 14:18  
Operator : MA/JU  
Sample : PB158159BL  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB158159BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|