


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010424\
Data File : BG060237.D
Acq On : 4 Jan 2024 9:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 30 03:14:04 2023

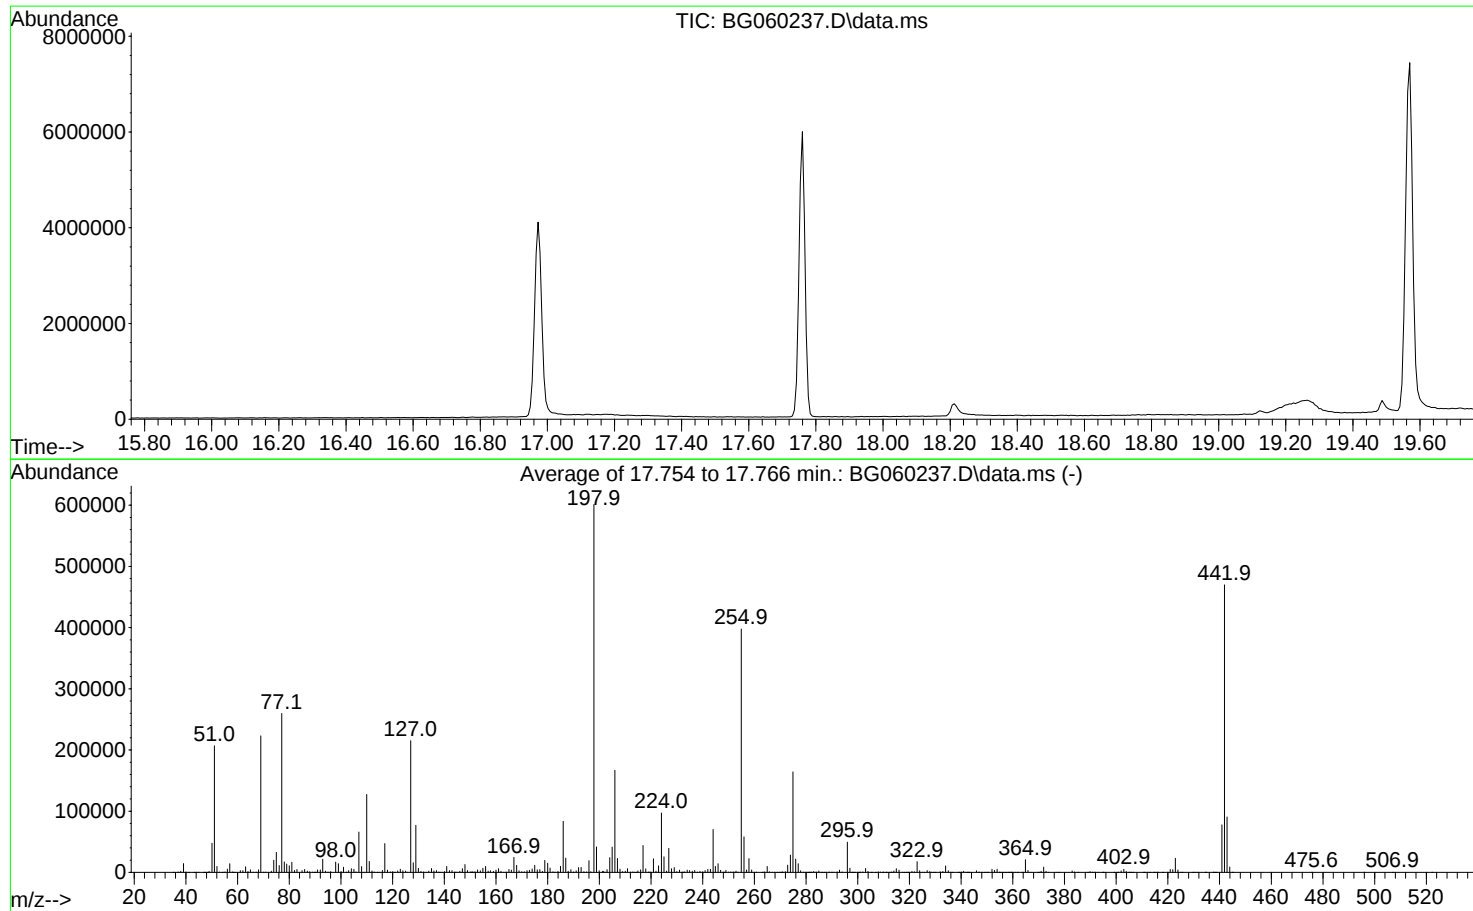

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	206969	PASS
68	69	0.00	2	1.9	4161	PASS
69	198	0.00	100	37.1	223034	PASS
70	69	0.00	2	0.2	386	PASS
127	198	10	80	35.8	215147	PASS
197	198	0.00	2	0.2	1060	PASS
198	198	100	100	100.0	601173	PASS
199	198	5	9	6.9	41560	PASS
275	198	10	60	27.3	164288	PASS
365	198	1	100	3.4	20587	PASS
441	198	0.01	100	12.9	77685	PASS
442	442	50	100	100.0	469845	PASS
443	442	15	24	19.2	90445	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/4/2024	BNA_G	<u>BG060237.D</u>
Compound Name	Response	Retention Time
DDT	1968126	20.797
DDD	99388	20.357
DDE	1795	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
101183	2069309	4.89

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010424\
Data File : BG060237.D
Acq On : 4 Jan 2024 9:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 04 11:19:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

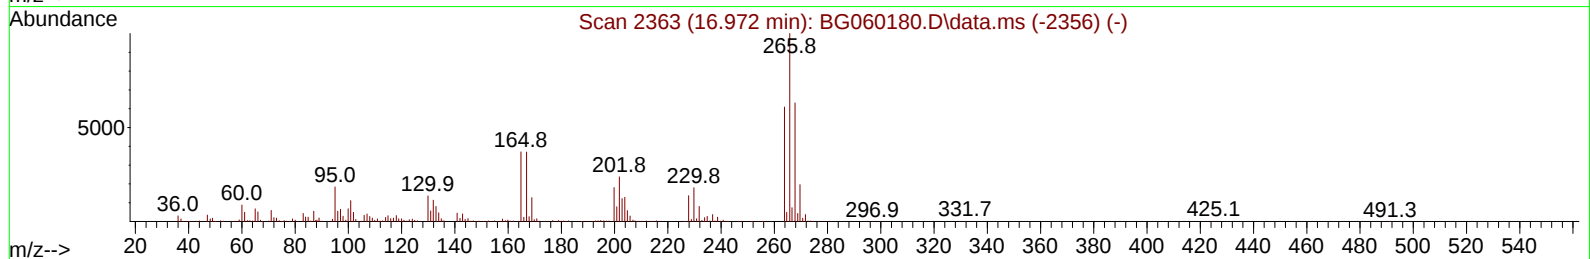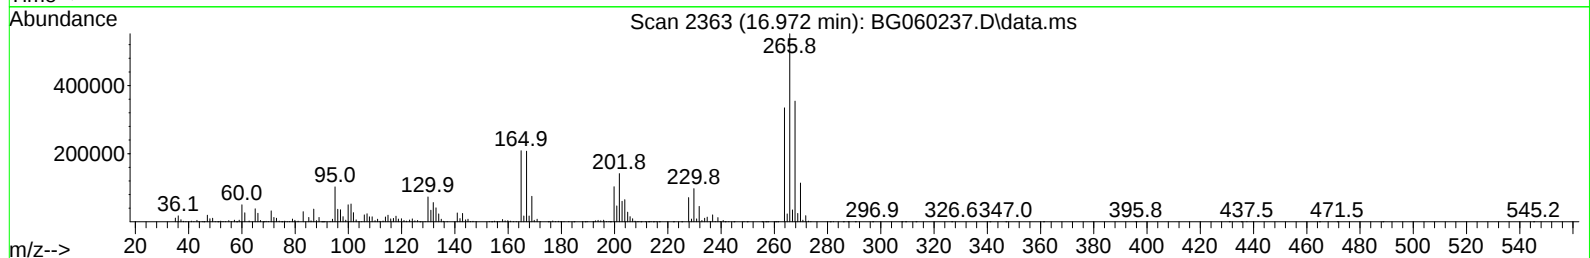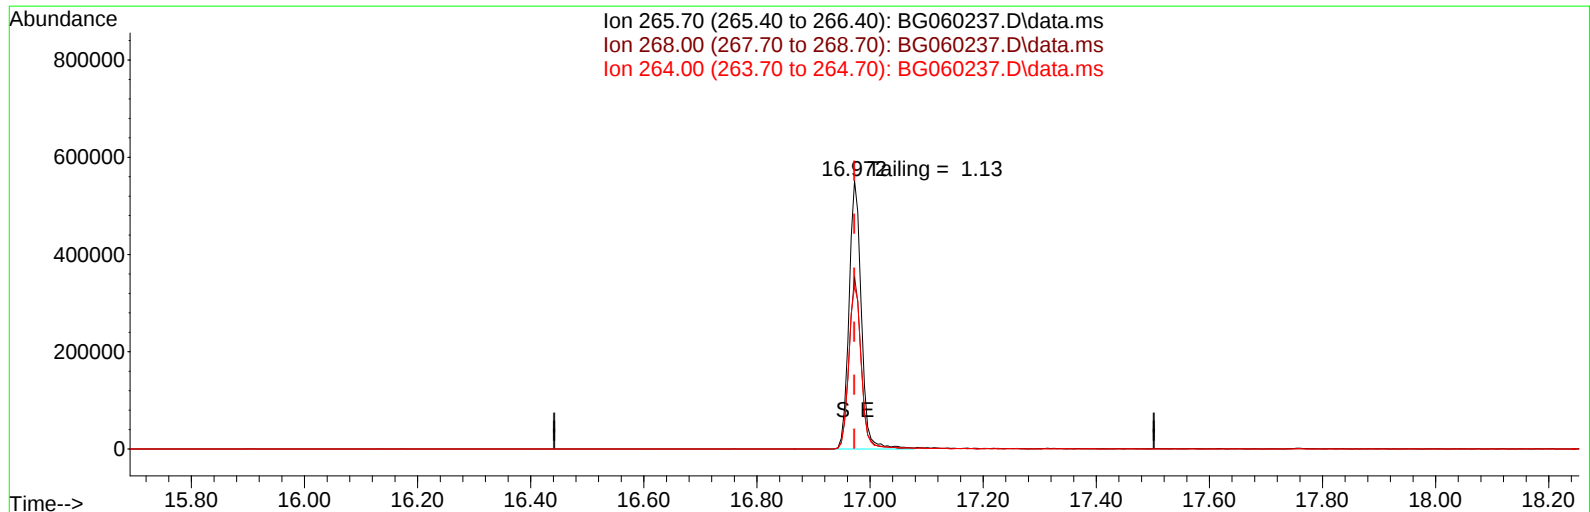

TIC: BG060237.D\data.ms

(70) Pentachlorophenol (C)

16.972min (+ 0.001) 1132366.21 ng




response 835129

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.16
264.00	65.80	60.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010424\
Data File : BG060237.D
Acq On : 4 Jan 2024 9:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 04 11:19:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

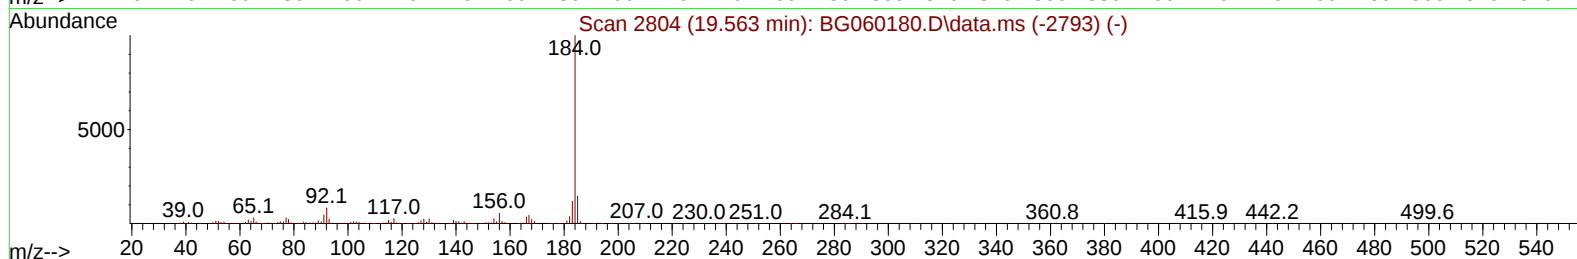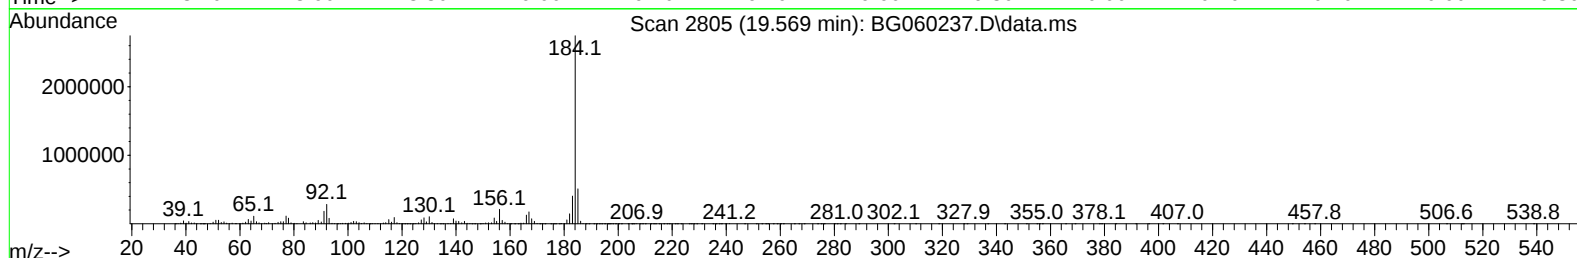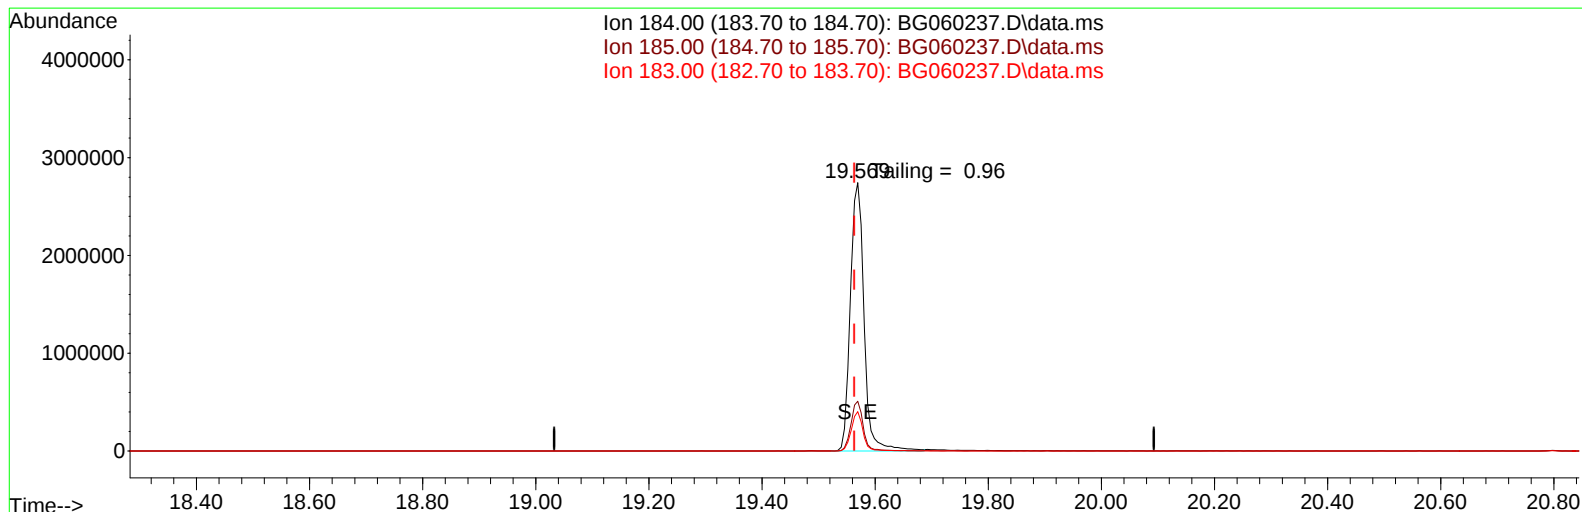

TIC: BG060237.D\data.ms

(77) Benzidine

19.569min (+ 0.006) 623628.53 ng

response 4625662

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	18.59#
183.00	11.80	14.71#
0.00	0.00	0.00