
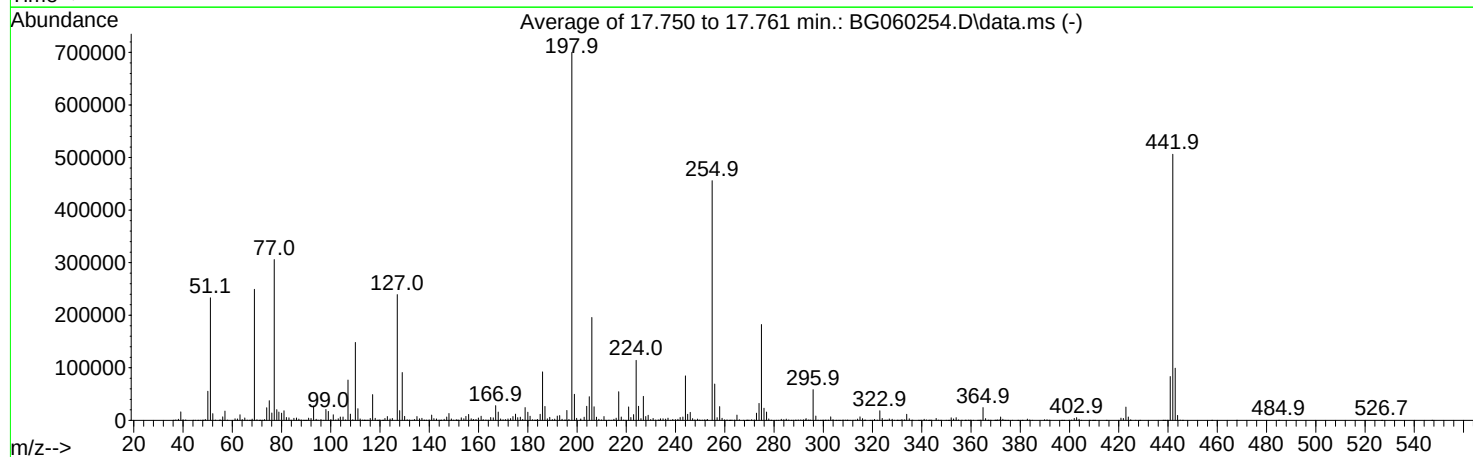


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010424\
Data File : BG060254.D
Acq On : 4 Jan 2024 21:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 30 03:14:04 2023

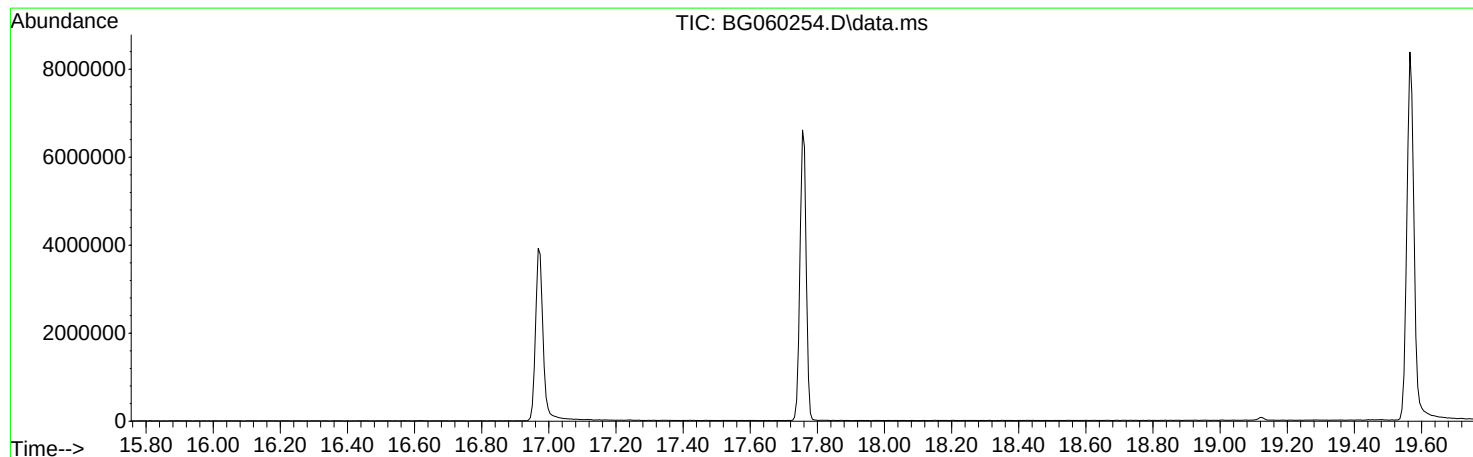

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	233301	PASS
68	69	0.00	2	1.0	2371	PASS
69	198	0.00	100	35.6	249182	PASS
70	69	0.00	2	0.5	1339	PASS
127	198	10	80	34.2	239211	PASS
197	198	0.00	2	0.2	1703	PASS
198	198	100	100	100.0	699819	PASS
199	198	5	9	7.1	49688	PASS
275	198	10	60	26.0	182211	PASS
365	198	1	100	3.5	24412	PASS
441	198	0.01	100	11.9	83264	PASS
442	442	50	100	100.0	506219	PASS
443	442	15	24	19.6	99168	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/4/2024	BNA_G	<u>BG060254.D</u>
Compound Name	Response	Retention Time
DDT	2355465	20.799
DDD	132741	20.353
DDE	7850	19.847
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
140591	2496056	5.63

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010424\
Data File : BG060254.D
Acq On : 4 Jan 2024 21:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 05 02:10:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

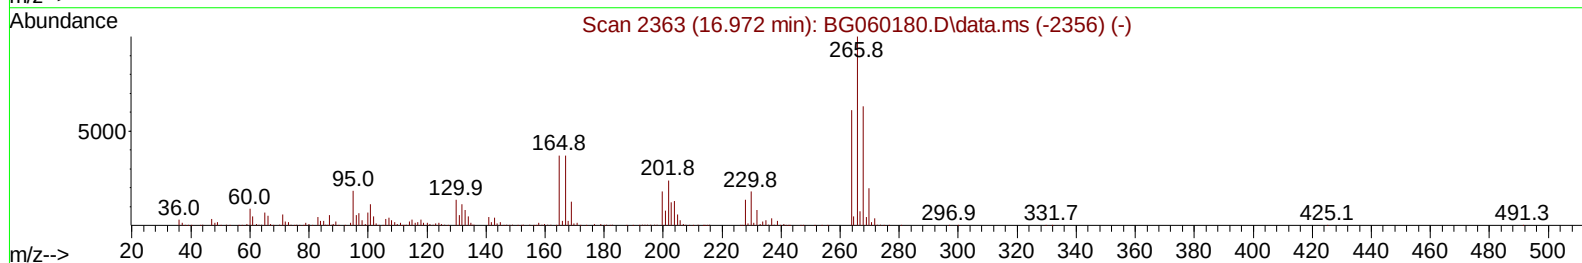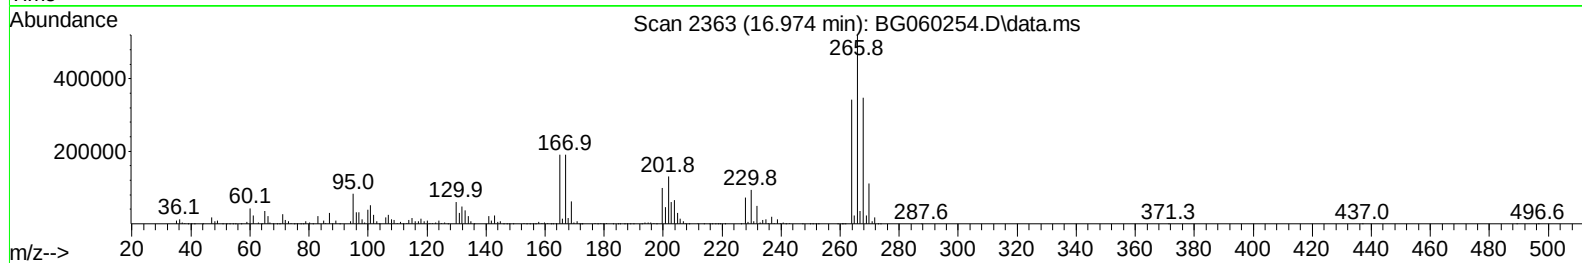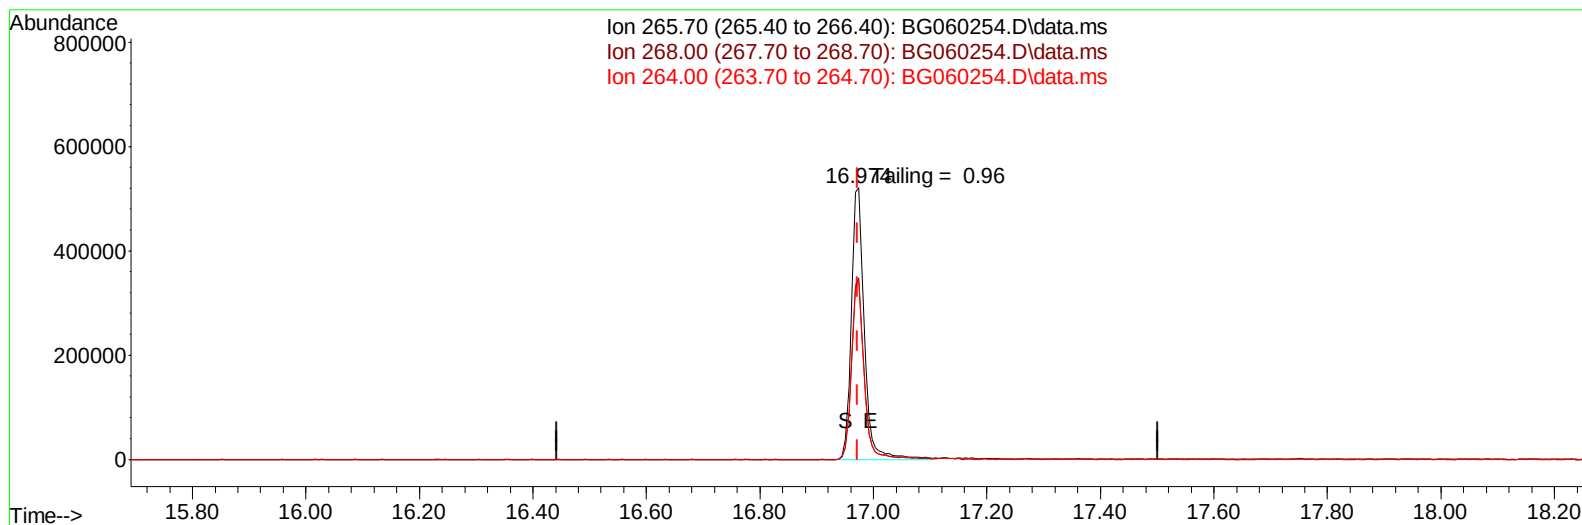

TIC: BG060254.D\data.ms

(70) Pentachlorophenol (C)

16.974min (+ 0.002) 527690.19 ng




response 836007

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	66.81
264.00	65.80	65.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010424\
Data File : BG060254.D
Acq On : 4 Jan 2024 21:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 05 02:10:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

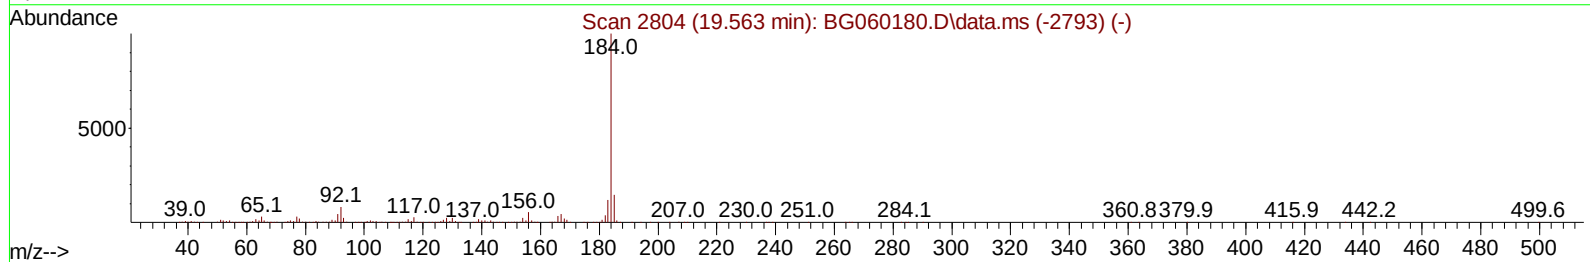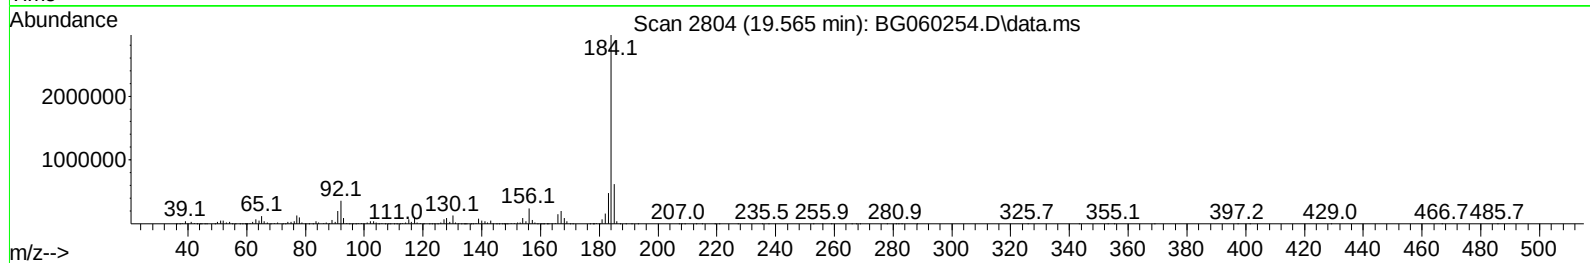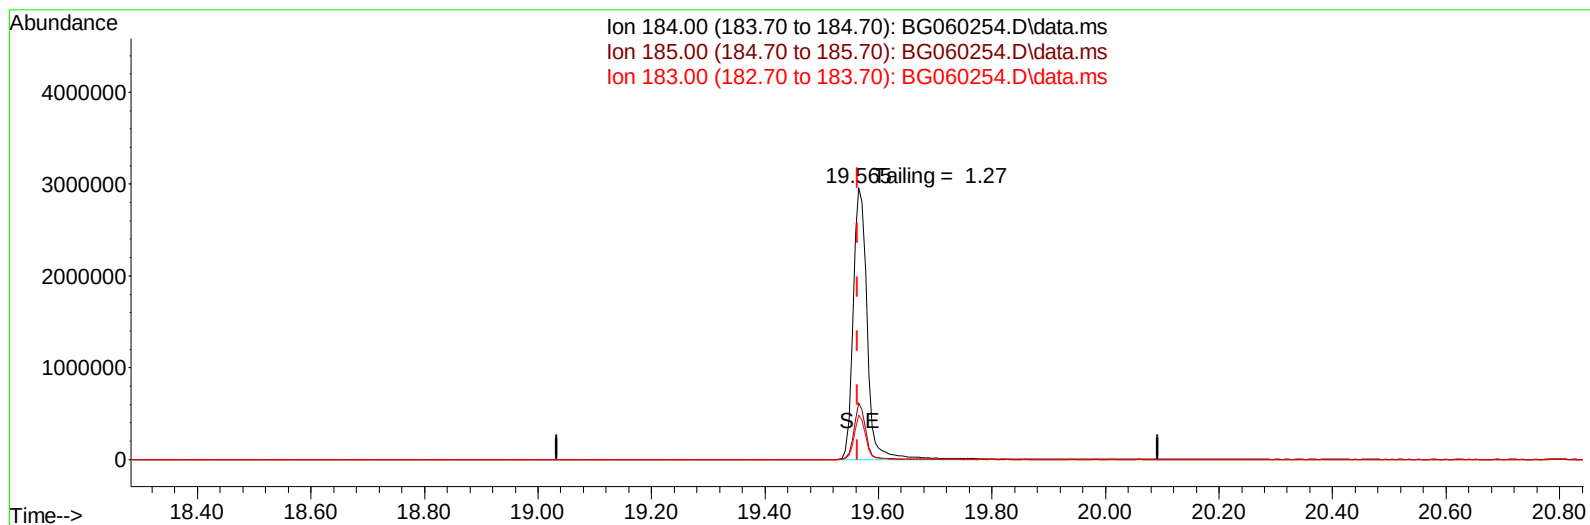

TIC: BG060254.D\data.ms

(77) Benzidine

19.565min (+ 0.002) 61383.74 ng

response 5072900

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	20.87#
183.00	11.80	16.35#
0.00	0.00	0.00