


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG010515\
 Data File : BG015837.D
 Acq On : 5 Jan 2015 9:17
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG010515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 06 03:51:36 2015

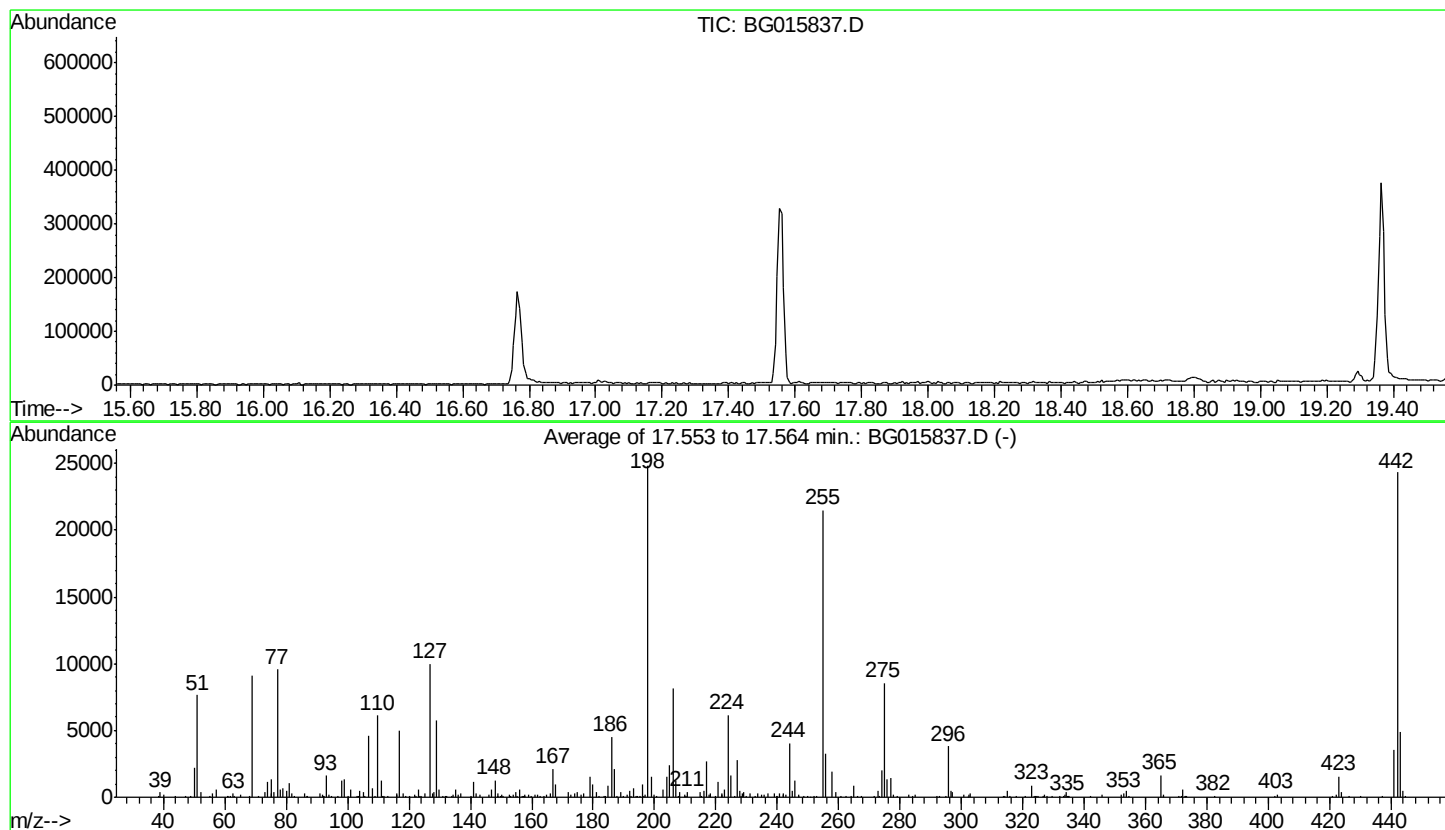

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	7644	PASS
68	69	0.00	2	1.4	129	PASS
69	198	0.00	100	36.7	9107	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.3	10019	PASS
197	198	0.00	2	0.6	153	PASS
198	198	100	100	100.0	24834	PASS
199	198	5	9	6.3	1569	PASS
275	198	10	60	34.4	8537	PASS
365	198	1	100	6.7	1666	PASS
441	442	0.01	24	14.6	3556	PASS
442	198	50	100	98.2	24378	PASS
443	442	15	24	20.0	4886	PASS