

Data Path : Z:\HPCHEM1\BNA_G\Data\BG010516\
 Data File : BG020668.D
 Acq On : 6 Jan 2016 8:41
 Operator : UM/SJ
 Sample : H1004-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Quant Time: Jan 06 11:05:45 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG123015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 06 04:25:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	14187	20.00	ng/ul	0.00
18) Naphthalene-d8	10.87	136	63514	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.69	164	47334	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.44	188	129980	20.00	ng/ul	0.00
78) Chrysene-d12	21.71	240	157749	20.00	ng/ul	0.00
86) Perylene-d12	24.96	264	145617	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	0.00	176	0	0.00	ng/ul	
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	17.44	188	129980	21.46	ng/ul	-0.10
79) Pyrene-d10	0.00	212	0	0.00	ng/ul	
90) Benzo(a)pyrene-d12	0.00	264	0	0.00	ng/ul	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
76) Di-n-butylphthalate	18.38	149	18362	2.57	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\Data\BG010516\
Data File : BG020668.D
Acq On : 6 Jan 2016 8:41
Operator : UM/SJ
Sample : H1004-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Time: Jan 06 11:05:45 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG123015.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 06 04:25:43 2016
Response via : Initial Calibration

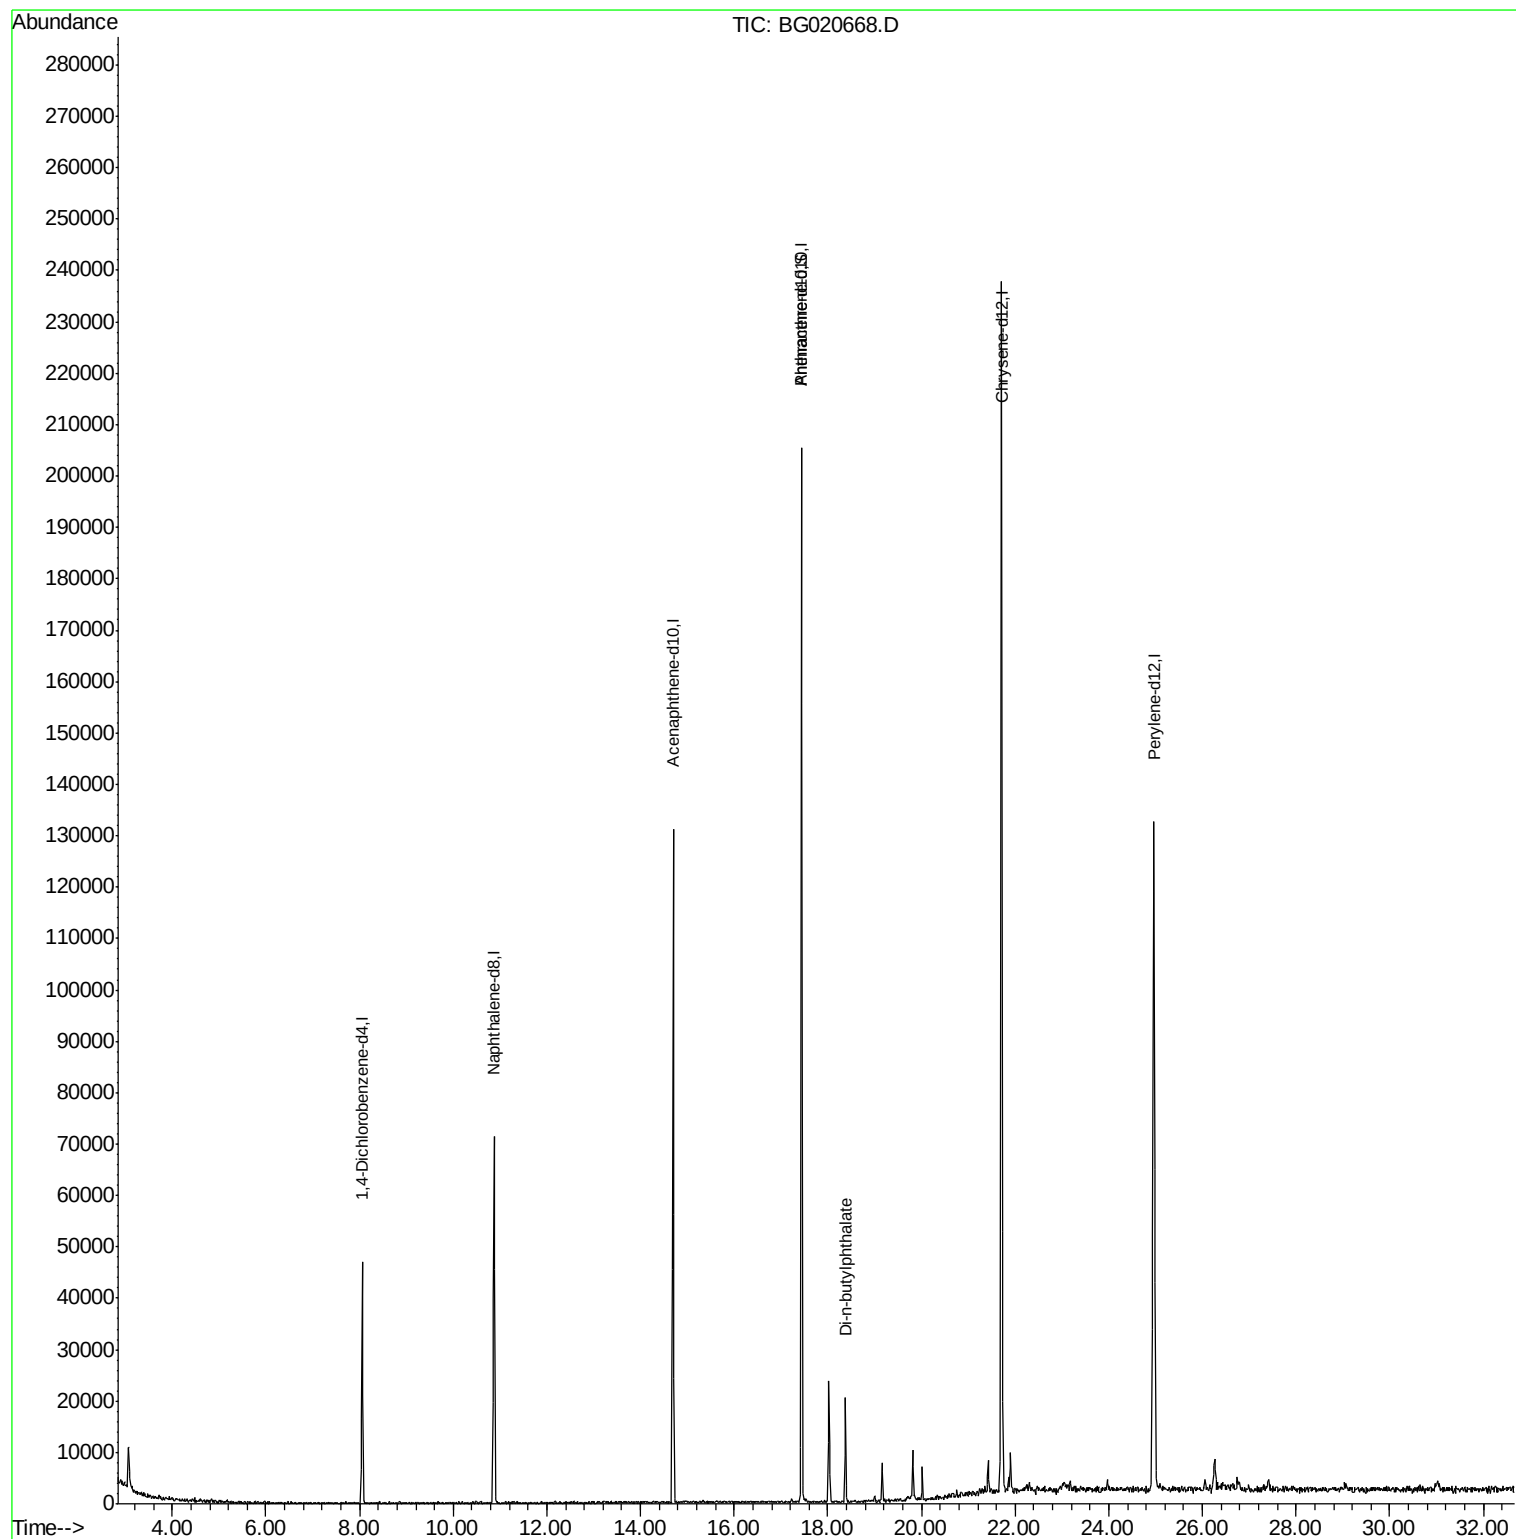

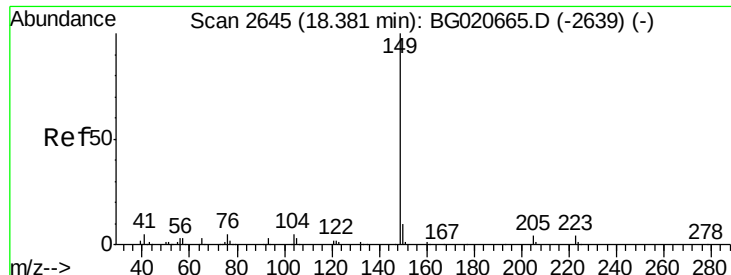

#76
 Di-n-butylphthalate
 Concen: 2.57 ng/ul
 RT: 18.38 min Scan# 2645
 Delta R.T. -0.00 min
 Lab File: BG020668.D
 Acq: 6 Jan 2016 8:41

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Tgt Ion:149 Resp: 18362
 Ion Ratio Lower Upper
 149 100
 150 8.4 7.5 11.3
 104 6.0 4.1 6.1

