

Data Path : Z:\HPCHEM1\BNA G\DATA\BG010516\
 Data File : BG020655.D
 Acq On : 5 Jan 2016 14:21
 Operator : UM/SJ
 Sample : G4846-12
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N58

Quant Time: Jan 06 01:04:20 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG123015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 06 00:15:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	15854	20.00	ng/ul	0.00
18) Naphthalene-d8	10.87	136	70207	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.69	164	51305	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	137998	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	162778	20.00	ng/ul	0.00
86) Perylene-d12	24.95	264	155403	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	395	1.49	ng/uL	0.00
5) Phenol-d5	7.21	99	10281	7.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.37	67	25958	32.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	28573	27.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.76	113	20689	18.01	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	18392	33.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.95	143	22562	35.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.49	165	38205	31.95	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	14.09	166	156580	37.29	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	169458	35.53	ng/ul	0.00
52) 4-Nitrophenol-d4	14.90	143	4383	6.66	ng/ul	0.00
58) Fluorene-d10	15.68	176	135685	35.65	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.81	200	21030	25.13	ng/ul	0.00
71) Anthracene-d10	17.53	188	231137	35.95	ng/ul	0.00
79) Pyrene-d10	19.82	212	264164	36.19	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.73	264	283235	36.53	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
28) Naphthalene	10.93	128	1590515	427.79	ng/ul#	94
34) 2-Methylnaphthalene	12.52	142	177054	63.64	ng/ul	98
41) 1,1'-Biphenyl	13.52	154	44435	11.51	ng/ul	97
48) Acenaphthylene	14.41	152	29363	5.78	ng/ul	99
50) Acenaphthene	14.75	153	163011	47.42	ng/ul	97
54) Dibenzofuran	15.09	168	126207	24.30	ng/ul	97
59) Fluorene	15.73	166	112369	26.89	ng/ul	96
70) Phenanthrene	17.48	178	302876	40.37	ng/ul	98
72) Anthracene	17.57	178	23935	3.12	ng/ul	97
75) Carbazole	17.84	167	21624	3.34	ng/ul	97
76) Di-n-butylphthalate	18.38	149	10704	1.41	ng/ul	98
77) Fluoranthene	19.48	202	55549	6.06	ng/ul	99
80) Pyrene	19.85	202	35290	3.74	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG010516\
Data File : BG020655.D
Acq On : 5 Jan 2016 14:21
Operator : UM/SJ
Sample : G4846-12
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9N58

Quant Time: Jan 06 01:04:20 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG123015.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 06 00:15:22 2016
Response via : Initial Calibration




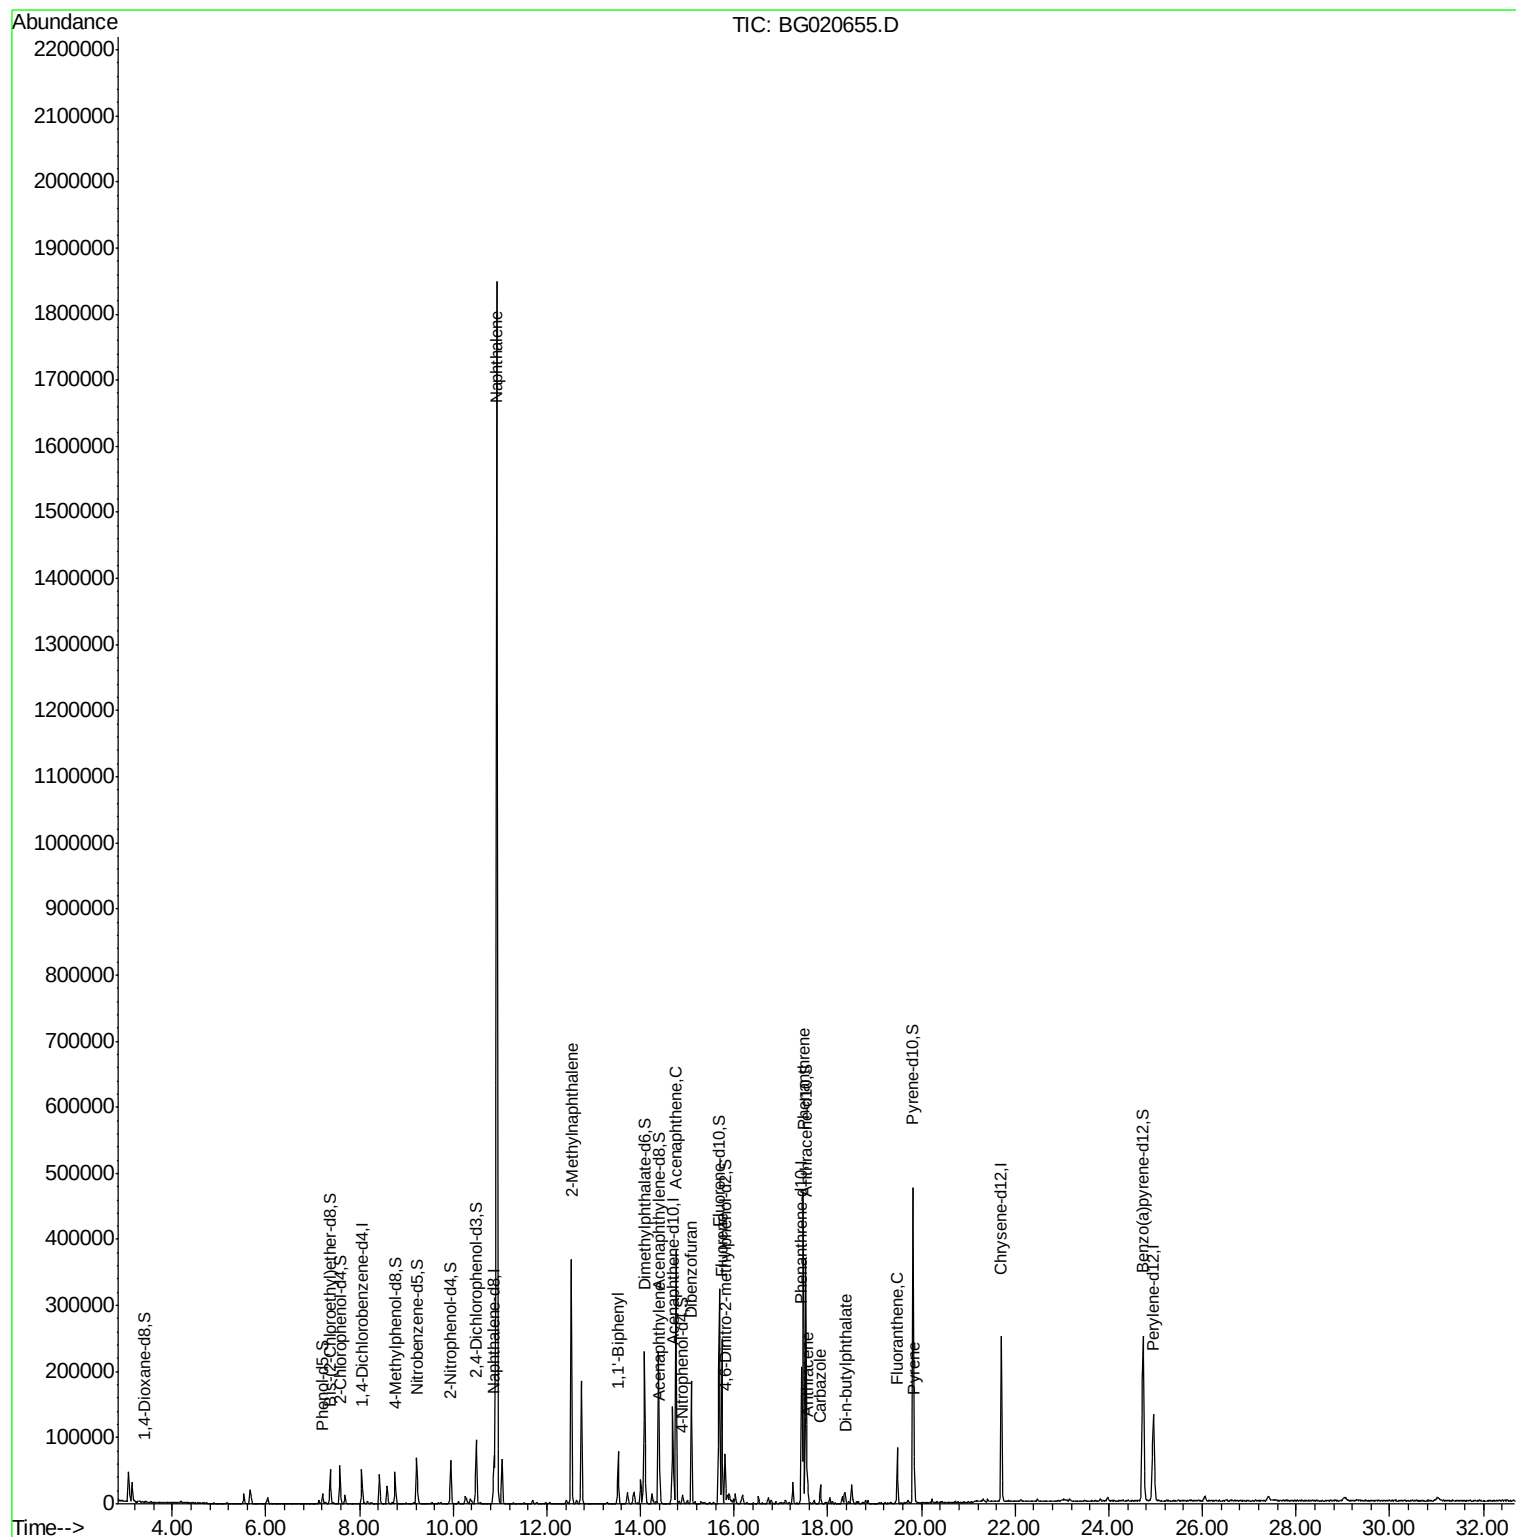


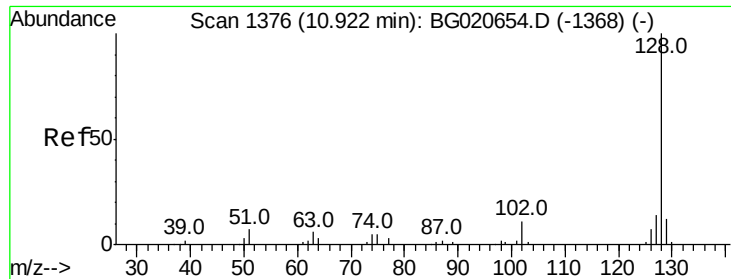

#28
Naphthalene
Concen: 427.79 ng/ul
RT: 10.93 min Scan# 1378
Delta R.T. 0.01 min
Lab File: BG020655.D
Acq: 5 Jan 2016 14:21




Instrument :
BNA_G
ClientSampleId :
D9N58


Tot Ion:128 Resp: 1590515
Ion Ratio Lower Upper
128 100
129 12.9 8.3 12.5#
127 16.0 10.8 16.2

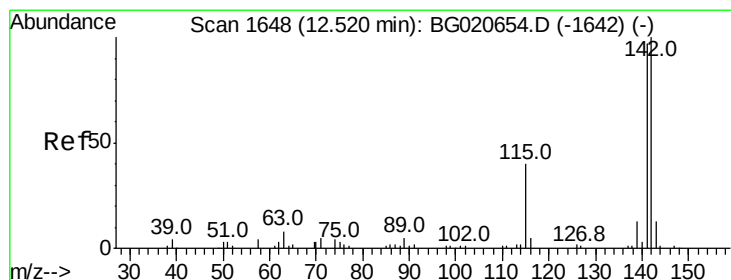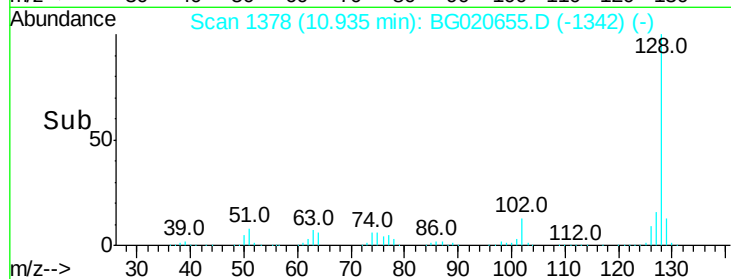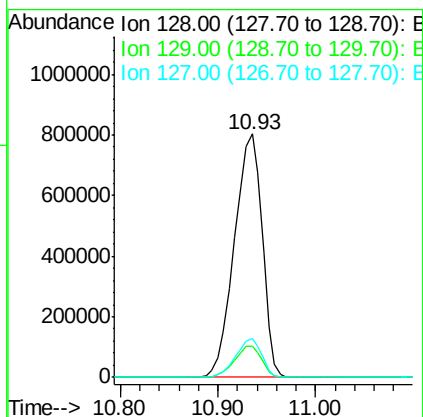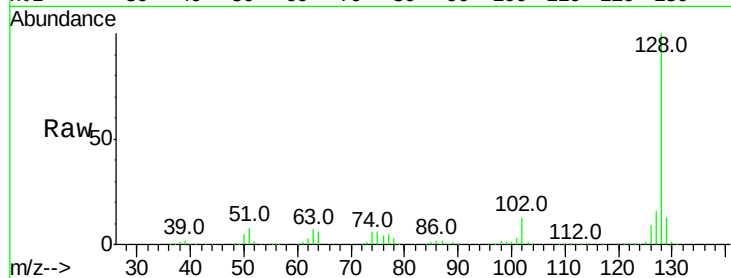

#34
2-Methylnaphthalene
Concen: 63.64 ng/ul
RT: 12.52 min Scan# 1648
Delta R.T. 0.00 min
Lab File: BG020655.D
Acq: 5 Jan 2016 14:21

Tgt Ion:142 Resp: 177054
Ion Ratio Lower Upper
142 100
141 91.3 71.4 107.2

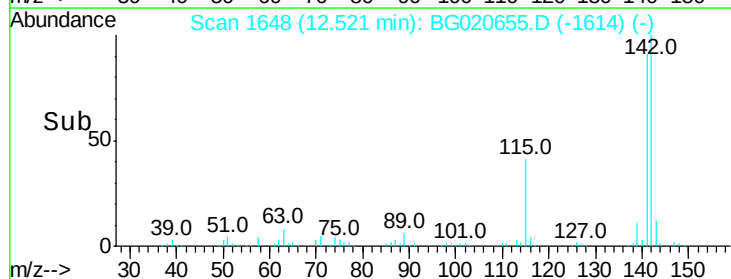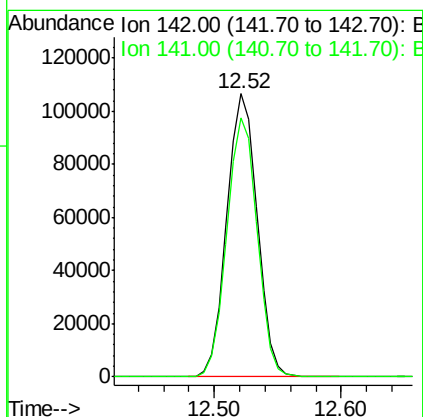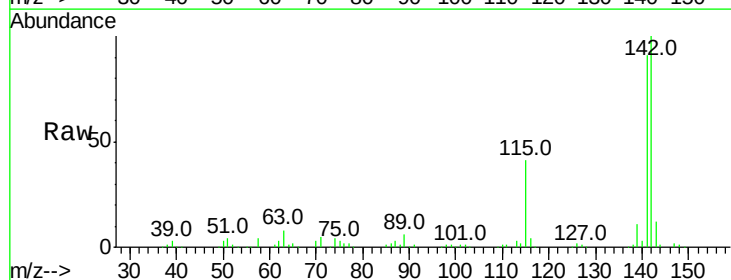


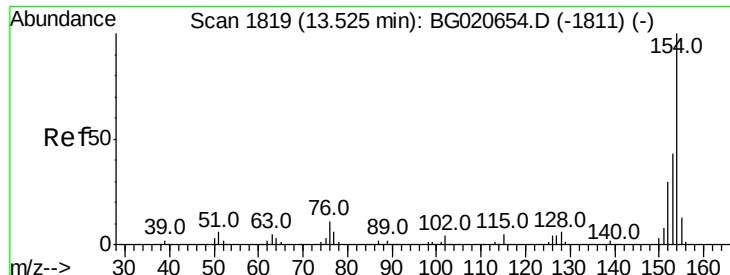


#41
 1,1'-Biphenyl
 Concen: 11.51 ng/ul
 RT: 13.52 min Scan# 1818
 Delta R.T. -0.01 min
 Lab File: BG020655.D
 Acq: 5 Jan 2016 14:21

Instrument :
 BNA_G
 ClientSampleId :
 D9N58



Tot Ion	Ratio	Lower	Upper
154	100		
153	41.0	34.0	51.0
76	12.6	8.4	12.6

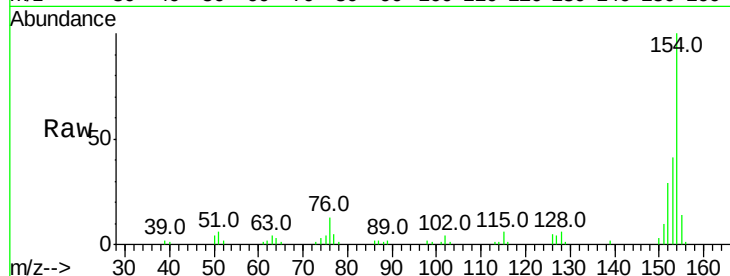

Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BGC

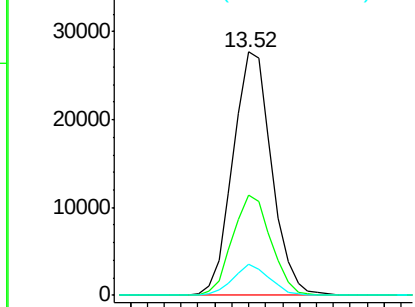


Time--> 13.45 13.50 13.55 13.60

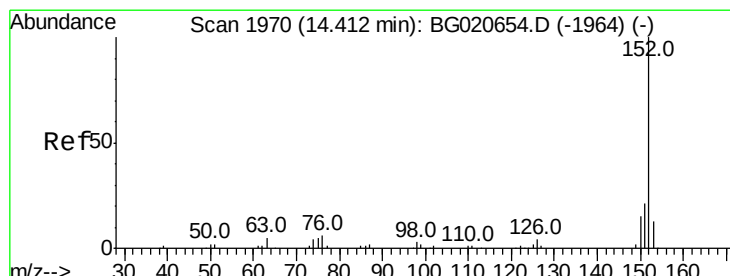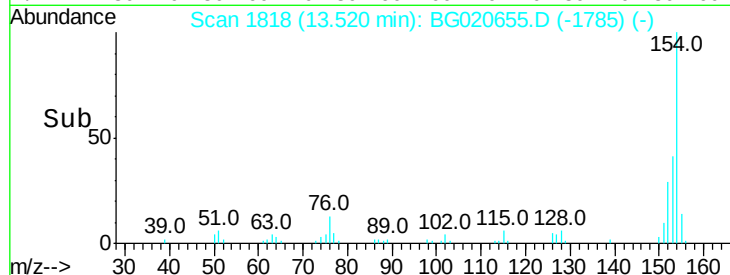


#48
 Acenaphthylene
 Concen: 5.78 ng/ul
 RT: 14.41 min Scan# 1970
 Delta R.T. 0.00 min
 Lab File: BG020655.D
 Acq: 5 Jan 2016 14:21


Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.8	16.1	24.1
153	13.1	10.8	16.2

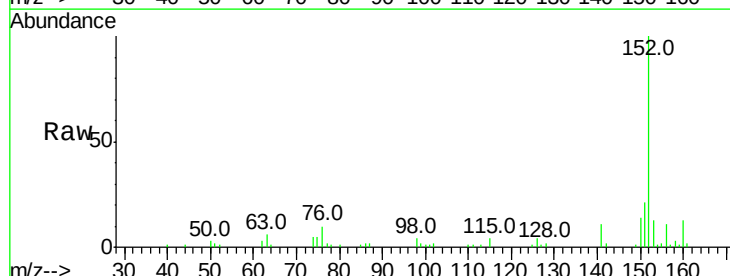


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 151.00 (150.70 to 151.70): E
 Ion 153.00 (152.70 to 153.70): E

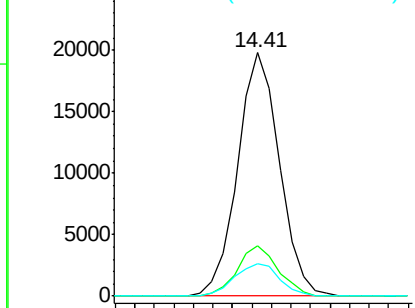

Time--> 14.35 14.40 14.45

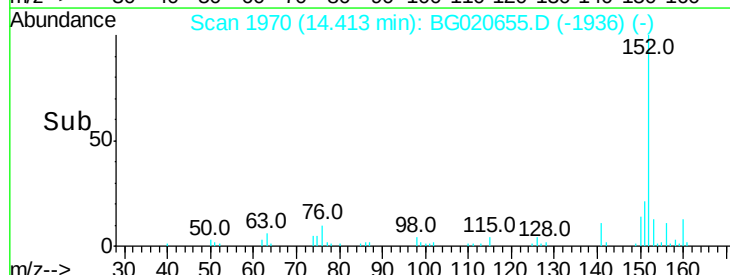

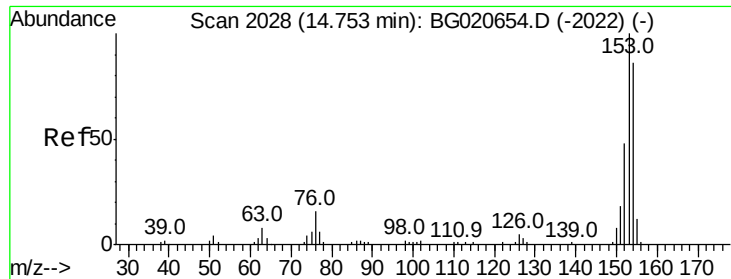

#50

Acenaphthene

Concen: 47.42 ng/ul

RT: 14.75 min Scan# 2028

Delta R.T. 0.00 min

Lab File: BG020655.D

Acq: 5 Jan 2016 14:21

Instrument :

BNA_G

ClientSampleId :

D9N58


Tot Ion:153 Resp: 163011

Ion Ratio Lower Upper

153 100

152 45.7 37.9 56.9




154 84.6 69.8 104.6

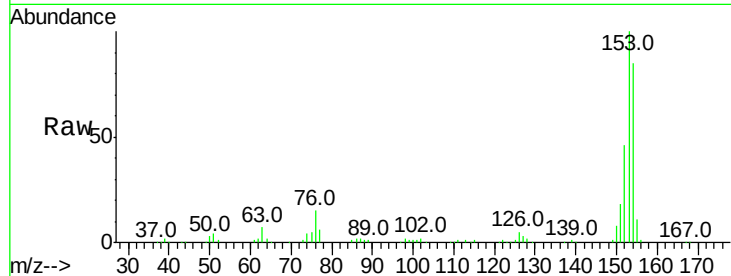

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

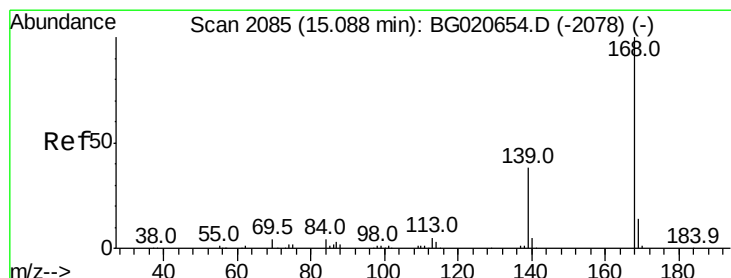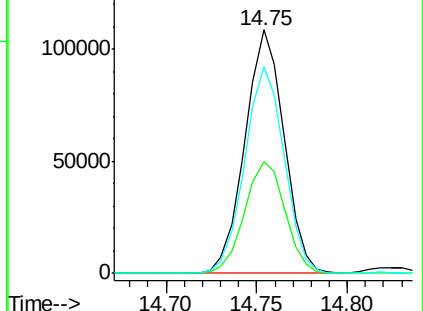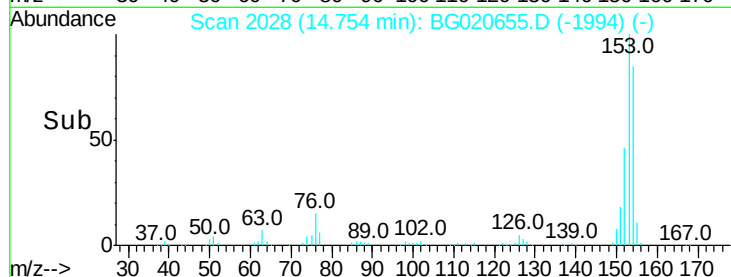

#54

Dibenzofuran

Concen: 24.30 ng/ul

RT: 15.09 min Scan# 2085

Delta R.T. 0.00 min

Lab File: BG020655.D


Acq: 5 Jan 2016 14:21

Tgt Ion:168 Resp: 126207

Ion Ratio Lower Upper



168 100


139 36.7 31.0 46.4

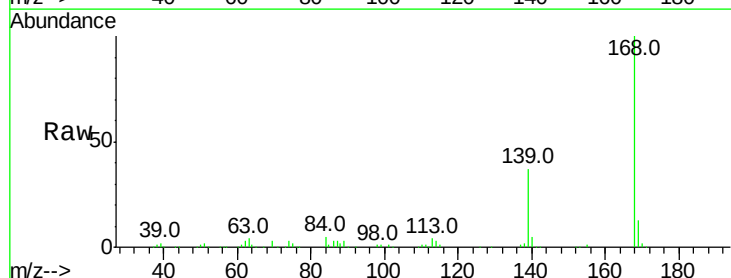

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

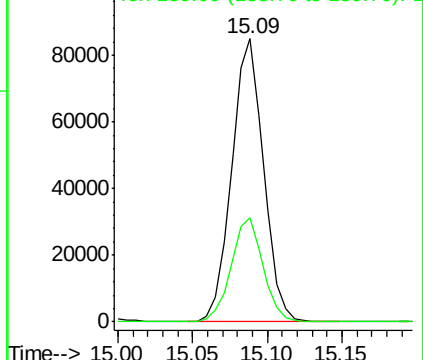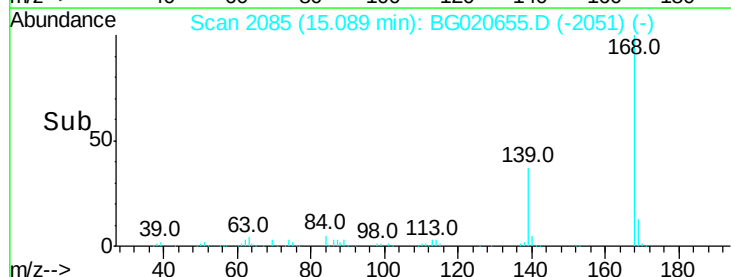

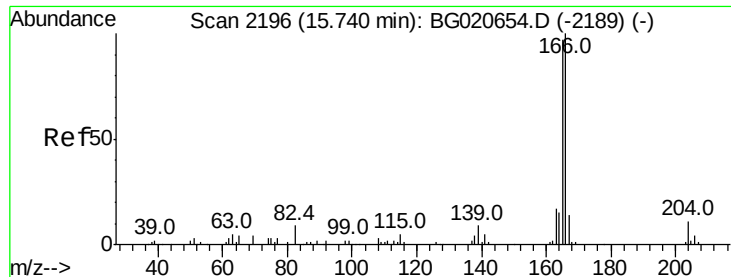

#59

Fluorene

Concen: 26.89 ng/ul

RT: 15.73 min Scan# 2195

Delta R.T. -0.01 min

Lab File: BG020655.D

Acq: 5 Jan 2016 14:21

Instrument :

BNA_G

ClientSampled :

D9N58


Tot Ion:166 Resp: 112369

Ion Ratio Lower Upper

166 100

165 101.9 78.4 117.6




167 14.6 11.1 16.7

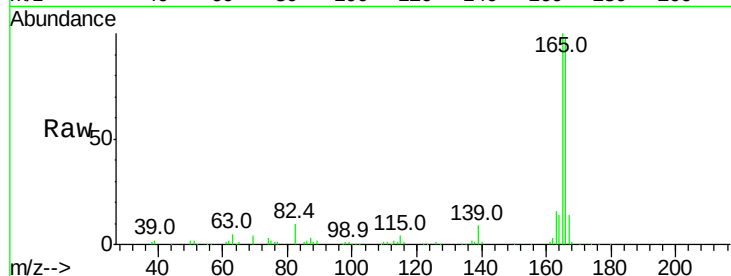

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

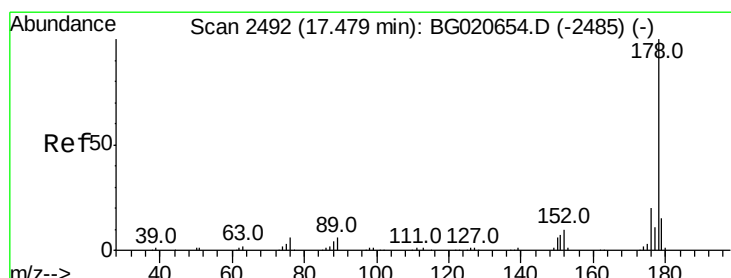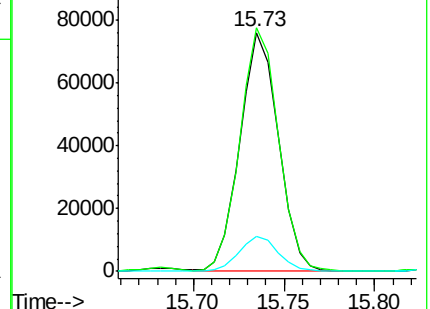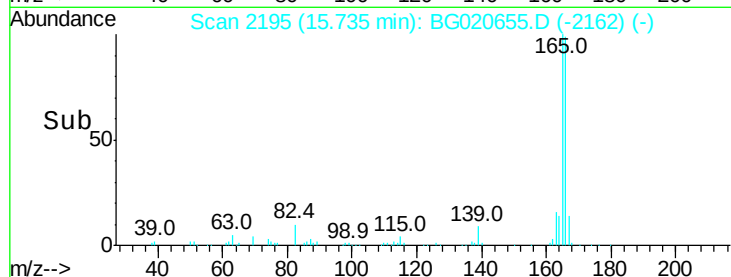

#70

Phenanthrene

Concen: 40.37 ng/ul

RT: 17.48 min Scan# 2492

Delta R.T. 0.00 min

Lab File: BG020655.D

Acq: 5 Jan 2016 14:21


Tgt Ion:178 Resp: 302876

Ion Ratio Lower Upper

178 100

179 16.4 12.3 18.5



176 20.0 15.4 23.0

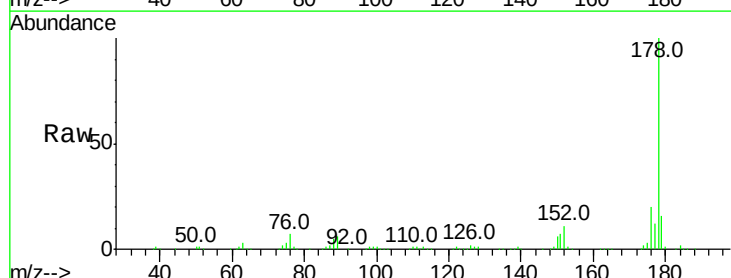


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

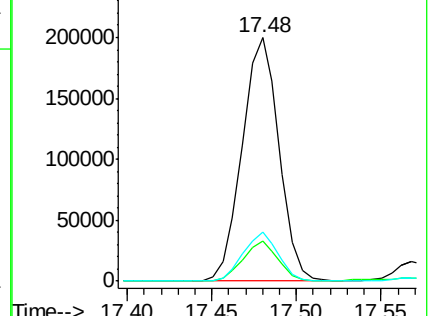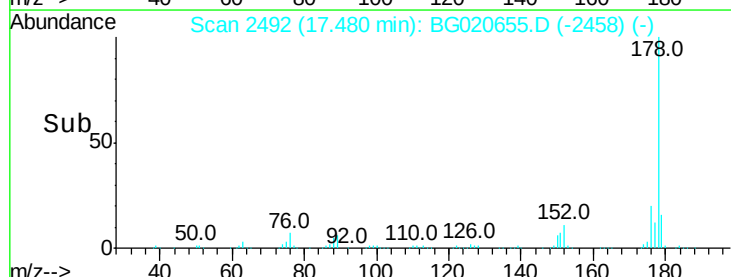

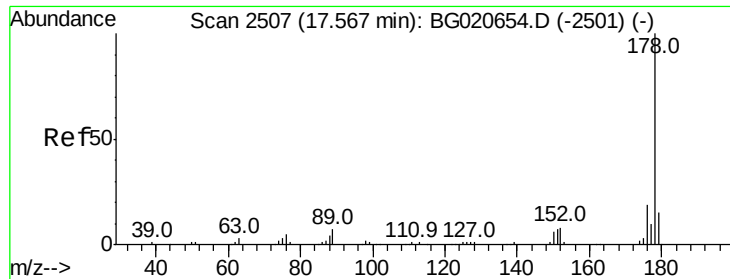

#72

Anthracene

Concen: 3.12 ng/ul

RT: 17.57 min Scan# 2507

Delta R.T. 0.00 min

Lab File: BG020655.D

Acq: 5 Jan 2016 14:21

Instrument :

BNA_G

ClientSampleId :

D9N58


Tot Ion:178 Resp: 23935

Ion	Ratio	Lower	Upper
178	100		
179	14.8	13.4	20.2
176	18.5	15.4	23.0

178 100

179 14.8 13.4 20.2




176 18.5 15.4 23.0

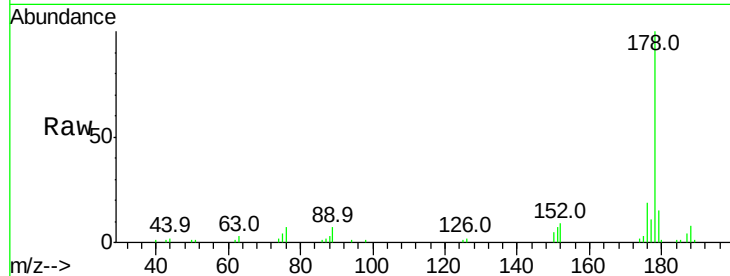

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

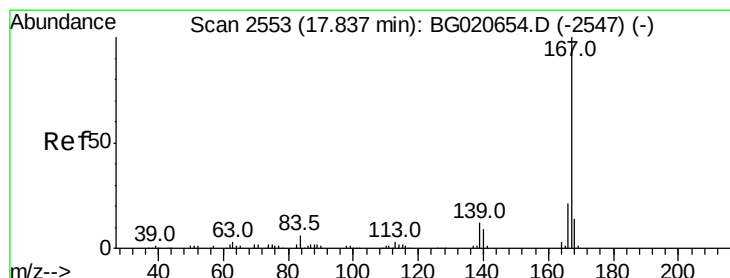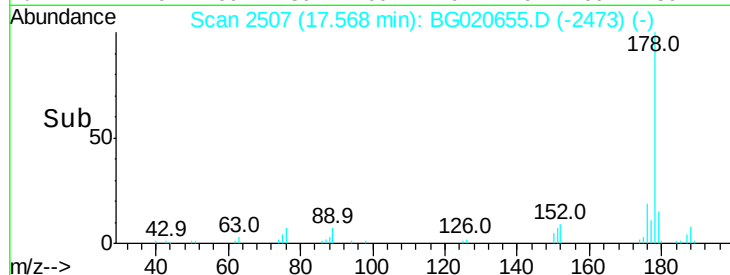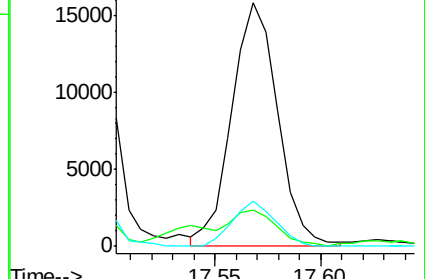

#75

Carbazole

Concen: 3.34 ng/ul

RT: 17.84 min Scan# 2553

Delta R.T. 0.00 min

Lab File: BG020655.D

Acq: 5 Jan 2016 14:21


Tgt Ion:167 Resp: 21624

Ion	Ratio	Lower	Upper
167	100		
166	23.0	17.0	25.4
139	10.7	9.1	13.7

167 100

166 23.0 17.0 25.4



139 10.7 9.1 13.7

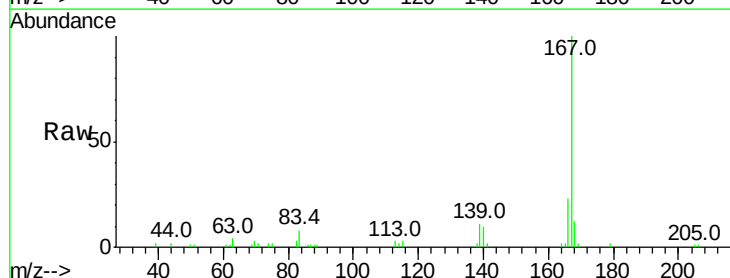


Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E



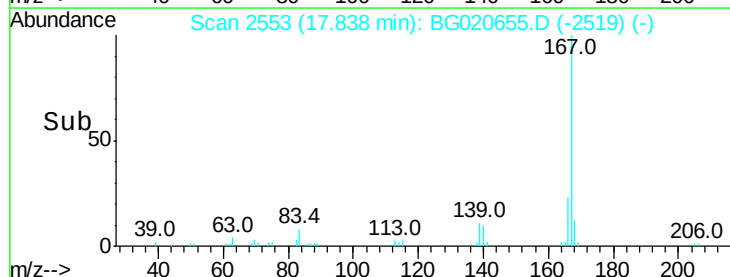
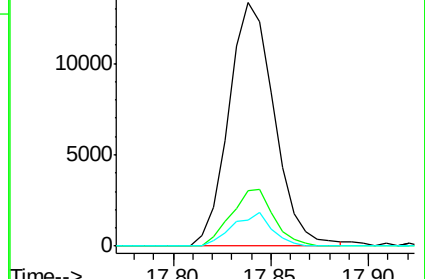


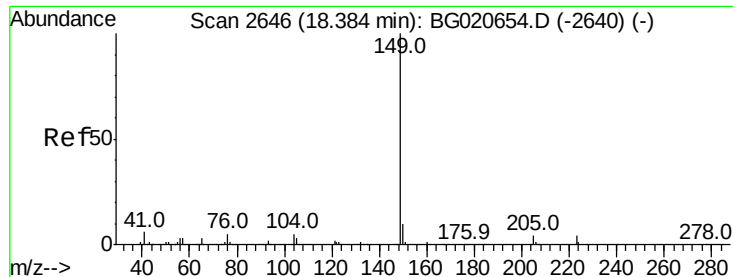

#76
Di-n-butylphthalate
Concen: 1.41 ng/ul
RT: 18.38 min Scan# 2645
Delta R.T. -0.01 min
Lab File: BG020655.D
Acq: 5 Jan 2016 14:21




Instrument :
BNA_G
ClientSampleId :
D9N58


Tot Ion:149 Resp: 10704
Ion Ratio Lower Upper
149 100
150 9.7 7.5 11.3
104 6.0 4.1 6.1

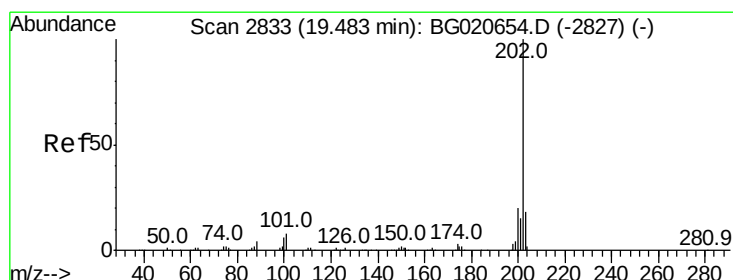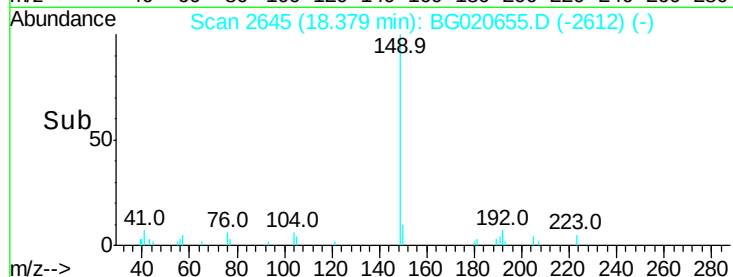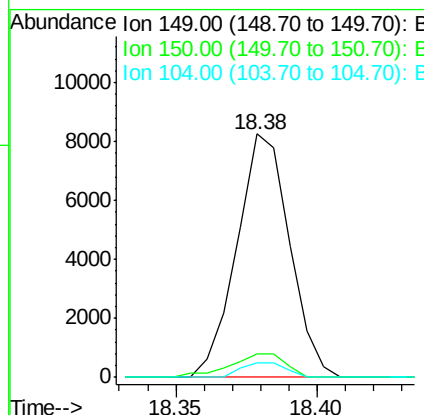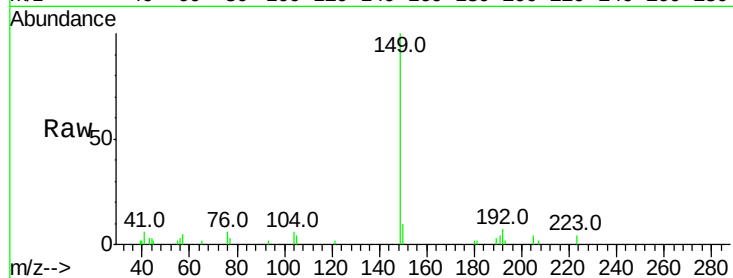

#77
Fluoranthene
Concen: 6.06 ng/ul
RT: 19.48 min Scan# 2833
Delta R.T. 0.00 min
Lab File: BG020655.D
Acq: 5 Jan 2016 14:21

Tgt Ion:202 Resp: 55549
Ion Ratio Lower Upper
202 100
101 7.6 6.1 9.1
100 6.2 4.6 7.0

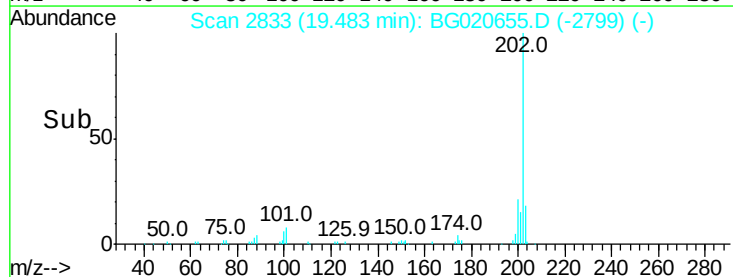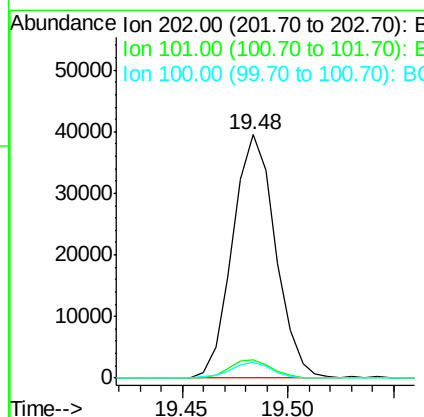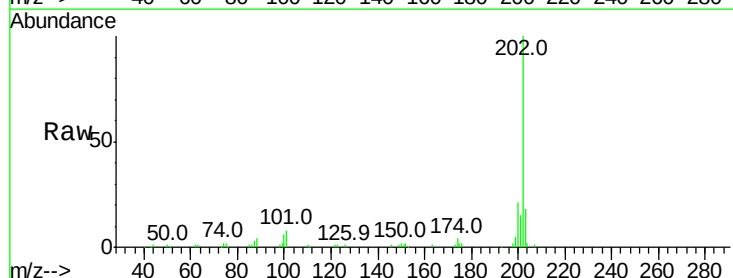

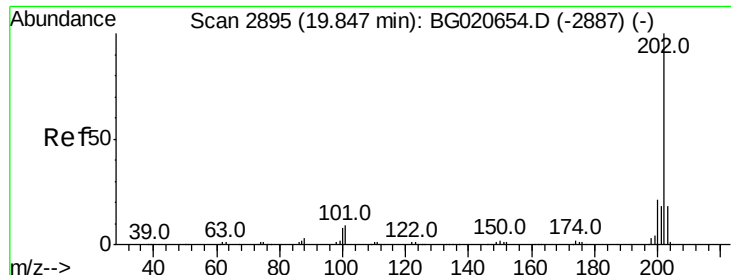

#80

Pvrene

Concen: 3.74 ng/ul

RT: 19.85 min Scan# 2895

Delta R.T. 0.00 min

Lab File: BG020655.D


Acq: 5 Jan 2016 14:21

Instrument :

BNA_G

ClientSampleId :

D9N58

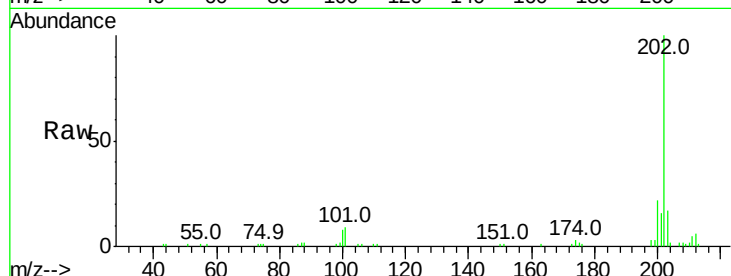


Tot Ion:202 Resp: 35290

Ion Ratio Lower Upper

202 100

101 9.0 6.9 10.3

100 7.8 5.6 8.4

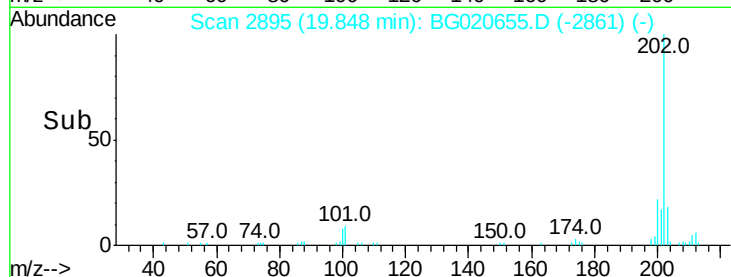

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

