


Data Path : Z:\HPCHEM1\BNA G\DATA\BG010516\
 Data File : BG020653.D
 Acq On : 5 Jan 2016 11:17
 Operator : UM/SJ
 Sample : DFTPP20
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP20

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG123015.M
 Title : SVOA CALIBRATION
 Last Update : Wed Jan 06 04:25:43 2016

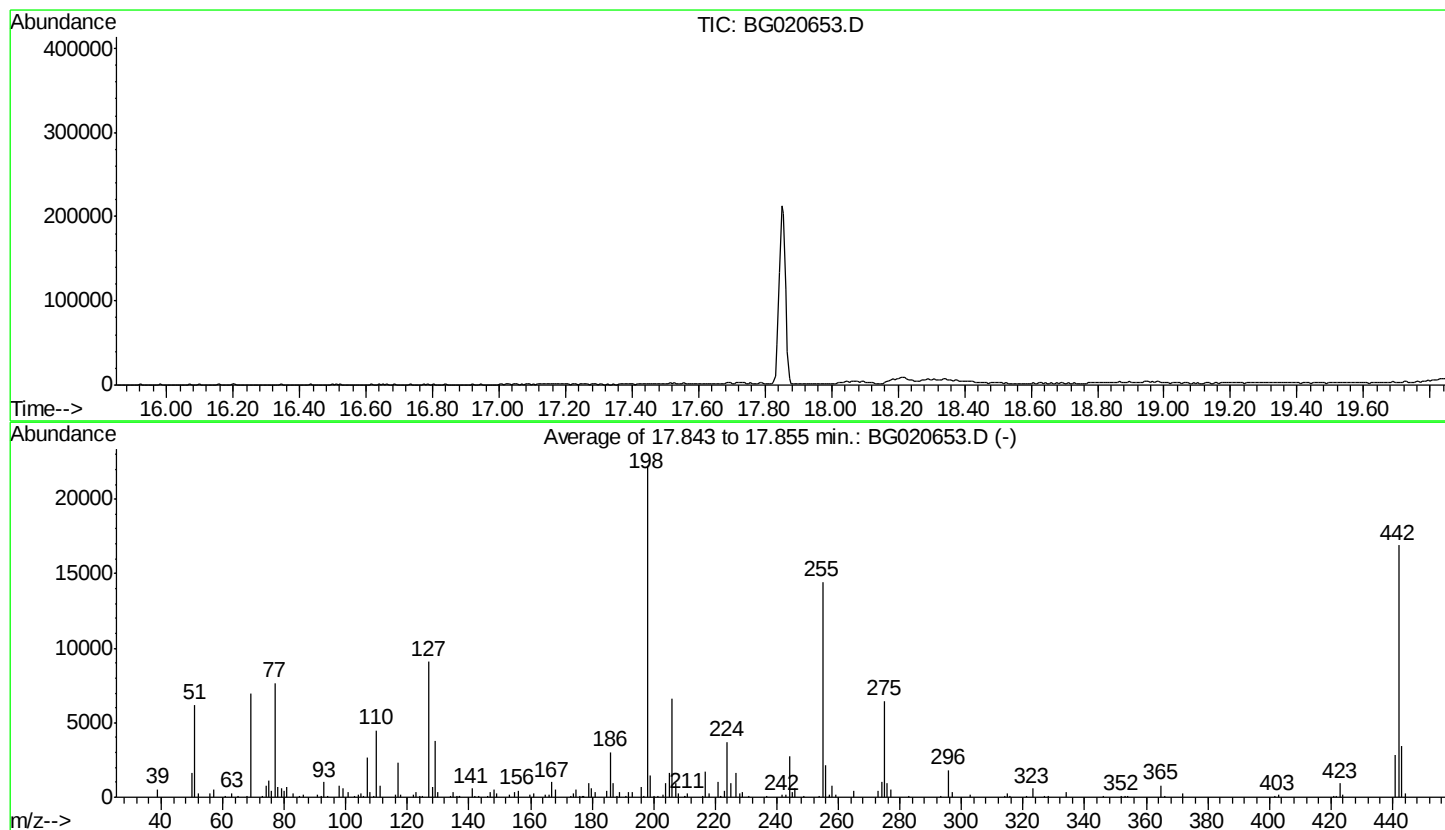

AutoFind: Scans 2554, 2555, 2556; Background Corrected with Scan 2549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	6195	PASS
68	69	0.00	2	0.8	58	PASS
69	198	0.00	100	31.4	6986	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.8	9087	PASS
197	198	0.00	2	0.4	100	PASS
198	198	100	100	100.0	22253	PASS
199	198	5	9	6.7	1501	PASS
275	198	10	60	29.1	6476	PASS
365	198	1	100	3.5	777	PASS
441	442	0.01	100	16.6	2801	PASS
442	198	50	100	76.0	16923	PASS
443	442	15	24	20.2	3413	PASS

m/z	Abundance
39.00	515.0
43.00	244.0
43.90	254.0
50.00	1263.0
51.00	5042.0
52.00	283.0
56.00	348.0
57.00	476.0
61.00	160.0
63.00	271.0
69.00	5948.0
74.00	755.0
75.00	917.0
76.00	272.0
77.00	6658.0
78.00	574.0
79.00	578.0
80.00	273.0
80.90	462.0
82.90	202.0
86.00	179.0
91.00	152.0
92.90	834.0
98.00	700.0
98.90	505.0
100.90	268.0
103.90	164.0
105.00	580.0
107.00	2205.0
108.00	350.0
108.90	158.0
109.90	3646.0
111.00	604.0
116.00	198.0
117.00	1693.0
118.00	171.0
122.00	226.0
122.90	284.0
127.00	7490.0
128.00	740.0
129.00	3050.0
130.00	219.0
133.90	160.0
135.00	265.0
141.00	454.0
145.90	176.0
147.00	242.0
148.00	382.0
149.00	217.0
152.90	153.0
155.00	252.0
155.90	418.0
159.90	167.0
161.00	229.0
167.00	791.0
168.00	422.0
173.90	177.0
174.90	526.0
176.90	196.0
178.90	617.0
179.90	448.0
181.00	240.0
184.90	313.0
186.00	2158.0
186.90	688.0
189.00	275.0
191.90	221.0
193.00	286.0
196.00	385.0
197.90	16816.0
198.90	1146.0
204.00	809.0
205.00	1109.0
206.00	4966.0
207.00	689.0
207.90	219.0
210.00	156.0
211.10	206.0
216.90	1323.0
218.00	157.0
221.00	698.0
221.70	190.0
222.90	285.0
224.00	2952.0
224.90	688.0
226.90	1256.0
227.80	172.0
228.90	182.0
242.90	189.0
244.00	1777.0
245.00	303.0
246.00	457.0

Instrument :
BNA_G
ClientSampleId :
DFTPP20

255.00	10251.0
255.90	1628.0
256.90	160.0
257.90	435.0
259.00	185.0
265.00	281.0
272.90	268.0
274.00	685.0
275.00	4189.0
276.00	482.0
276.90	302.0
296.00	1268.0
297.00	248.0
303.00	157.0
314.90	227.0
323.00	396.0
334.00	209.0
364.90	499.0
372.00	157.0
423.00	590.0
441.00	1424.0
442.00	9321.0
443.00	2286.0

Instrument :
BNA_G
ClientSampleId :
DFTPP20

m/z	Abundance
39.00	629.0
39.90	267.0
43.10	340.0
43.90	333.0
50.00	2018.0
51.00	7407.0
52.10	270.0
55.00	158.0
55.90	323.0
57.00	617.0
63.00	326.0
65.00	172.0
69.00	8310.0
74.00	907.0
75.00	1283.0
76.00	492.0
77.00	9401.0
78.00	651.0
78.90	684.0
79.90	572.0
81.00	838.0
83.00	286.0
84.90	182.0
86.00	226.0
90.90	286.0
92.00	214.0
93.00	1173.0
98.00	931.0
99.00	623.0
101.00	328.0
103.00	180.0
103.90	224.0
105.00	432.0
105.90	173.0
107.00	3233.0
108.00	470.0
110.00	5133.0
111.00	934.0
116.00	192.0
117.00	2871.0
117.90	178.0
122.00	185.0
123.00	338.0
123.90	186.0
124.90	236.0
127.00	10426.0
128.00	785.0
128.90	4528.0
130.00	464.0
135.00	366.0
135.90	178.0
136.90	231.0
141.00	741.0
147.00	259.0
147.90	640.0
148.90	343.0
153.00	192.0
155.00	342.0
156.00	529.0
160.00	230.0
161.00	285.0
164.90	384.0
166.00	221.0
166.90	1227.0
167.90	637.0
173.90	443.0
175.00	474.0
176.00	257.0
176.90	198.0
178.90	968.0
180.00	755.0
180.90	351.0
184.90	506.0
186.00	3841.0
187.00	1188.0
188.90	388.0
191.90	416.0
193.00	455.0
196.00	895.0
196.70	302.0
197.90	25760.0
198.90	1847.0
200.00	158.0
201.50	195.0
203.00	277.0
204.00	1112.0
205.00	1850.0
206.00	7821.0
207.00	1127.0
207.90	395.0
211.00	260.0
216.90	1899.0

Instrument :
BNA_G
ClientSampleId :
DFTPP20

218.00	316.0
220.90	1206.0
223.00	403.0
224.00	3883.0
225.00	1249.0
226.90	1979.0
227.90	362.0
228.90	398.0
231.00	161.0
241.90	231.0
244.00	3657.0
245.00	426.0
245.90	679.0
249.00	190.0
253.90	212.0
255.00	16219.0
256.00	2362.0
257.20	177.0
258.00	901.0
258.90	159.0
264.90	454.0
272.90	560.0
274.00	1085.0
275.00	7528.0
276.00	1094.0
277.00	543.0
283.00	165.0
295.90	1974.0
297.00	386.0
302.90	286.0
315.00	204.0
323.00	691.0
327.00	156.0
334.00	360.0
345.90	232.0
352.00	206.0
364.90	817.0
372.00	284.0
401.90	236.0
403.00	225.0
421.00	171.0
423.00	1004.0
424.00	208.0
441.00	3103.0
442.00	19464.0
443.00	3633.0
444.00	389.0

Instrument :
BNA_G
ClientSampleId :
DFTPP20

m/z	Abundance
39.00	447.0
39.90	190.0
43.00	286.0
44.00	395.0
50.00	1514.0
51.00	6137.0
52.00	312.0
55.00	162.0
55.90	231.0
57.00	581.0
63.00	280.0
68.00	175.0
69.00	6702.0
73.00	170.0
74.00	777.0
75.00	1183.0
76.00	472.0
77.00	7551.0
78.00	736.0
79.00	464.0
80.00	470.0
81.00	740.0
83.00	196.0
86.00	198.0
90.90	199.0
92.90	1020.0
94.00	156.0
98.00	773.0
98.90	666.0
101.00	330.0
103.90	244.0
104.90	463.0
107.00	2620.0
108.00	297.0
110.00	4680.0
110.90	738.0
115.90	204.0
117.00	2331.0
118.00	168.0
122.00	184.0
123.00	309.0
127.00	9345.0
128.00	606.0
128.90	3792.0
130.00	367.0
135.00	354.0
137.10	184.0
141.00	493.0
141.90	245.0
143.00	155.0
146.90	484.0
148.00	523.0
149.00	274.0
152.90	243.0
155.00	348.0
156.00	389.0
159.90	246.0
160.90	337.0
165.00	249.0
166.00	312.0
167.00	1065.0
168.00	621.0
172.90	151.0
173.90	264.0
175.00	530.0
177.10	216.0
178.90	1180.0
179.90	668.0
181.00	352.0
184.90	538.0
186.00	3136.0
186.90	973.0
188.00	170.0
189.00	382.0
190.90	203.0
192.00	362.0
192.90	320.0
195.90	874.0
197.90	24184.0
198.90	1510.0
203.00	230.0
204.00	806.0
205.00	1891.0
206.00	7125.0
207.00	1145.0
207.90	252.0
210.30	198.0
210.90	275.0
215.90	208.0
216.90	1972.0
218.00	247.0
220.90	1178.0

Instrument :
BNA_G
ClientSampleId :
DFTPP20

221.90	260.0
222.90	504.0
224.00	4278.0
225.00	1032.0
226.90	1671.0
227.90	164.0
229.00	371.0
231.00	184.0
236.90	244.0
241.90	249.0
243.00	208.0
244.00	2926.0
245.00	365.0
246.00	786.0
248.80	155.0
255.00	16960.0
255.90	2524.0
257.00	285.0
257.90	928.0
259.00	194.0
264.90	498.0
273.00	531.0
273.90	1319.0
275.00	7713.0
275.90	1171.0
276.90	778.0
293.10	163.0
295.90	2304.0
296.90	365.0
303.00	206.0
313.90	167.0
314.80	287.0
315.90	251.0
321.00	156.0
323.00	706.0
328.00	174.0
334.00	438.0
352.00	182.0
353.00	158.0
354.00	202.0
364.90	1016.0
366.00	151.0
372.00	320.0
402.90	183.0
421.00	186.0
421.90	155.0
423.00	1165.0
424.00	199.0
441.00	3877.0
442.00	21984.0
443.00	4322.0
444.00	357.0

Instrument :
BNA_G
ClientSampleId :
DFTPP20

Scan 2549 (17.814 min): BG020653.D
DFTPP20

m/z	Abundance
40.00	152.0
43.00	353.0
44.00	336.0
45.10	169.0
55.00	165.0
77.00	192.0
105.00	259.0

Instrument :
BNA_G
ClientSampleId :
DFTPP20