


Data Path : U:\HPCHEM1\BNA G\Data\BG010518\
 Data File : BG031929.D
 Acq On : 5 Jan 2018 12:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 05 15:31:34 2018

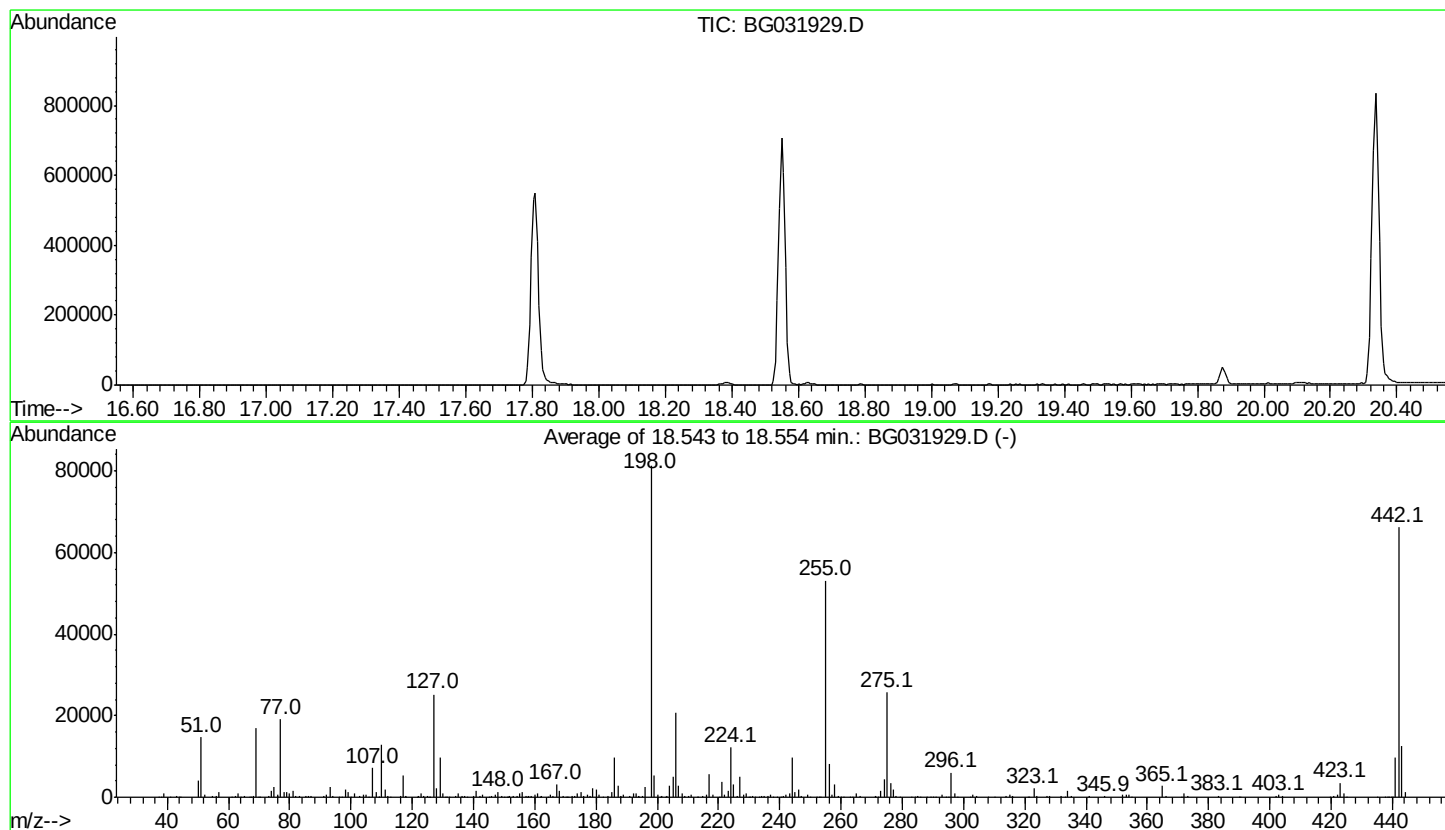

AutoFind: Scans 2596, 2597, 2598; Background Corrected with Scan 2590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.0	14607	PASS
68	69	0.00	2	1.1	187	PASS
69	198	0.00	100	20.8	16885	PASS
70	69	0.00	2	0.4	69	PASS
127	198	10	80	31.0	25192	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81266	PASS
199	198	5	9	6.5	5320	PASS
275	198	10	60	31.5	25616	PASS
365	198	1	100	3.5	2808	PASS
441	442	0.01	24	14.8	9806	PASS
442	198	50	100	81.3	66058	PASS
443	442	15	24	19.1	12605	PASS