
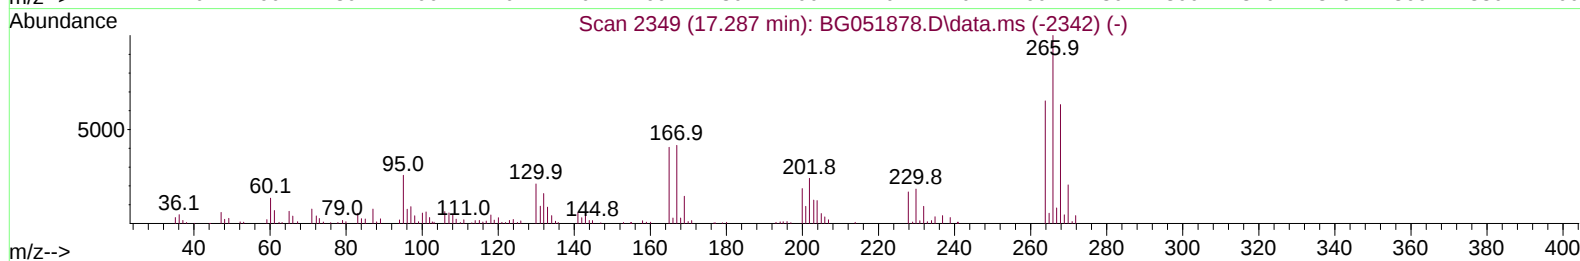
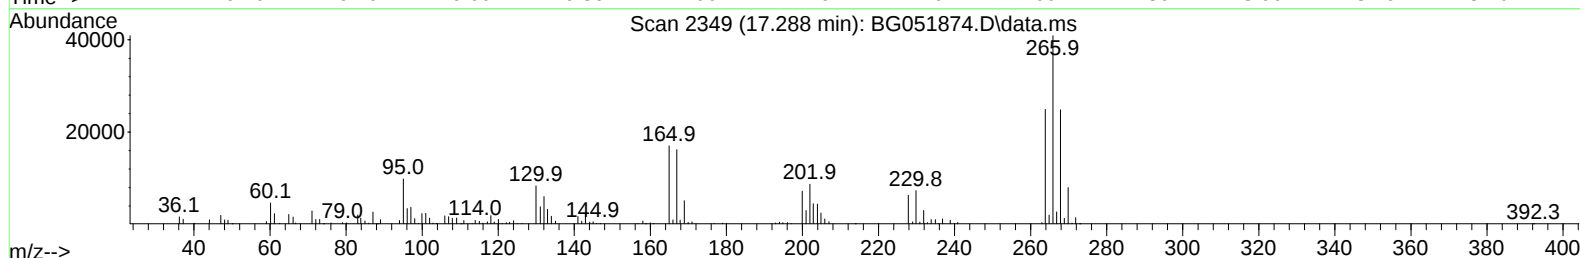


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010522\
Data File : BG051874.D
Acq On : 5 Jan 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 06:53:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 07 06:40:51 2022
Response via : Initial Calibration

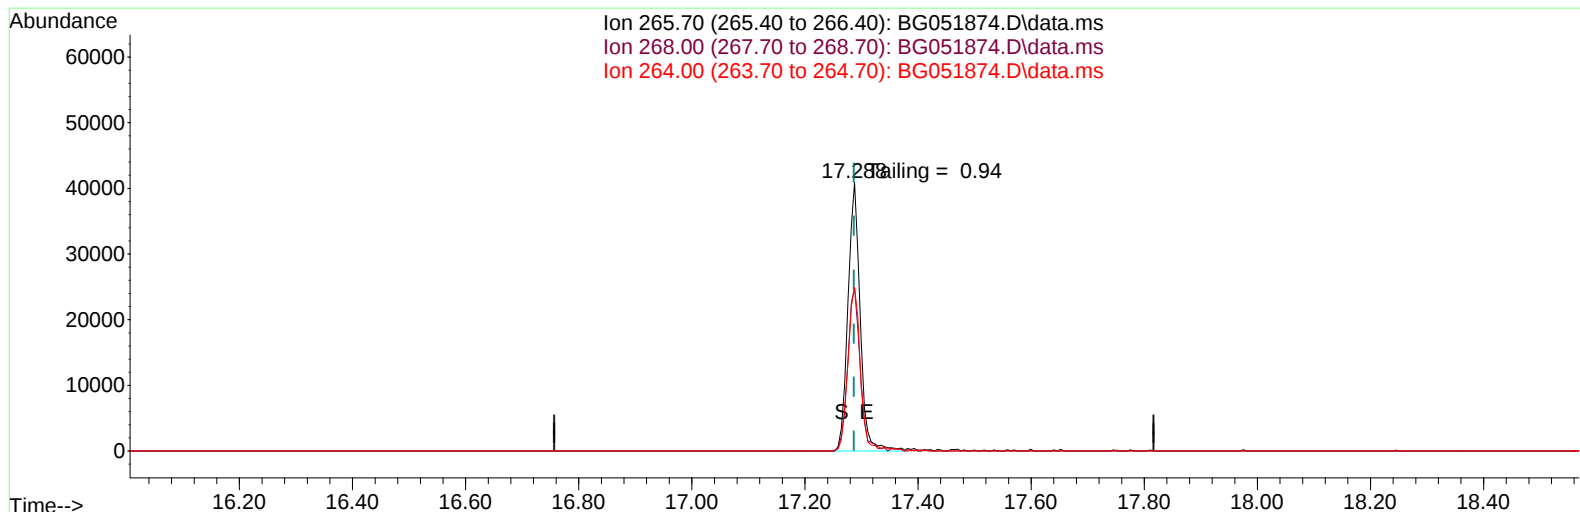

TIC: BG051874.D\data.ms

(70) Pentachlorophenol (C)




17.288min (+ 0.001) 19727.97 ng

response 61769

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	60.74
264.00	65.20	61.03
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010522\  
Data File : BG051874.D  
Acq On    : 5 Jan 2022 10:11  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Jan 07 06:53:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 07 06:40:51 2022
Response via : Initial Calibration

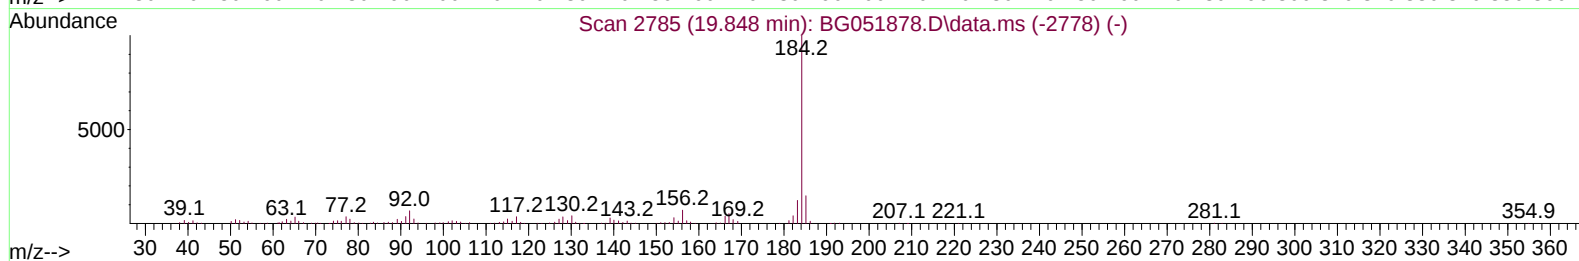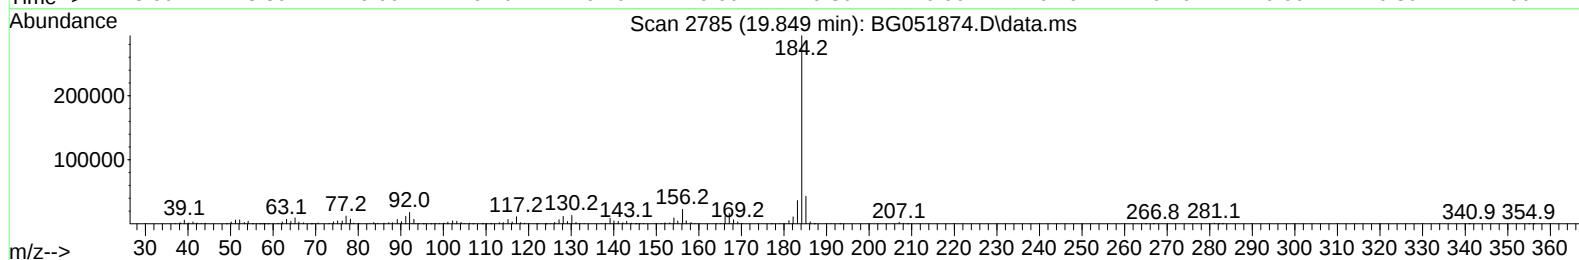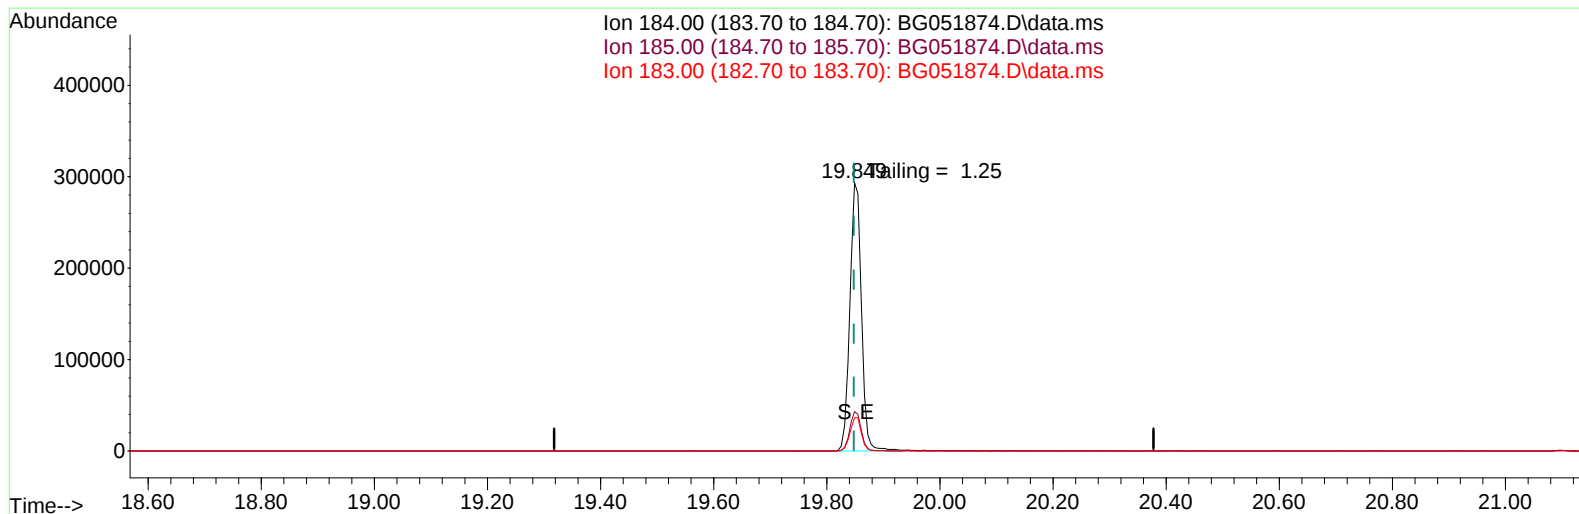

TIC: BG051874.D\data.ms

(77) Benzidine

19.849min (+ 0.001) 0.00 ng m

response **417755**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.80	14.67
--------	-------	-------

183.00	12.20	12.41
--------	-------	-------

0.00 0.00 0.00