

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010523\
 Data File : BG056209.D
 Acq On : 5 Jan 2023 10:28
 Operator : CG/JU
 Sample : PB149944BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK944

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056209.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	7	12	16	rVB3	9408	13476	0.84%	0.092%
2	3.634	55	59	63	rVB2	7698	10894	0.68%	0.074%
3	3.781	81	84	87	rVB2	2182	3058	0.19%	0.021%
4	3.811	87	89	91	rBV2	2411	2307	0.14%	0.016%
5	4.069	130	133	147	rBV	96225	162476	10.07%	1.108%
6	4.163	147	149	153	rVB2	1979	1621	0.10%	0.011%
7	4.422	190	193	198	rVB3	2233	3243	0.20%	0.022%
8	7.459	702	710	720	rBV	135503	238681	14.79%	1.628%
9	7.642	733	741	749	rVB	112541	186735	11.57%	1.274%
10	7.859	771	778	787	rBV	138545	241125	14.95%	1.645%
11	8.335	847	859	867	rBB	128200	213680	13.24%	1.458%
12	9.022	969	976	987	rBV	200701	339826	21.06%	2.318%
13	9.504	1050	1058	1066	rBB	129753	234407	14.53%	1.599%
14	10.233	1175	1182	1191	rBB	125439	217593	13.49%	1.484%
15	10.773	1267	1274	1282	rBV	213177	381457	23.64%	2.602%
16	11.167	1333	1341	1350	rBB	186136	331054	20.52%	2.258%
17	11.290	1354	1362	1372	rVV	197699	347396	21.53%	2.370%
18	12.730	1600	1607	1611	rBB	3829	6409	0.40%	0.044%
19	14.334	1872	1880	1888	rVB	485591	704618	43.68%	4.807%
20	14.645	1925	1933	1942	rVB	523528	840506	52.10%	5.733%
21	14.945	1976	1984	1993	rVB	400765	617939	38.30%	4.215%
22	15.109	2005	2012	2021	rBV	179158	276667	17.15%	1.887%
23	15.168	2021	2022	2028	rVV3	2318	3441	0.21%	0.023%
24	15.926	2144	2151	2159	rBV	759073	1160777	71.95%	7.918%
25	16.032	2163	2169	2178	rVV	190299	283900	17.60%	1.937%
26	16.167	2188	2192	2199	rBV2	2343	3917	0.24%	0.027%
27	17.471	2411	2414	2418	rVB3	1327	2083	0.13%	0.014%
28	17.677	2442	2449	2456	rBV	593035	888499	55.07%	6.061%
29	17.777	2459	2466	2476	rVB	883453	1332766	82.61%	9.091%
30	18.317	2554	2558	2559	rBV3	2353	2630	0.16%	0.018%
31	18.605	2604	2607	2612	rBV4	3245	5563	0.34%	0.038%
32	18.676	2615	2619	2622	rBV3	1179	1760	0.11%	0.012%
33	19.610	2774	2778	2783	rVB4	12842	19009	1.18%	0.130%
34	19.680	2785	2790	2795	rVV2	12420	16852	1.04%	0.115%
35	19.721	2795	2797	2799	rVB2	2370	1829	0.11%	0.012%
36	19.751	2799	2802	2804	rBV3	2464	2816	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010523\
 Data File : BG056209.D
 Acq On : 5 Jan 2023 10:28
 Operator : CG/JU
 Sample : PB149944BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK944

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
 Title : SVOA CALIBRATION

37	19.898	2825	2827	2828	rBV2	1927	1731	0.11%	0.012%
38	19.921	2828	2831	2834	rVB5	3001	3449	0.21%	0.024%
39	20.045	2845	2852	2859	rBV	1158561	1613293	100.00%	11.005%
40	20.139	2867	2868	2871	rVB2	3120	2153	0.13%	0.015%

41	20.403	2911	2913	2916	rBV4	3032	2633	0.16%	0.018%
42	20.926	3001	3002	3006	rBV4	3504	3449	0.21%	0.024%
43	21.020	3016	3018	3019	rBV	3504	2328	0.14%	0.016%
44	21.061	3023	3025	3027	rVB3	4039	3401	0.21%	0.023%
45	21.179	3044	3045	3046	rBV	4794	2482	0.15%	0.017%

46	21.196	3046	3048	3050	rVV3	5391	5792	0.36%	0.040%
47	21.461	3092	3093	3096	rBV3	3236	2512	0.16%	0.017%
48	21.484	3096	3097	3098	rBV	5234	2114	0.13%	0.014%
49	21.790	3147	3149	3150	rBV2	4165	2729	0.17%	0.019%
50	21.972	3173	3180	3189	rVB2	572421	980122	60.75%	6.686%

51	22.119	3203	3205	3206	rBV	3671	2526	0.16%	0.017%
52	22.295	3233	3235	3236	rBV2	3949	2068	0.13%	0.014%
53	22.330	3239	3241	3244	rBV4	3901	3629	0.22%	0.025%
54	22.559	3278	3280	3281	rBV2	3565	2620	0.16%	0.018%
55	23.529	3441	3445	3449	rVB6	14004	22961	1.42%	0.157%

56	23.605	3456	3458	3459	rBV	4270	4036	0.25%	0.028%
57	24.152	3549	3551	3553	rBV4	4645	3048	0.19%	0.021%
58	24.398	3587	3593	3598	rVB6	23596	45524	2.82%	0.311%
59	24.704	3644	3645	3647	rBV2	4550	2924	0.18%	0.020%
60	25.192	3717	3728	3740	rBV	529000	1525546	94.56%	10.406%

61	25.432	3757	3769	3780	rBV2	346156	1055163	65.40%	7.198%
62	25.844	3837	3839	3840	rBV2	4857	4020	0.25%	0.027%
63	26.325	3919	3921	3923	rBV3	4746	2663	0.17%	0.018%
64	26.643	3966	3975	3983	rVB5	32006	103523	6.42%	0.706%
65	27.741	4160	4162	4164	rBV3	4644	3388	0.21%	0.023%

66	27.877	4183	4185	4187	rBV2	5969	5670	0.35%	0.039%
67	27.947	4195	4197	4199	rBV3	4681	4617	0.29%	0.031%
68	28.100	4217	4223	4232	rVB7	27314	74746	4.63%	0.510%
69	28.341	4263	4264	4265	rBV	6614	3380	0.21%	0.023%
70	29.874	4517	4525	4526	rBV7	20279	35734	2.21%	0.244%

71	30.009	4546	4548	4550	rBV2	3690	3099	0.19%	0.021%
72	30.403	4613	4615	4617	rBV3	4599	5300	0.33%	0.036%
73	30.438	4619	4621	4622	rVB2	4840	2376	0.15%	0.016%
74	30.456	4622	4624	4625	rBV2	3717	2636	0.16%	0.018%
75	30.808	4682	4684	4685	rBV	4701	4199	0.26%	0.029%

76	31.279	4762	4764	4766	rVB3	3963	2766	0.17%	0.019%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010523\
Data File : BG056209.D
Acq On : 5 Jan 2023 10:28
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK944

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Title : SVOA CALIBRATION

77	31.837	4857	4859	4860	rBV2	4186	2318	0.14%	0.016%
----	--------	------	------	------	------	------	------	-------	--------




Sum of corrected areas: 14659678

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010523\
Data File : BG056209.D
Acq On : 5 Jan 2023 10:28
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

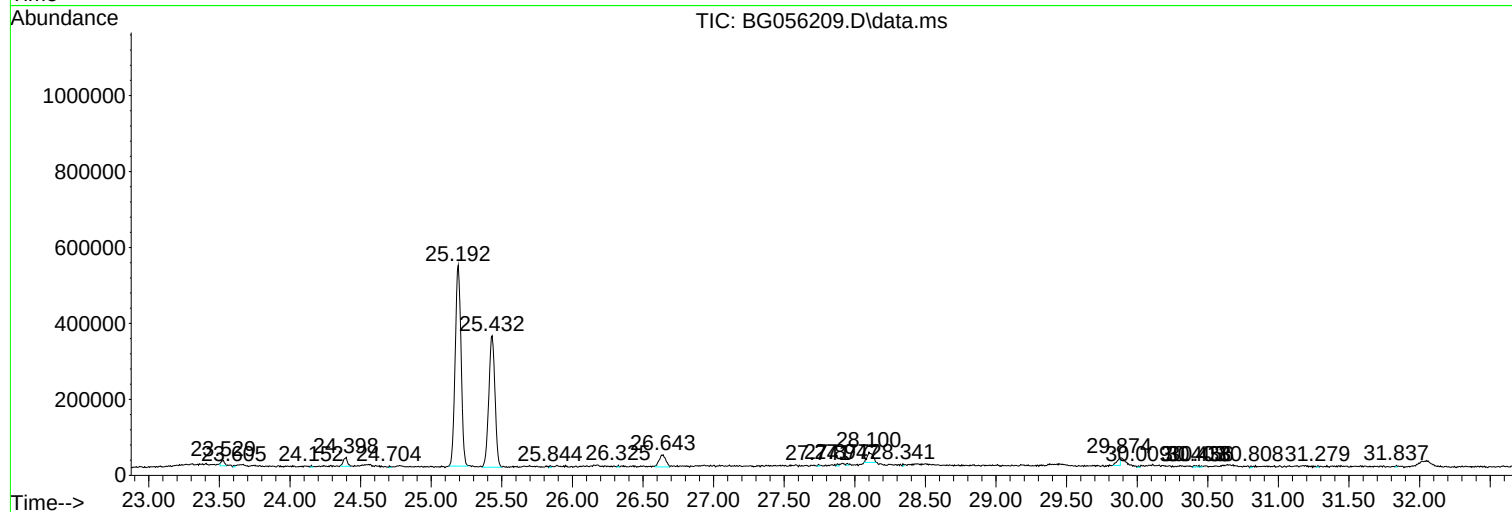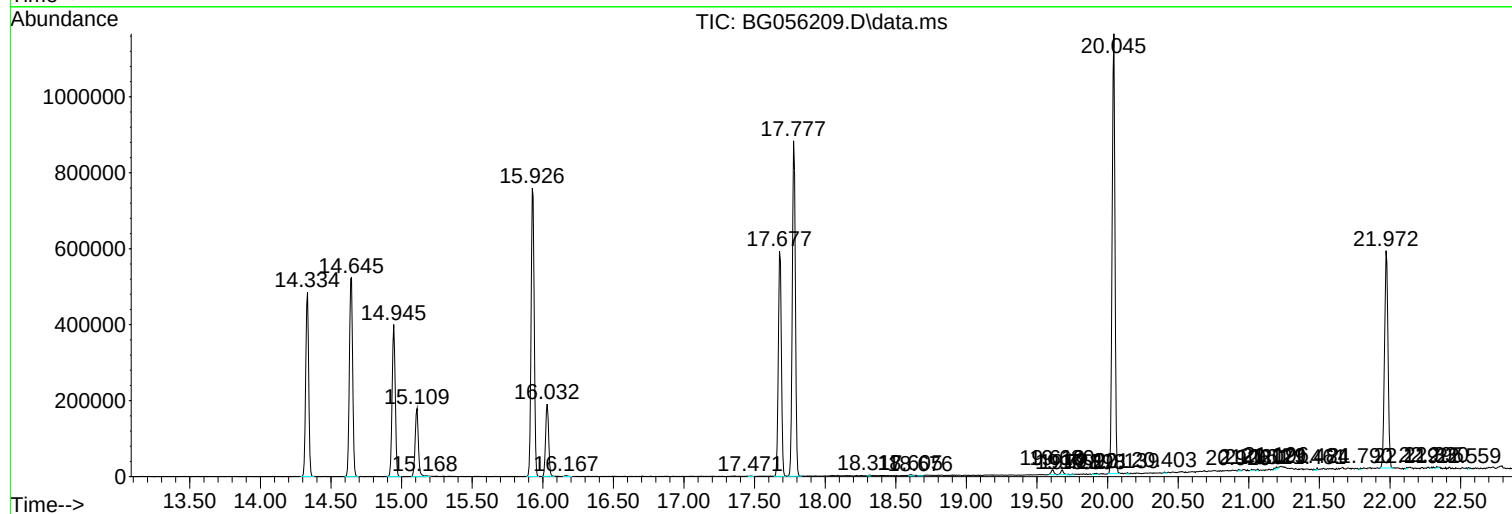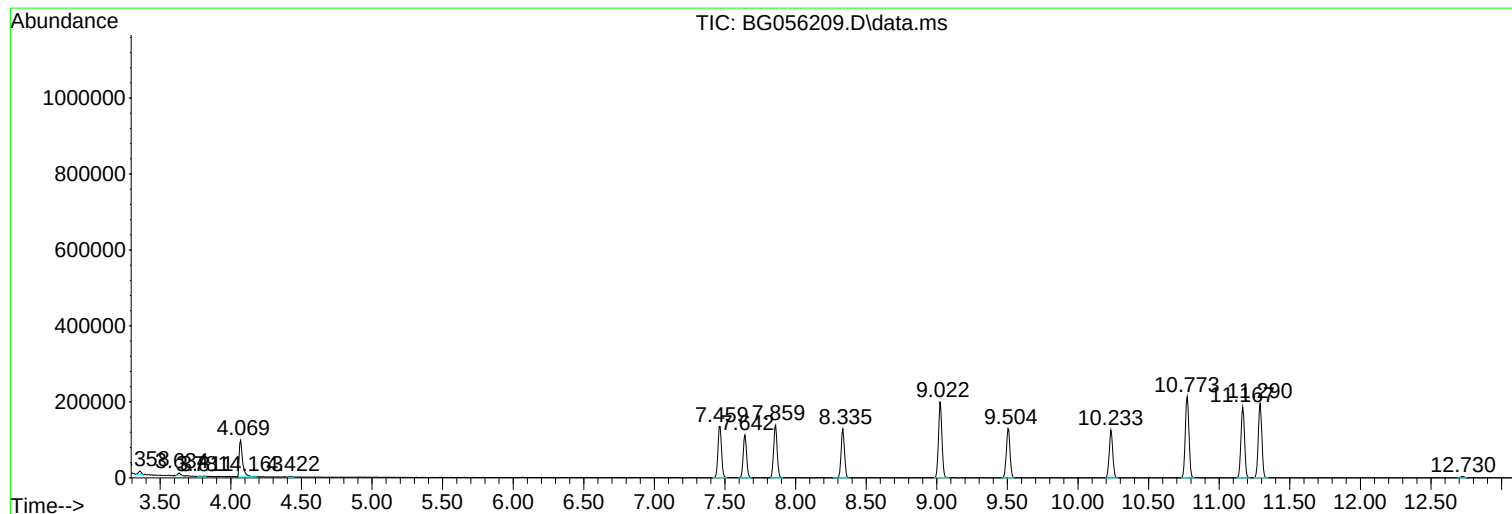

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010523\
Data File : BG056209.D
Acq On : 5 Jan 2023 10:28
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010523\
Data File : BG056209.D
Acq On : 5 Jan 2023 10:28
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc