


Data Path : S:\HPCHEM1\BNA_G\DATA\BG010615\
 Data File : BG015853.D
 Acq On : 6 Jan 2015 9:48
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG010515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 06 08:46:19 2015

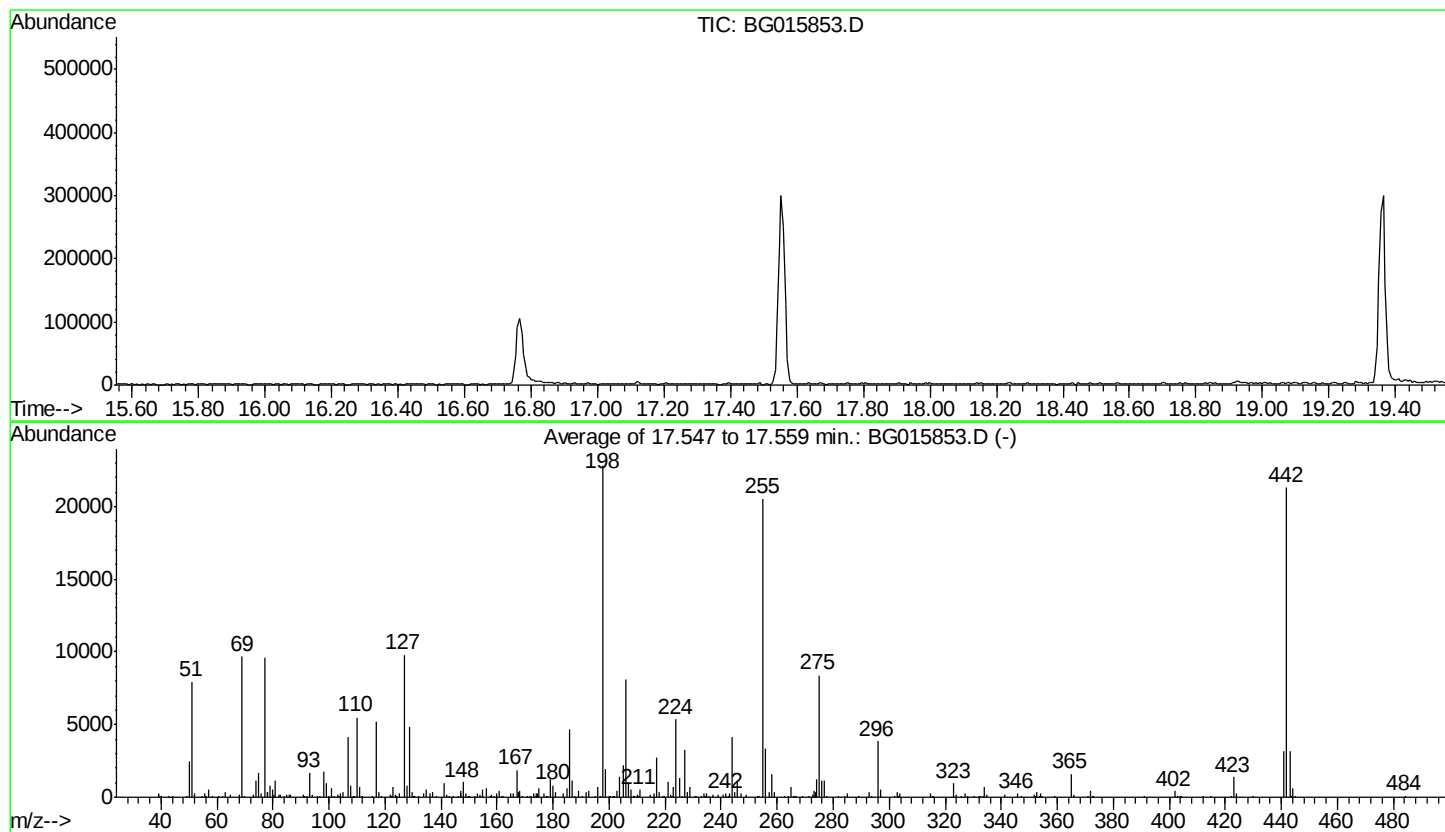

AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	7950	PASS
68	69	0.00	2	1.5	148	PASS
69	198	0.00	100	42.4	9667	PASS
70	69	0.00	2	1.1	106	PASS
127	198	10	80	42.9	9782	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22810	PASS
199	198	5	9	8.6	1973	PASS
275	198	10	60	36.7	8380	PASS
365	198	1	100	7.1	1617	PASS
441	442	0.01	24	14.8	3156	PASS
442	198	50	100	93.4	21305	PASS
443	442	15	24	15.0	3199	PASS