

Data File : BG043934.D

Acq On : 6 Jan 2020 16:41

Operator : JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Jan 07 07:52:34 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 31 13:32:23 2019

Response via : Initial Calibration

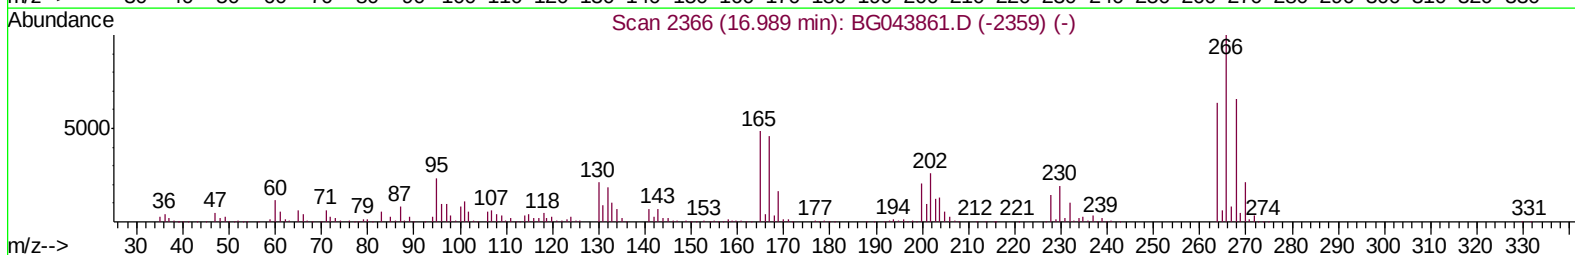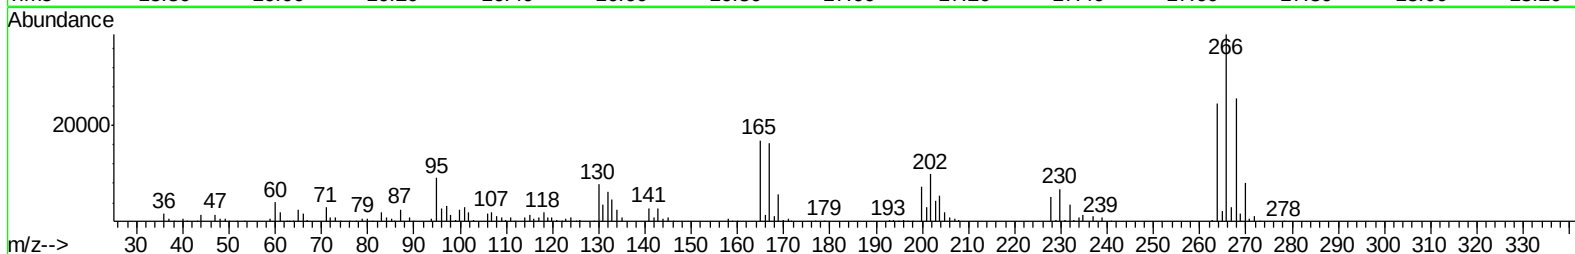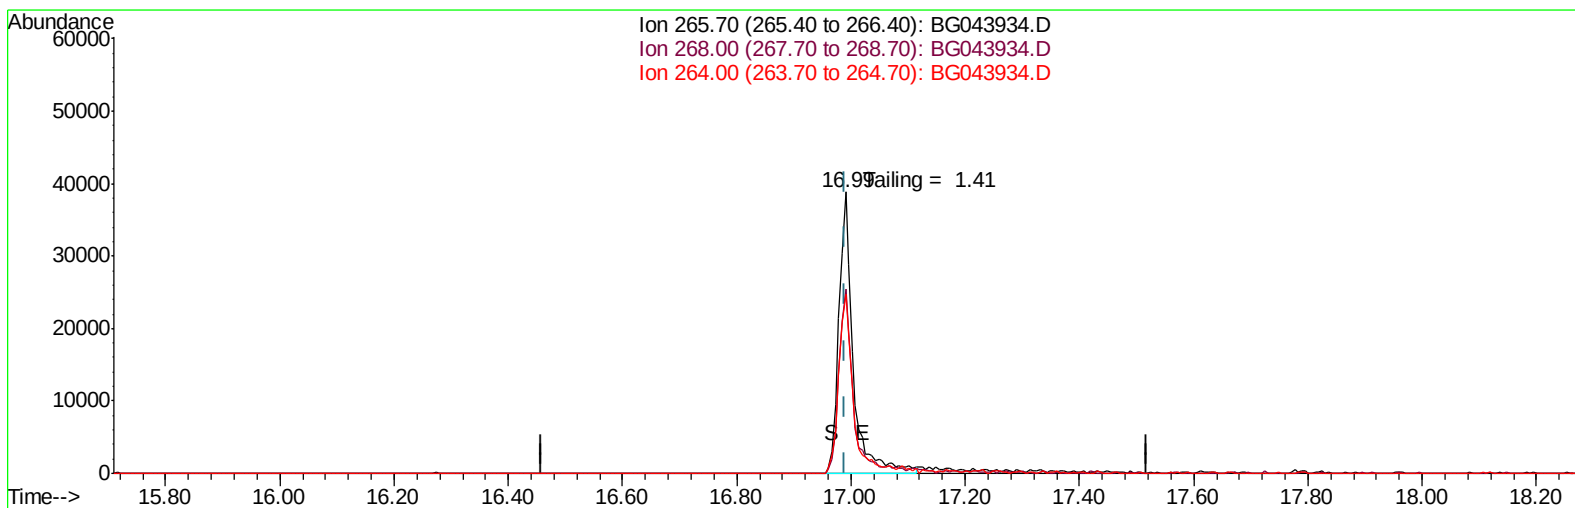

TIC: BG043934.D

(70) Pentachlorophenol (C)




16.990min (+0.001) 16738.55ng

response 66982

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	65.65
264.00	63.50	63.45
0.00	0.00	0.00

Data File : BG043934.D
Acq On : 6 Jan 2020 16:41
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 07:52:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

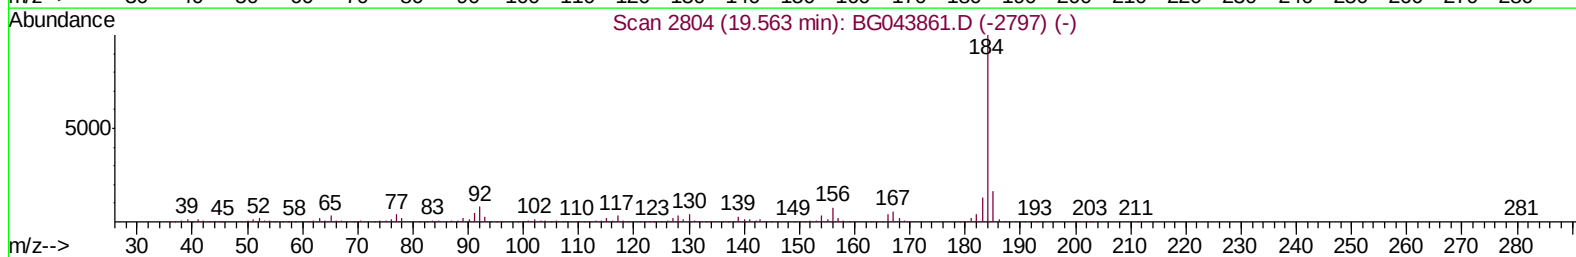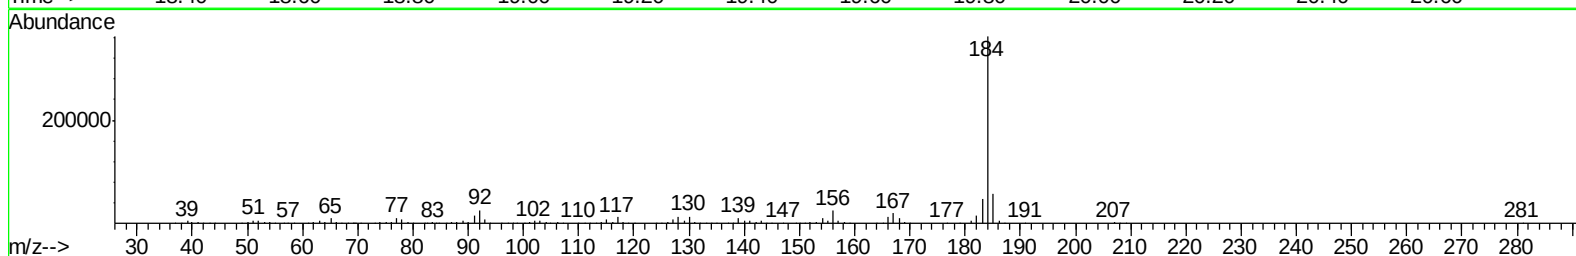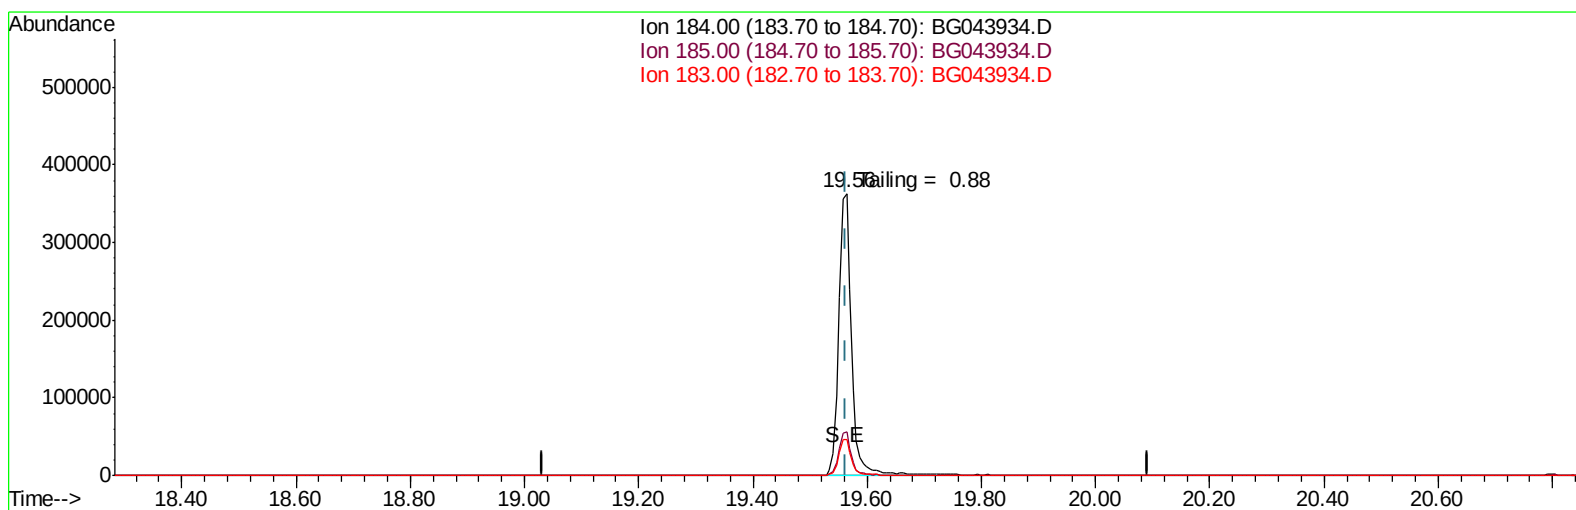

TIC: BG043934.D

(77) Benzidine

19.564min (+0.001) 0.00ng m

response 561558

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.69
183.00	13.20	12.80
0.00	0.00	0.00