


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG010620\
 Data File : BG043934.D
 Acq On : 6 Jan 2020 16:41
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

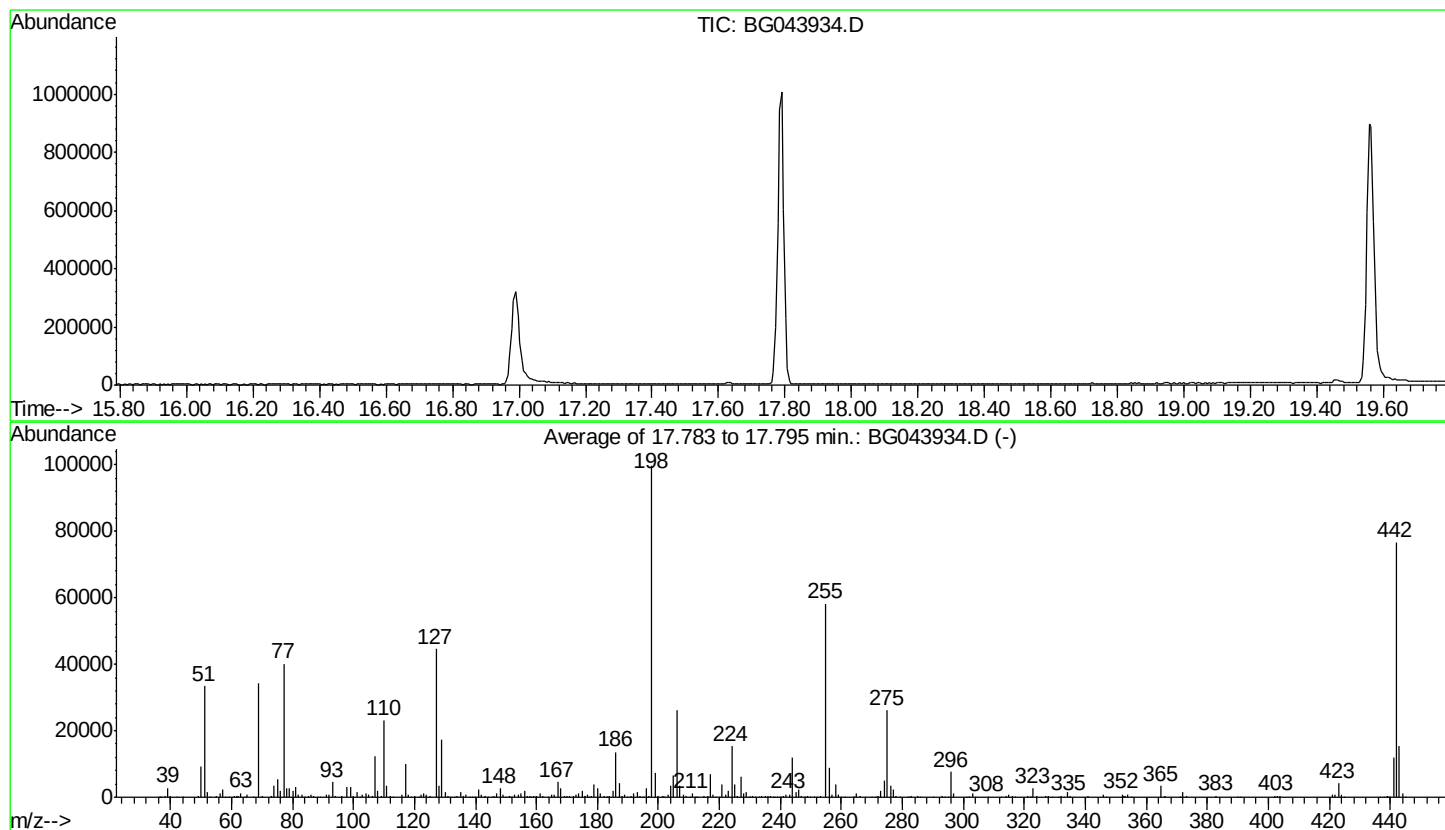

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	33453	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.3	34160	PASS
70	69	0.00	2	0.6	216	PASS
127	198	10	80	44.7	44616	PASS
197	198	0.00	2	0.3	309	PASS
198	198	100	100	100.0	99730	PASS
199	198	5	9	7.3	7270	PASS
275	198	10	60	26.2	26106	PASS
365	198	1	100	3.4	3342	PASS
441	198	0.01	100	11.9	11820	PASS
442	198	50	100	76.7	76482	PASS
443	442	15	24	20.4	15569	PASS