

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051928.D
 Acq On : 7 Jan 2022 23:28
 Operator : CG/JU
 Sample : N1026-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLG9

Quant Time: Jan 08 01:55:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.240	152	18168	20.000	ng/ul	-0.01
20) Naphthalene-d8	11.083	136	79653	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.890	164	62834	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.633	188	171818	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.957	240	190150	20.000	ng/ul	# 0.00
88) Perylene-d12	25.434	264	194067	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.570	96	2720	5.350	ng/uL	0.00
4) Pyridine-d5	4.004	84	7753	4.905	ng/ul	0.00
7) Phenol-d5	7.382	99	21390	12.029	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.547	67	17502	15.505	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.770	132	15325	13.017	ng/ul	0.00
15) 4-Methylphenol-d8	8.945	113	18191	13.160	ng/ul	0.00
21) Nitrobenzene-d5	9.421	128	9455	15.022	ng/ul	0.00
24) 2-Nitrophenol-d4	10.149	143	10455	15.019	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.695	165	17275	12.696	ng/ul	0.00
31) 4-Chloroaniline-d4	11.206	131	19246	10.157	ng/ul	0.00
46) Dimethylphthalate-d6	14.273	166	94533	18.201	ng/ul	0.00
49) Acenaphthylene-d8	14.578	160	79343	12.647	ng/ul	0.00
54) 4-Nitrophenol-d4	15.066	143	11595	13.353	ng/ul	0.00
60) Fluorene-d10	15.877	176	68379	15.100	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.976	200	9129	8.422	ng/ul	0.00
73) Anthracene-d10	17.733	188	120802	14.821	ng/ul	0.00
81) Pyrene-d10	20.012	212	143378	13.102	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.199	264	117630	11.514	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.816	149	28930	4.565	ng/ul#	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051928.D
Acq On : 7 Jan 2022 23:28
Operator : CG/JU
Sample : N1026-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLG9


Quant Time: Jan 08 01:55:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

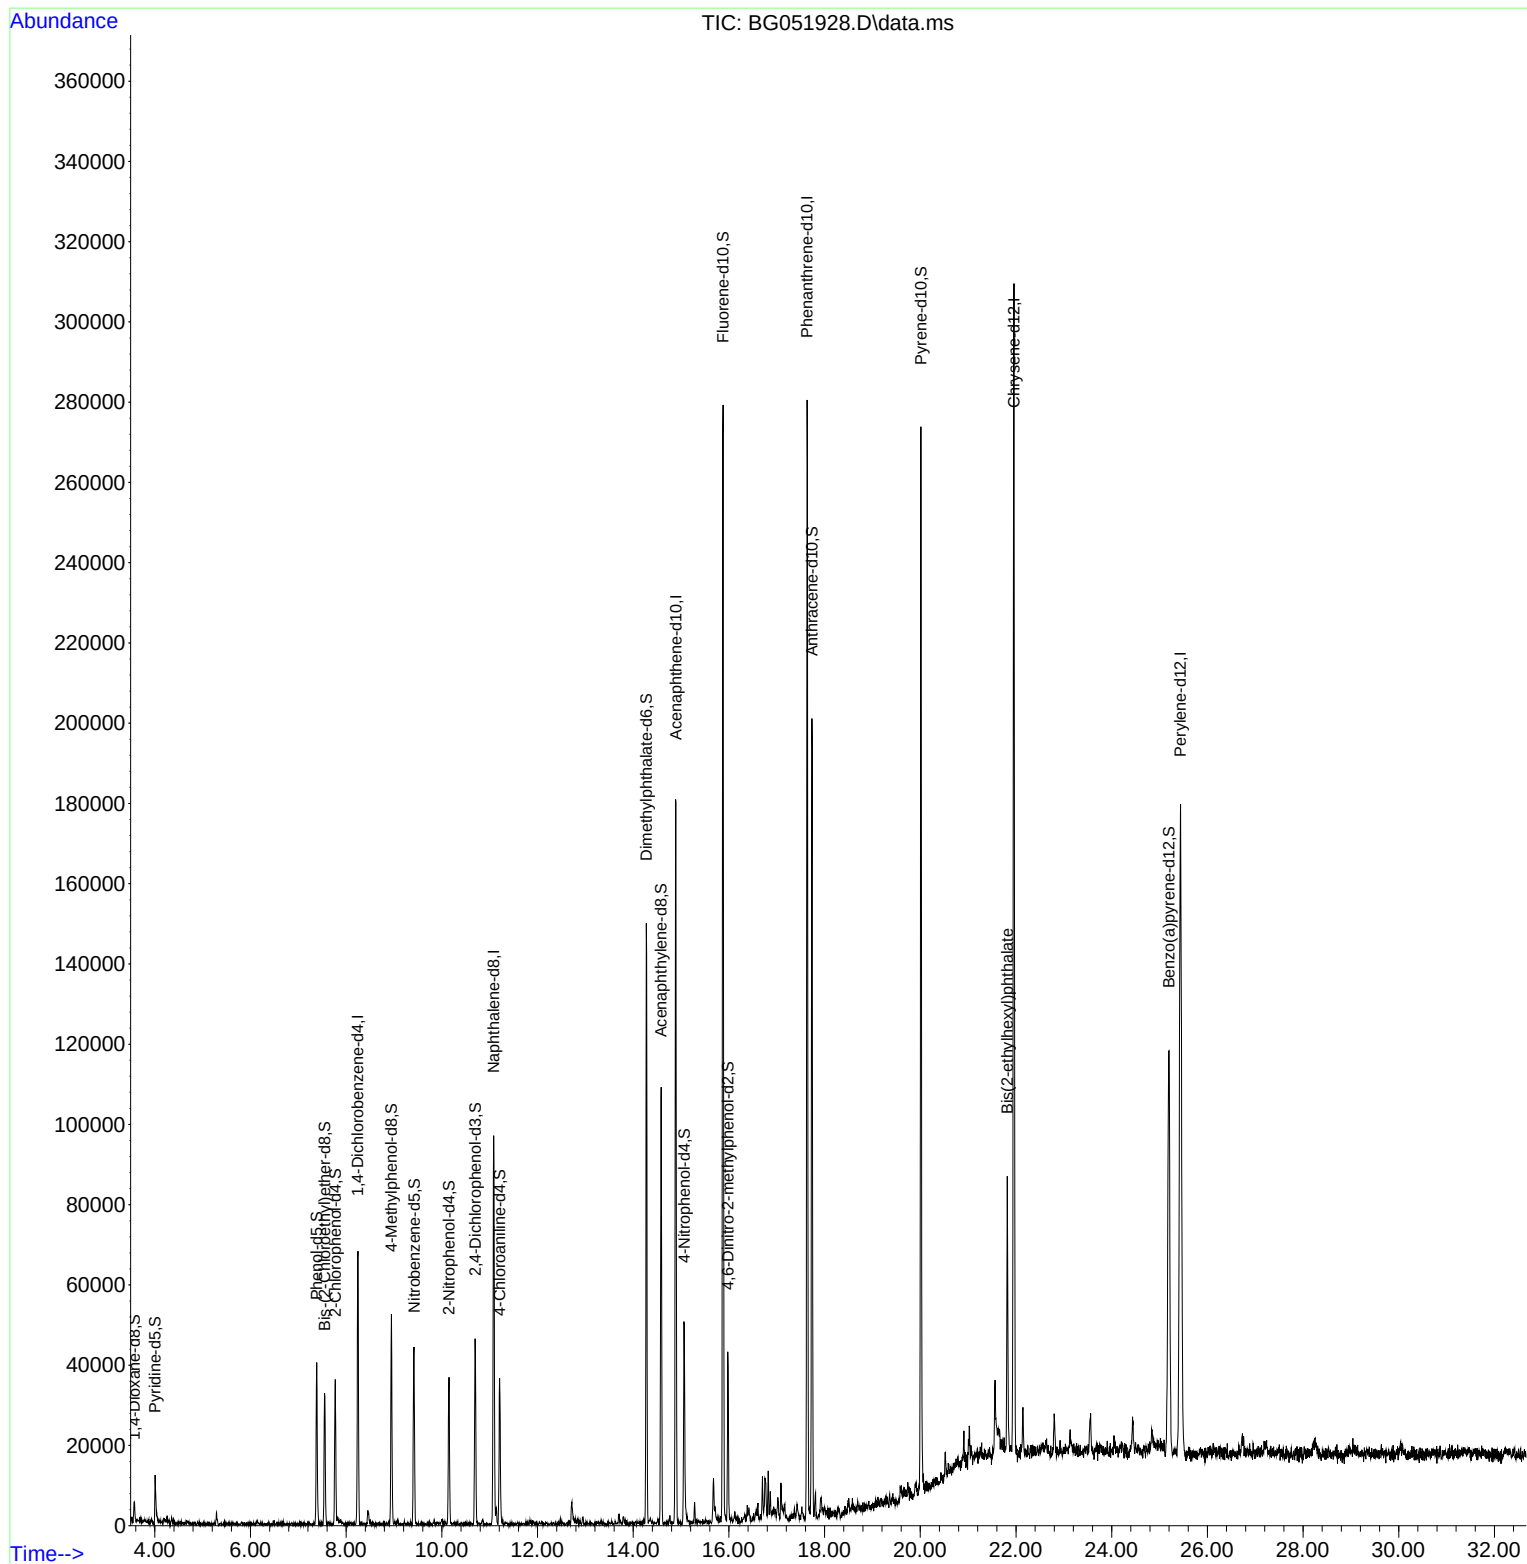

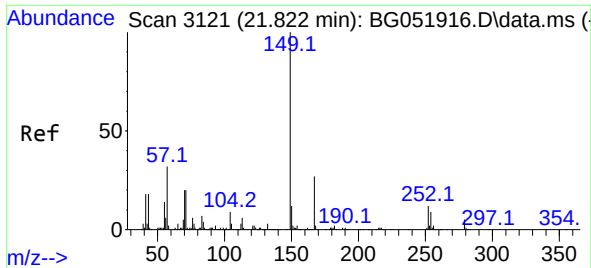

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 4.565 ng/ul
 RT: 21.816 min Scan# 31
 Delta R.T. -0.001 min
 Lab File: BG051928.D
 Acq: 7 Jan 2022 23:28

Instrument :
 BNA_G
 ClientSampleId :
 BGLG9

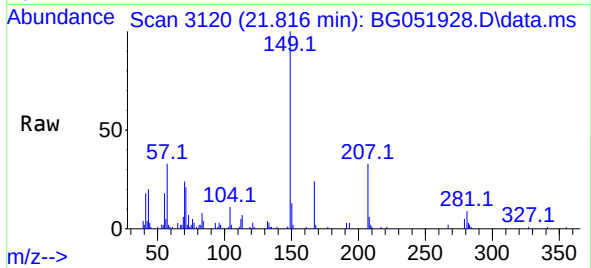

Tgt Ion:149 Resp: 28930
 Ion Ratio Lower Upper
 149 100
 167 23.8 21.1 31.7
 279 4.8 2.7 4.1#

