

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051893.D
 Acq On : 6 Jan 2022 15:01
 Operator : CG/JU
 Sample : PB141855BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK855

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.576	10	15	22	rVB3	10816	18278	1.71%	0.179%
2	3.929	70	75	78	rBV3	900	1275	0.12%	0.012%
3	3.999	83	87	108	rVV	118316	199863	18.66%	1.953%
4	4.363	145	149	155	rVV4	1720	2902	0.27%	0.028%
5	4.493	168	171	174	rBV3	1011	1262	0.12%	0.012%
6	5.292	304	307	311	rVB3	815	1355	0.13%	0.013%
7	5.380	319	322	326	rBV	952	1314	0.12%	0.013%
8	5.527	345	347	350	rVB2	1095	1143	0.11%	0.011%
9	6.278	471	475	479	rBV	768	1477	0.14%	0.014%
10	7.389	656	664	673	rBV	148422	253855	23.70%	2.480%
11	7.559	686	693	703	rVV	106905	178766	16.69%	1.747%
12	7.635	703	706	709	rVB	1093	1081	0.10%	0.011%
13	7.776	724	730	739	rBV	139560	233820	21.83%	2.285%
14	8.252	805	811	820	rVB	100855	169832	15.85%	1.659%
15	8.951	924	930	939	rBV	173800	296052	27.64%	2.893%
16	9.010	939	940	944	rVB	979	1085	0.10%	0.011%
17	9.421	1004	1010	1017	rVB	146561	252063	23.53%	2.463%
18	10.156	1127	1135	1144	rBV2	123373	216410	20.20%	2.114%
19	10.702	1221	1228	1239	rVB2	174268	298657	27.88%	2.918%
20	11.090	1286	1294	1303	rVB	138921	250275	23.36%	2.445%
21	11.213	1308	1315	1325	rBV	166671	303277	28.31%	2.963%
22	12.670	1557	1563	1569	rVB3	2809	4591	0.43%	0.045%
23	14.285	1829	1838	1844	rBV	364228	531246	49.59%	5.190%
24	14.591	1883	1890	1898	rBV	364094	579303	54.08%	5.660%
25	14.896	1935	1942	1949	rVB	233011	373552	34.87%	3.650%
26	15.067	1964	1971	1983	rBV	176815	282416	26.36%	2.759%
27	15.883	2103	2110	2116	rBV	494201	731296	68.26%	7.145%
28	15.983	2120	2127	2135	rBV	172379	256200	23.92%	2.503%
29	16.118	2148	2150	2154	rVB2	2107	2239	0.21%	0.022%
30	16.488	2212	2213	2216	rBV2	1050	1188	0.11%	0.012%
31	16.688	2244	2247	2250	rBV2	851	1087	0.10%	0.011%
32	17.422	2370	2372	2378	rVB3	1129	1782	0.17%	0.017%
33	17.640	2402	2409	2418	rBV	337625	509683	47.58%	4.980%
34	17.739	2419	2426	2433	rBV2	575048	852827	79.61%	8.332%
35	18.015	2470	2473	2480	rVB3	1670	2830	0.26%	0.028%
36	18.086	2480	2485	2487	rBV	1123	1882	0.18%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051893.D
 Acq On : 6 Jan 2022 15:01
 Operator : CG/JU
 Sample : PB141855BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK855

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	18.286	2517	2519	2523	rBV2	1167	1343	0.13%	0.013%
38	18.656	2577	2582	2585	rBV2	1278	2100	0.20%	0.021%
39	18.703	2589	2590	2593	rBV3	1231	1429	0.13%	0.014%
40	18.991	2636	2639	2640	rBV2	1159	1136	0.11%	0.011%

41	19.208	2675	2676	2679	rBV3	1394	1154	0.11%	0.011%
42	19.302	2688	2692	2695	rBV5	2219	2240	0.21%	0.022%
43	19.337	2695	2698	2700	rBV2	1330	1833	0.17%	0.018%
44	19.361	2700	2702	2707	rBV3	1077	2122	0.20%	0.021%
45	19.496	2721	2725	2727	rBV4	1327	1371	0.13%	0.013%

46	19.584	2737	2740	2744	rBV5	8053	11248	1.05%	0.110%
47	19.654	2747	2752	2756	rBV3	7929	10415	0.97%	0.102%
48	19.737	2760	2766	2768	rBV5	1889	3613	0.34%	0.035%
49	19.825	2780	2781	2784	rBV3	1524	1792	0.17%	0.018%
50	20.019	2808	2814	2823	rVV	782213	1071280	100.00%	10.467%

51	20.083	2823	2825	2826	rVB2	2180	1123	0.10%	0.011%
52	20.195	2842	2844	2847	rVB4	1981	1368	0.13%	0.013%
53	20.295	2859	2861	2862	rBV2	2082	1186	0.11%	0.012%
54	20.377	2874	2875	2878	rBV3	3303	2184	0.20%	0.021%
55	20.688	2925	2928	2929	rBV2	3717	3283	0.31%	0.032%

56	20.788	2943	2945	2947	rBV2	3103	3131	0.29%	0.031%
57	20.959	2973	2974	2975	rVB	4377	1543	0.14%	0.015%
58	20.988	2977	2979	2982	rVB3	2986	2365	0.22%	0.023%
59	21.734	3104	3106	3107	rBV2	3522	2741	0.26%	0.027%
60	21.957	3138	3144	3153	rVB2	335681	592431	55.30%	5.788%

61	24.448	3564	3568	3575	rVB7	8793	20647	1.93%	0.202%
62	24.524	3580	3581	3582	rBV	3230	1160	0.11%	0.011%
63	25.047	3668	3670	3671	rBV2	3958	3001	0.28%	0.029%
64	25.212	3687	3698	3709	rVB2	361794	1019386	95.16%	9.960%
65	25.447	3728	3738	3756	rVB	186363	592540	55.31%	5.789%

66	26.580	3929	3931	3932	rBV2	3686	1857	0.17%	0.018%
67	26.739	3955	3958	3959	rBV3	5961	6029	0.56%	0.059%
68	26.856	3976	3978	3979	rBV2	4571	3076	0.29%	0.030%
69	27.814	4137	4141	4143	rBV5	3629	5047	0.47%	0.049%
70	28.243	4211	4214	4216	rBV4	6418	8137	0.76%	0.080%

71	28.396	4238	4240	4243	rBV4	3349	2424	0.23%	0.024%
72	28.725	4294	4296	4298	rVB3	3417	1403	0.13%	0.014%
73	29.306	4393	4395	4396	rBV2	3623	2543	0.24%	0.025%
74	29.324	4396	4398	4399	rVB2	3262	1428	0.13%	0.014%
75	29.471	4421	4423	4424	rBV	3529	2311	0.22%	0.023%

76	29.606	4444	4446	4448	rBV3	3009	2470	0.23%	0.024%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051893.D
Acq On : 6 Jan 2022 15:01
Operator : CG/JU
Sample : PB141855BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK855

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

77	29.735	4467	4468	4470	rBV2	4682	3362	0.31%	0.033%
78	30.775	4643	4645	4648	rBV4	4278	3052	0.28%	0.030%
79	31.016	4684	4686	4688	rBV2	3385	2321	0.22%	0.023%
80	31.121	4703	4704	4707	rBV3	4034	2837	0.26%	0.028%
81	32.190	4884	4886	4887	rBV2	3338	2658	0.25%	0.026%
82	32.608	4954	4957	4959	rBV3	5220	6767	0.63%	0.066%




Sum of corrected areas: 10235051

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051893.D
Acq On : 6 Jan 2022 15:01
Operator : CG/JU
Sample : PB141855BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK855

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

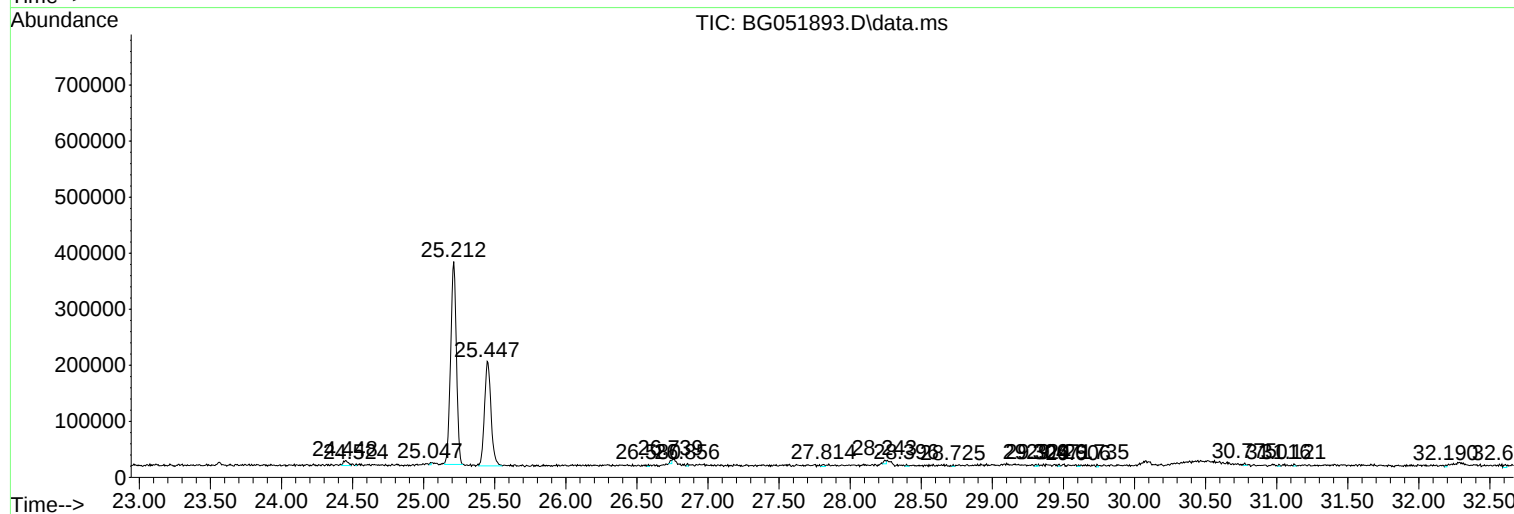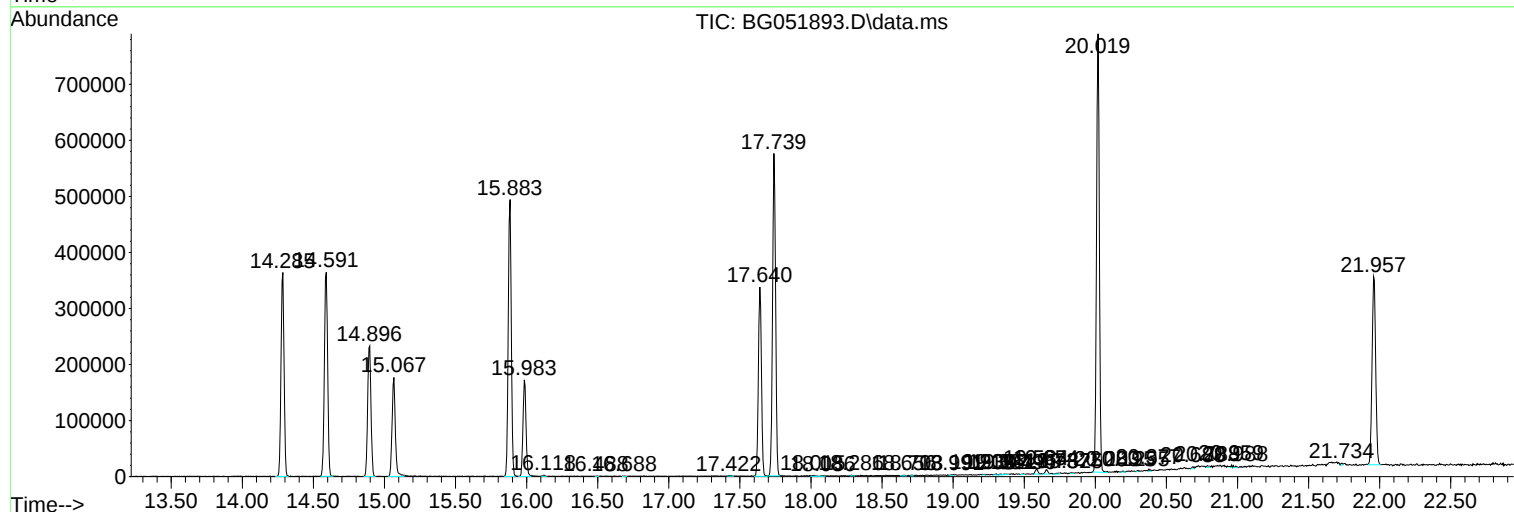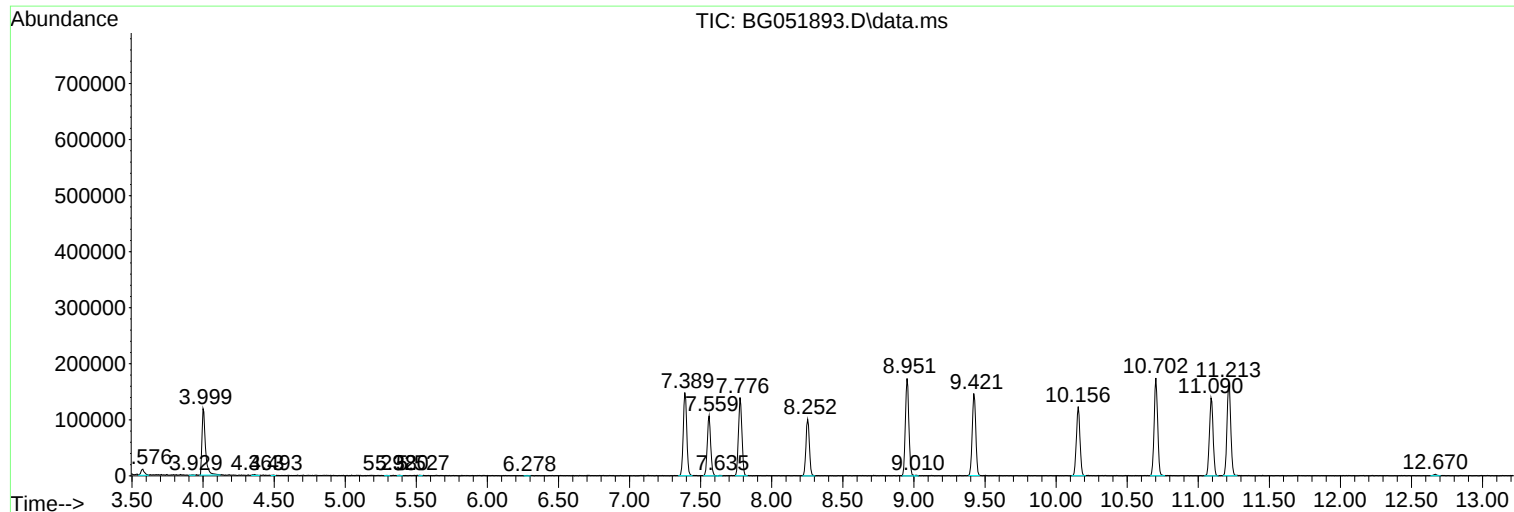

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051893.D
Acq On : 6 Jan 2022 15:01
Operator : CG/JU
Sample : PB141855BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK855

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051893.D
Acq On : 6 Jan 2022 15:01
Operator : CG/JU
Sample : PB141855BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK855

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc