

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051911.D
 Acq On : 7 Jan 2022 12:23
 Operator : CG/JU
 Sample : PB141891BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK891

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.576	11	15	22	rVB2	9316	13231	1.33%	0.145%
2	4.005	83	88	104	rBV	108871	191260	19.26%	2.096%
3	4.357	145	148	151	rVB2	1343	1684	0.17%	0.018%
4	5.996	422	427	429	rVB	596	1040	0.10%	0.011%
5	7.300	645	649	652	rBV	767	1404	0.14%	0.015%
6	7.388	657	664	672	rBV	132259	224358	22.59%	2.459%
7	7.553	681	692	701	rVB	84566	146401	14.74%	1.604%
8	7.776	723	730	739	rVB	116860	195468	19.69%	2.142%
9	8.252	804	811	817	rBV	94047	159232	16.04%	1.745%
10	8.951	923	930	939	rBV2	150793	257122	25.89%	2.818%
11	9.421	1000	1010	1018	rBV	117241	206944	20.84%	2.268%
12	10.149	1126	1134	1143	rBV	96914	175829	17.71%	1.927%
13	10.702	1220	1228	1240	rBV	151894	266669	26.86%	2.923%
14	11.089	1287	1294	1301	rVB	127358	228849	23.05%	2.508%
15	11.213	1307	1315	1325	rBV	159532	282048	28.40%	3.091%
16	12.664	1555	1562	1566	rBV2	1971	3469	0.35%	0.038%
17	14.279	1830	1837	1844	rBV	288789	426249	42.93%	4.671%
18	14.408	1856	1859	1862	rBV2	781	1270	0.13%	0.014%
19	14.585	1882	1889	1898	rVV	315337	478096	48.15%	5.240%
20	14.890	1934	1941	1949	rVB	226599	351008	35.35%	3.847%
21	15.066	1965	1971	1987	rBV2	108310	207458	20.89%	2.274%
22	15.671	2071	2074	2080	rVB2	724	1156	0.12%	0.013%
23	15.877	2103	2109	2118	rVB	398428	610793	61.51%	6.694%
24	15.983	2122	2127	2137	rVV	47515	67785	6.83%	0.743%
25	16.112	2145	2149	2154	rBV3	1101	2054	0.21%	0.023%
26	16.411	2196	2200	2202	rBV	637	995	0.10%	0.011%
27	17.410	2368	2370	2373	rBV2	1402	1888	0.19%	0.021%
28	17.639	2397	2409	2415	rBV	323643	493450	49.69%	5.408%
29	17.739	2419	2426	2433	rVV	511565	779079	78.46%	8.538%
30	18.332	2523	2527	2531	rBV3	890	1548	0.16%	0.017%
31	18.450	2543	2547	2548	rVB3	1265	1127	0.11%	0.012%
32	18.473	2548	2551	2553	rBV2	1395	1241	0.12%	0.014%
33	18.550	2560	2564	2567	rBV2	849	1142	0.12%	0.013%
34	18.685	2586	2587	2592	rVV2	874	1395	0.14%	0.015%
35	18.767	2596	2601	2602	rVB3	1331	1716	0.17%	0.019%
36	18.896	2620	2623	2624	rBV3	1133	997	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051911.D
 Acq On : 7 Jan 2022 12:23
 Operator : CG/JU
 Sample : PB141891BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK891

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	18.949	2631	2632	2635	rBV3	1487	1308	0.13%	0.014%
38	19.155	2664	2667	2669	rVB2	1661	1276	0.13%	0.014%
39	19.319	2694	2695	2697	rVB	1579	1101	0.11%	0.012%
40	19.337	2697	2698	2702	rBV3	1467	1801	0.18%	0.020%

41	19.431	2712	2714	2717	rVB4	1191	1094	0.11%	0.012%
42	19.584	2736	2740	2745	rVV2	7469	9991	1.01%	0.109%
43	19.648	2749	2751	2757	rVB4	5464	8672	0.87%	0.095%
44	19.801	2775	2777	2778	rBV2	1539	1010	0.10%	0.011%
45	19.854	2783	2786	2787	rVV3	1410	1488	0.15%	0.016%

46	19.918	2795	2797	2800	rVB3	1749	1583	0.16%	0.017%
47	20.012	2807	2813	2820	rBV	677033	992975	100.00%	10.882%
48	20.101	2826	2828	2829	rBV2	2574	1905	0.19%	0.021%
49	20.118	2829	2831	2833	rVB3	2984	1692	0.17%	0.019%
50	20.136	2833	2834	2837	rBV3	1724	1605	0.16%	0.018%

51	20.165	2837	2839	2841	rBV3	2802	1862	0.19%	0.020%
52	20.324	2863	2866	2869	rBV5	1863	2476	0.25%	0.027%
53	20.371	2873	2874	2876	rBV2	2345	1768	0.18%	0.019%
54	20.471	2889	2891	2892	rBV2	1952	1669	0.17%	0.018%
55	20.541	2901	2903	2905	rBV3	2309	2313	0.23%	0.025%

56	20.676	2925	2926	2928	rBV2	3585	2873	0.29%	0.031%
57	20.712	2930	2932	2933	rVB2	3347	1624	0.16%	0.018%
58	20.835	2951	2953	2954	rBV2	2312	1309	0.13%	0.014%
59	21.217	3015	3018	3020	rBV4	3331	3800	0.38%	0.042%
60	21.369	3042	3044	3046	rVB3	2698	1482	0.15%	0.016%

61	21.957	3137	3144	3151	rBV2	348532	581211	58.53%	6.370%
62	22.145	3174	3176	3177	rBV2	4197	3699	0.37%	0.041%
63	22.926	3307	3309	3312	rBV4	3382	2938	0.30%	0.032%
64	23.296	3370	3372	3376	rBV4	4509	6177	0.62%	0.068%
65	23.349	3379	3381	3382	rVB	3714	2019	0.20%	0.022%

66	23.384	3386	3387	3390	rBV3	3751	2947	0.30%	0.032%
67	23.502	3404	3407	3409	rBV4	3439	4319	0.43%	0.047%
68	23.555	3414	3416	3423	rVB8	8514	14202	1.43%	0.156%
69	24.219	3528	3529	3533	rVB3	5020	3948	0.40%	0.043%
70	24.430	3560	3565	3566	rBV5	12381	13120	1.32%	0.144%

71	25.012	3663	3664	3665	rBV	3929	1642	0.17%	0.018%
72	25.205	3686	3697	3710	rVB2	331027	932110	93.87%	10.215%
73	25.440	3727	3737	3755	rVB2	185410	605705	61.00%	6.638%
74	25.711	3781	3783	3784	rBV	2975	1450	0.15%	0.016%
75	25.987	3828	3830	3832	rBV3	3293	3032	0.31%	0.033%

76	26.539	3922	3924	3928	rBV4	3201	4436	0.45%	0.049%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051911.D
 Acq On : 7 Jan 2022 12:23
 Operator : CG/JU
 Sample : PB141891BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK891

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	26.586	3931	3932	3935	rVB3	6412	4009	0.40%	0.044%
78	26.739	3954	3958	3959	rBV4	8467	10560	1.06%	0.116%
79	27.138	4024	4026	4028	rBV3	2995	2194	0.22%	0.024%
80	27.408	4071	4072	4073	rVB	3254	1147	0.12%	0.013%
81	28.242	4206	4214	4223	rBV8	12263	42519	4.28%	0.466%
82	28.754	4299	4301	4303	rBV2	3682	3374	0.34%	0.037%
83	29.940	4501	4503	4506	rBV3	3240	2048	0.21%	0.022%
84	30.028	4515	4518	4519	rBV3	5144	5182	0.52%	0.057%
85	30.469	4591	4593	4594	rVB2	3178	2092	0.21%	0.023%
86	30.657	4623	4625	4626	rBV2	3819	2986	0.30%	0.033%
87	30.886	4662	4664	4665	rBV2	3166	2620	0.26%	0.029%
88	31.197	4716	4717	4719	rVV2	4211	1819	0.18%	0.020%
89	31.215	4719	4720	4723	rVB3	3506	2802	0.28%	0.031%
90	31.990	4850	4852	4853	rBV2	3486	2235	0.23%	0.024%
91	32.143	4876	4878	4879	rBV2	2777	1124	0.11%	0.012%
92	32.255	4894	4897	4899	rBV3	5428	7246	0.73%	0.079%
93	32.443	4927	4929	4930	rBV2	3622	2163	0.22%	0.024%
94	32.525	4940	4943	4947	rBV6	4790	7534	0.76%	0.083%
95	32.554	4947	4948	4951	rBV3	4029	3783	0.38%	0.041%




Sum of corrected areas: 9124524

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051911.D
Acq On : 7 Jan 2022 12:23
Operator : CG/JU
Sample : PB141891BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK891

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

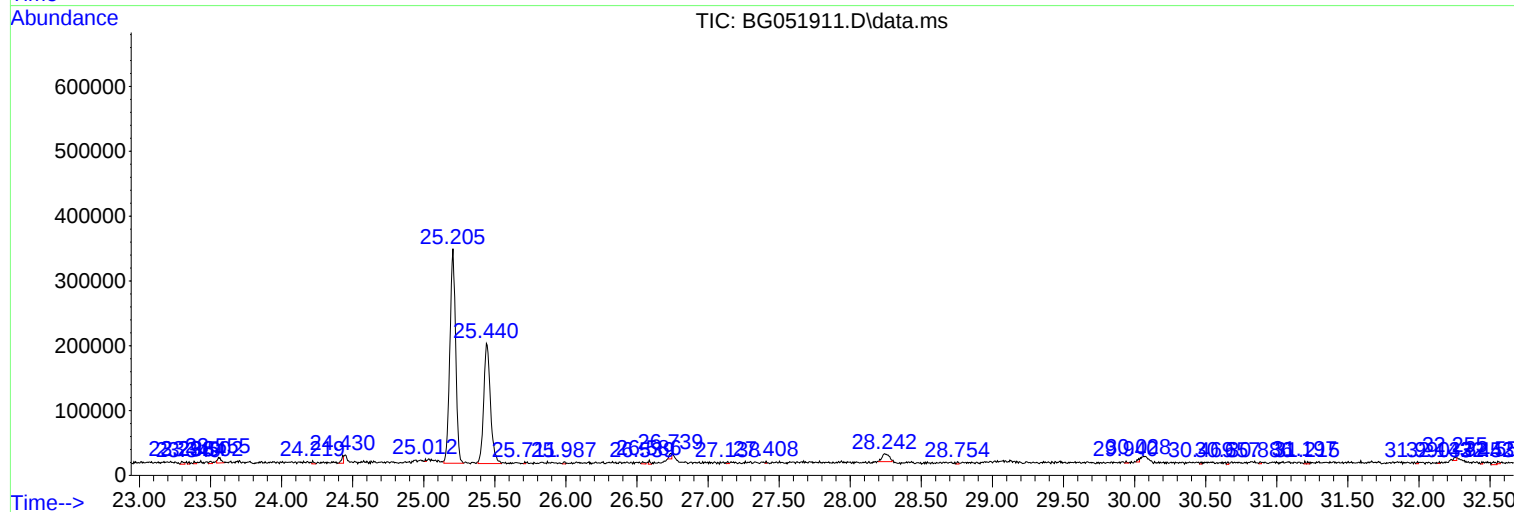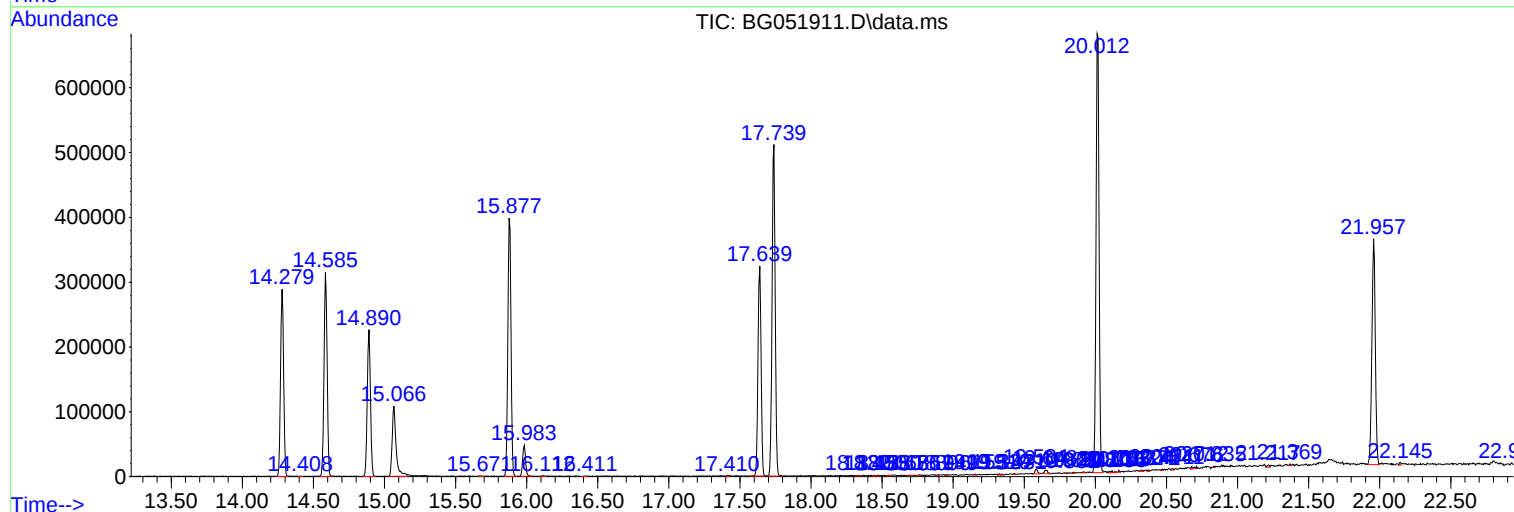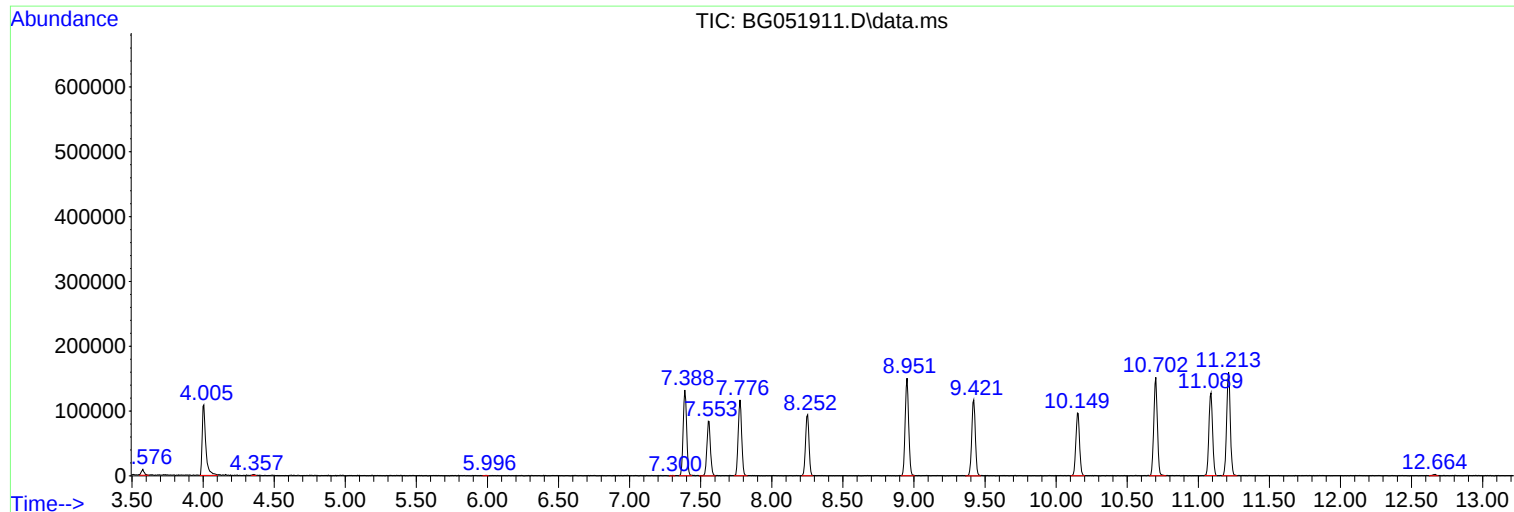

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051911.D
Acq On : 7 Jan 2022 12:23
Operator : CG/JU
Sample : PB141891BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK891

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051911.D
Acq On : 7 Jan 2022 12:23
Operator : CG/JU
Sample : PB141891BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK891

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc