

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051913.D
 Acq On : 7 Jan 2022 13:38
 Operator : CG/JU
 Sample : N1027-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0J16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051913.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.576	6	15	21	rBV5	11667	25434	2.39%	0.306%
2	3.617	21	22	27	rBV4	1578	1804	0.17%	0.022%
3	3.675	27	32	35	rVV2	723	1146	0.11%	0.014%
4	4.010	85	89	103	rBV	24216	42910	4.04%	0.516%
5	4.251	125	130	134	rBV3	3172	4654	0.44%	0.056%
6	4.357	143	148	151	rBV3	1610	2673	0.25%	0.032%
7	4.803	222	224	229	rBV2	827	1484	0.14%	0.018%
8	7.247	635	640	643	rVB	789	1227	0.12%	0.015%
9	7.382	658	663	671	rVB3	25434	44714	4.21%	0.537%
10	7.553	683	692	701	rBV	84566	144229	13.57%	1.733%
11	7.776	723	730	737	rVV	87159	150743	14.18%	1.811%
12	8.246	804	810	818	rBB	79536	133511	12.56%	1.604%
13	8.951	923	930	937	rVB3	69667	122339	11.51%	1.470%
14	9.415	1001	1009	1017	rBV	119174	210417	19.80%	2.528%
15	9.844	1078	1082	1084	rBV3	1577	2130	0.20%	0.026%
16	10.149	1128	1134	1142	rVB2	97678	168452	15.85%	2.024%
17	10.537	1196	1200	1205	rVB	589	1340	0.13%	0.016%
18	10.701	1220	1228	1241	rBV	135638	250678	23.59%	3.012%
19	11.089	1285	1294	1301	rBV	105985	194829	18.33%	2.341%
20	11.212	1307	1315	1324	rBV	135734	248644	23.40%	2.987%
21	12.340	1503	1507	1513	rVB2	2685	4098	0.39%	0.049%
22	12.663	1557	1562	1570	rBV3	2412	3940	0.37%	0.047%
23	14.279	1831	1837	1843	rBV	317310	459598	43.25%	5.522%
24	14.584	1883	1889	1896	rVB	312220	500264	47.07%	6.011%
25	14.890	1934	1941	1948	rBV	196879	294157	27.68%	3.534%
26	15.072	1966	1972	1983	rBV3	18800	35840	3.37%	0.431%
27	15.683	2071	2076	2082	rVB2	830	1904	0.18%	0.023%
28	15.877	2101	2109	2117	rVB	426446	669902	63.04%	8.049%
29	15.982	2121	2127	2133	rBV2	89398	126919	11.94%	1.525%
30	16.117	2144	2150	2154	rVB4	1601	2271	0.21%	0.027%
31	16.975	2293	2296	2300	rBV	868	1233	0.12%	0.015%
32	17.639	2403	2409	2419	rBV	283250	422955	39.80%	5.082%
33	17.739	2419	2426	2434	rVB	545013	831057	78.20%	9.985%
34	18.291	2516	2520	2522	rVV	1205	1142	0.11%	0.014%
35	18.579	2568	2569	2574	rVV4	980	1265	0.12%	0.015%
36	18.767	2598	2601	2605	rVB4	1084	1528	0.14%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051913.D
 Acq On : 7 Jan 2022 13:38
 Operator : CG/JU
 Sample : N1027-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0J16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	19.090	2655	2656	2660	rBV3	961	1424	0.13%	0.017%
38	19.342	2697	2699	2701	rBV2	1545	1169	0.11%	0.014%
39	19.372	2701	2704	2705	rBV3	902	1093	0.10%	0.013%
40	19.466	2715	2720	2721	rBV3	1102	2015	0.19%	0.024%

41	19.489	2723	2724	2727	rVV3	1799	1600	0.15%	0.019%
42	19.536	2730	2732	2735	rBV3	1857	1539	0.14%	0.018%
43	19.583	2735	2740	2744	rBV5	8356	11276	1.06%	0.135%
44	19.648	2747	2751	2759	rVV	6757	11676	1.10%	0.140%
45	19.718	2761	2763	2766	rBV3	1688	1262	0.12%	0.015%

46	19.807	2774	2778	2779	rBV3	1036	1257	0.12%	0.015%
47	19.912	2794	2796	2799	rVB2	1332	1256	0.12%	0.015%
48	20.018	2807	2814	2820	rBV	710285	1062738	100.00%	12.769%
49	20.177	2839	2841	2843	rBV3	2252	1143	0.11%	0.014%
50	20.271	2856	2857	2859	rBV2	1832	1289	0.12%	0.015%

51	20.335	2866	2868	2869	rBV	1661	1197	0.11%	0.014%
52	20.647	2920	2921	2923	rBV2	2277	2002	0.19%	0.024%
53	21.657	3091	3093	3097	rVB5	6017	7144	0.67%	0.086%
54	21.957	3137	3144	3151	rBV	292590	498334	46.89%	5.987%
55	22.509	3236	3238	3241	rBV4	4195	5005	0.47%	0.060%

56	22.714	3271	3273	3274	rBV2	3087	1460	0.14%	0.018%
57	23.554	3414	3416	3422	rVB6	7678	11214	1.06%	0.135%
58	24.036	3495	3498	3499	rBV3	3505	3845	0.36%	0.046%
59	24.159	3517	3519	3521	rVB3	4777	3450	0.32%	0.041%
60	24.206	3525	3527	3528	rVV	3053	1417	0.13%	0.017%

61	24.306	3542	3544	3547	rBV3	2618	2093	0.20%	0.025%
62	24.624	3596	3598	3599	rBV2	3399	1905	0.18%	0.023%
63	24.829	3631	3633	3635	rBV2	3271	2424	0.23%	0.029%
64	25.205	3685	3697	3709	rVB2	353786	1008798	94.92%	12.121%
65	25.452	3728	3739	3753	rVB3	155864	505251	47.54%	6.071%

66	26.033	3836	3838	3842	rBB5	2962	2146	0.20%	0.026%
67	26.274	3877	3879	3880	rBV2	3010	1892	0.18%	0.023%
68	26.580	3929	3931	3934	rBV4	3304	3295	0.31%	0.040%
69	26.920	3987	3989	3990	rVB2	3562	1550	0.15%	0.019%
70	26.991	3999	4001	4002	rBV2	2813	1837	0.17%	0.022%

71	27.197	4035	4036	4039	rBV4	2637	2530	0.24%	0.030%
72	27.320	4055	4057	4059	rVB3	3877	2208	0.21%	0.027%
73	27.590	4102	4103	4104	rVB	3424	1207	0.11%	0.015%
74	28.219	4207	4210	4211	rBV3	5965	5824	0.55%	0.070%
75	28.401	4238	4241	4243	rBV4	3106	3760	0.35%	0.045%

76	29.276	4388	4390	4391	rVB2	3153	1504	0.14%	0.018%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051913.D
 Acq On : 7 Jan 2022 13:38
 Operator : CG/JU
 Sample : N1027-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0J16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	29.576	4439	4441	4442	rBV2	2664	1385	0.13%	0.017%
78	29.617	4446	4448	4449	rBV2	2647	1633	0.15%	0.020%
79	29.681	4457	4459	4461	rVB3	3015	1475	0.14%	0.018%
80	30.263	4556	4558	4559	rVB	3672	2014	0.19%	0.024%
81	30.281	4559	4561	4563	rBV3	2477	1564	0.15%	0.019%
82	30.809	4649	4651	4652	rBV2	2735	1781	0.17%	0.021%
83	30.880	4661	4663	4664	rBV2	3206	1832	0.17%	0.022%
84	31.285	4730	4732	4734	rBV	3524	2924	0.28%	0.035%
85	31.767	4813	4814	4815	rBV	3803	2029	0.19%	0.024%
86	32.284	4900	4902	4906	rVB5	4326	4777	0.45%	0.057%
87	32.560	4947	4949	4952	rBV3	3932	6154	0.58%	0.074%




Sum of corrected areas: 8323028

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051913.D
Acq On : 7 Jan 2022 13:38
Operator : CG/JU
Sample : N1027-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0J16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

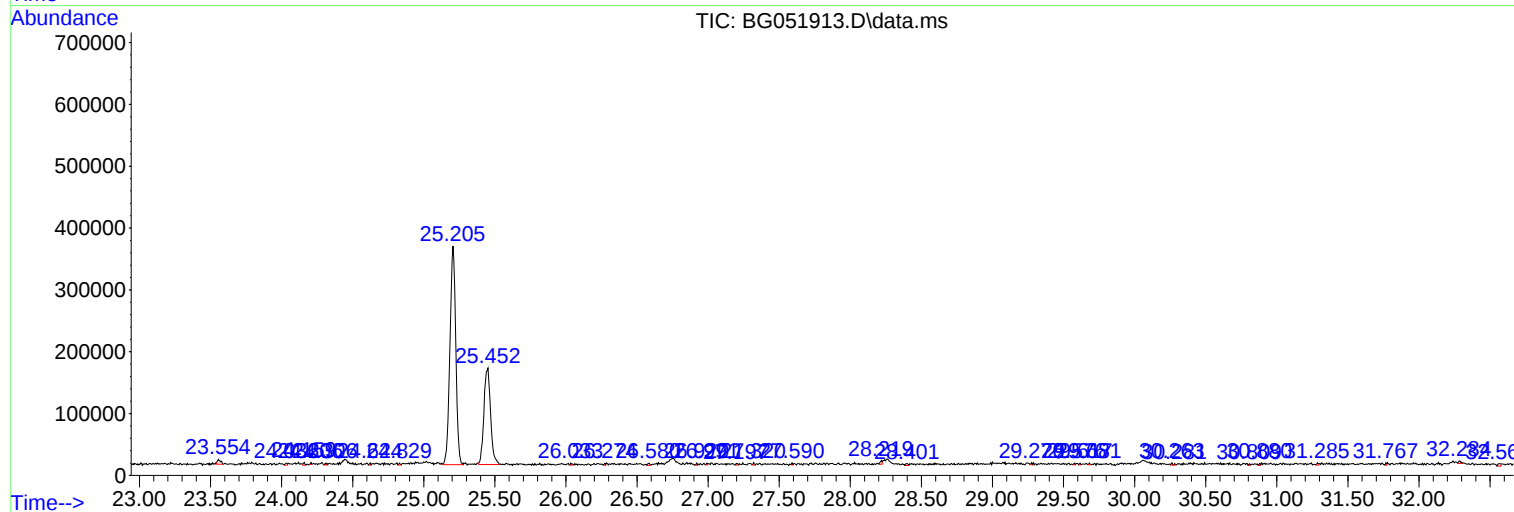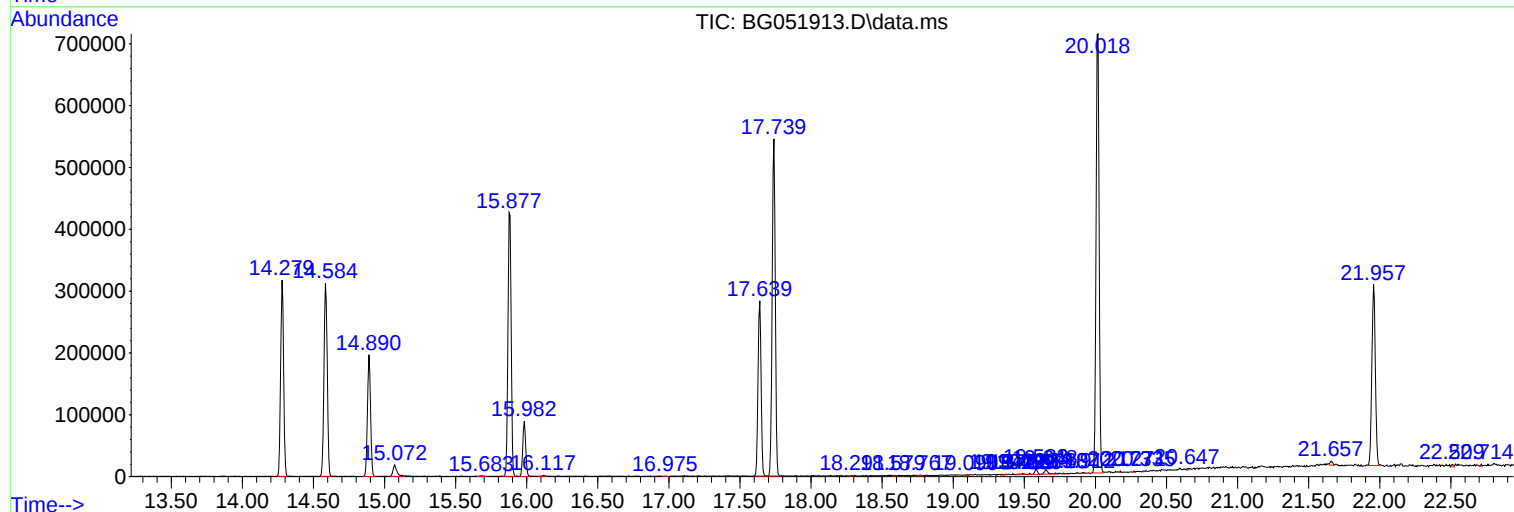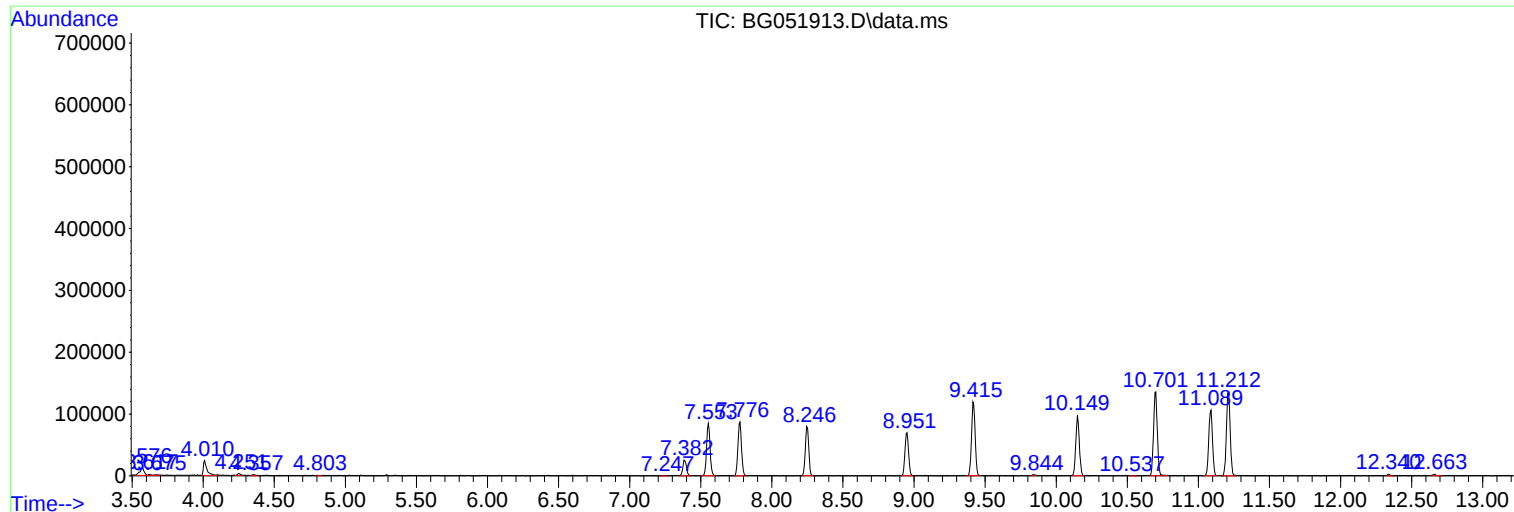

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051913.D
Acq On : 7 Jan 2022 13:38
Operator : CG/JU
Sample : N1027-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0J16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051913.D
Acq On : 7 Jan 2022 13:38
Operator : CG/JU
Sample : N1027-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0J16

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------