

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051917.D
 Acq On : 7 Jan 2022 16:20
 Operator : CG/JU
 Sample : PB141891BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK891

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.576	9	15	23	rVB2	8464	14834	1.44%	0.154%
2	3.870	62	65	69	rVB3	1117	1265	0.12%	0.013%
3	3.929	71	75	78	rVB3	1244	2062	0.20%	0.021%
4	3.999	83	87	103	rBV	110703	195532	19.02%	2.026%
5	4.099	103	104	107	rVB	1395	1140	0.11%	0.012%
6	4.252	128	130	134	rBV2	1218	1442	0.14%	0.015%
7	4.358	141	148	154	rVB4	4469	7627	0.74%	0.079%
8	4.716	205	209	210	rBV4	1152	1096	0.11%	0.011%
9	5.979	422	424	428	rBV	1033	1209	0.12%	0.013%
10	6.725	548	551	554	rBV	983	1170	0.11%	0.012%
11	7.389	655	664	671	rBV	140034	239584	23.31%	2.483%
12	7.553	685	692	703	rVB	95690	162132	15.77%	1.680%
13	7.777	722	730	738	rBV	128077	218745	21.28%	2.267%
14	8.041	771	775	778	rBV2	692	1120	0.11%	0.012%
15	8.252	803	811	818	rBV	96498	162747	15.83%	1.687%
16	8.634	874	876	880	rVV2	897	1145	0.11%	0.012%
17	8.951	923	930	938	rBV	158038	273781	26.63%	2.837%
18	9.421	1001	1010	1017	rBV	123703	230854	22.46%	2.392%
19	9.721	1058	1061	1063	rBV	819	1055	0.10%	0.011%
20	10.150	1127	1134	1141	rBV	111194	198620	19.32%	2.058%
21	10.696	1221	1227	1236	rBV	156738	276531	26.90%	2.866%
22	11.090	1286	1294	1301	rBV	124377	229907	22.37%	2.383%
23	11.213	1308	1315	1323	rBV	158173	288545	28.07%	2.990%
24	11.307	1328	1331	1334	rVB2	952	1109	0.11%	0.011%
25	12.006	1448	1450	1455	rVB2	731	1132	0.11%	0.012%
26	12.658	1556	1561	1567	rBV2	2733	4296	0.42%	0.045%
27	14.280	1830	1837	1846	rBV	356263	501430	48.78%	5.196%
28	14.585	1882	1889	1896	rBV	342448	536445	52.19%	5.559%
29	14.890	1934	1941	1947	rVV	226086	344657	33.53%	3.572%
30	15.067	1962	1971	1987	rBV2	170088	288056	28.02%	2.985%
31	15.877	2103	2109	2117	rVB	473942	695347	67.64%	7.206%
32	15.983	2121	2127	2136	rBV	174925	254997	24.81%	2.643%
33	16.083	2141	2144	2147	rVB	831	1051	0.10%	0.011%
34	16.118	2147	2150	2151	rBV	1055	1295	0.13%	0.013%
35	16.206	2162	2165	2168	rVB2	849	1085	0.11%	0.011%
36	16.418	2198	2201	2203	rBV2	1049	1076	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051917.D
 Acq On : 7 Jan 2022 16:20
 Operator : CG/JU
 Sample : PB141891BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK891

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	17.422	2367	2372	2373	rBV	1915	1778	0.17%	0.018%
38	17.640	2402	2409	2415	rBV	327481	490042	47.67%	5.078%
39	17.734	2419	2425	2434	rVB	546209	854060	83.08%	8.851%
40	17.892	2449	2452	2453	rBV2	1195	1041	0.10%	0.011%
41	18.157	2496	2497	2500	rVB	1621	1250	0.12%	0.013%
42	18.533	2557	2561	2564	rBV3	1301	2116	0.21%	0.022%
43	18.662	2580	2583	2585	rVB4	1108	1237	0.12%	0.013%
44	18.685	2585	2587	2590	rVB2	1553	1387	0.13%	0.014%
45	18.773	2599	2602	2605	rVB2	1113	1337	0.13%	0.014%
46	18.897	2620	2623	2626	rBV4	1629	1558	0.15%	0.016%
47	18.967	2633	2635	2638	rVB2	1530	1391	0.14%	0.014%
48	19.138	2663	2664	2669	rBV2	1204	1547	0.15%	0.016%
49	19.279	2687	2688	2692	rBV3	1472	1198	0.12%	0.012%
50	19.326	2694	2696	2700	rVB3	1618	2425	0.24%	0.025%
51	19.390	2702	2707	2709	rBV5	1596	2565	0.25%	0.027%
52	19.437	2713	2715	2717	rVV3	1721	1288	0.13%	0.013%
53	19.461	2717	2719	2720	rVB2	1965	1243	0.12%	0.013%
54	19.508	2726	2727	2730	rBV3	1499	1682	0.16%	0.017%
55	19.537	2730	2732	2733	rVV	1517	1151	0.11%	0.012%
56	19.578	2735	2739	2743	rVB5	8601	12240	1.19%	0.127%
57	19.649	2748	2751	2756	rVV2	7747	11617	1.13%	0.120%
58	19.696	2757	2759	2762	rVB4	1796	1369	0.13%	0.014%
59	19.725	2762	2764	2767	rBV4	1785	1670	0.16%	0.017%
60	19.801	2775	2777	2779	rVB3	2654	1765	0.17%	0.018%
61	19.825	2779	2781	2784	rVB3	2444	2171	0.21%	0.022%
62	19.848	2784	2785	2786	rBV	2664	1130	0.11%	0.012%
63	20.013	2805	2813	2820	rBV	704663	1027954	100.00%	10.653%
64	20.066	2820	2822	2824	rBV3	1615	1581	0.15%	0.016%
65	20.119	2829	2831	2832	rVB2	3357	1880	0.18%	0.019%
66	20.230	2848	2850	2851	rBV2	2481	1467	0.14%	0.015%
67	20.336	2866	2868	2869	rVB	3311	2056	0.20%	0.021%
68	20.360	2869	2872	2875	rBV5	4035	5853	0.57%	0.061%
69	20.512	2896	2898	2901	rBV4	2326	2279	0.22%	0.024%
70	20.612	2914	2915	2918	rVB2	3853	2135	0.21%	0.022%
71	20.882	2959	2961	2963	rBV3	3070	2258	0.22%	0.023%
72	21.141	3003	3005	3007	rBV3	3832	2929	0.28%	0.030%
73	21.652	3088	3092	3097	rBV4	13865	25033	2.44%	0.259%
74	21.899	3132	3134	3135	rBV2	3212	1925	0.19%	0.020%
75	21.957	3137	3144	3154	rVB2	312297	543039	52.83%	5.628%
76	22.797	3285	3287	3294	rVB6	9148	13900	1.35%	0.144%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051917.D
 Acq On : 7 Jan 2022 16:20
 Operator : CG/JU
 Sample : PB141891BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK891

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	23.250	3360	3364	3366	rBV5	4320	4567	0.44%	0.047%
78	24.319	3544	3546	3548	rBV3	3411	2353	0.23%	0.024%
79	24.771	3621	3623	3624	rBV2	4020	2494	0.24%	0.026%
80	25.200	3686	3696	3707	rVB3	308212	906802	88.21%	9.397%
81	25.447	3728	3738	3752	rVB2	168856	525992	51.17%	5.451%
82	25.911	3815	3817	3818	rVB2	5082	3049	0.30%	0.032%
83	26.528	3920	3922	3923	rBV2	3555	3174	0.31%	0.033%
84	27.168	4029	4031	4033	rBV3	3766	3266	0.32%	0.034%
85	27.614	4106	4107	4108	rBV	4132	1962	0.19%	0.020%
86	30.152	4537	4539	4546	rVB7	3660	4217	0.41%	0.044%
87	30.323	4566	4568	4569	rBV2	3350	2042	0.20%	0.021%
88	30.417	4582	4584	4586	rVB4	5208	3912	0.38%	0.041%
89	31.157	4709	4710	4712	rBV2	4026	1899	0.18%	0.020%
90	32.384	4917	4919	4920	rBV	4275	3295	0.32%	0.034%




Sum of corrected areas: 9649690

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051917.D
Acq On : 7 Jan 2022 16:20
Operator : CG/JU
Sample : PB141891BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK891

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

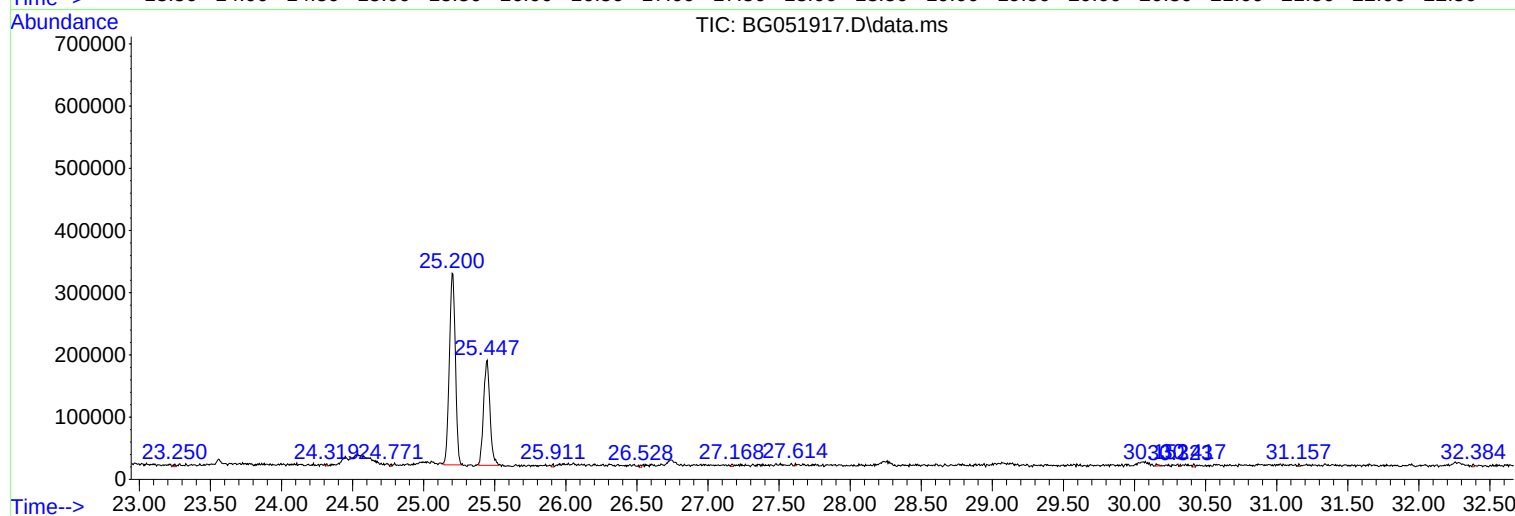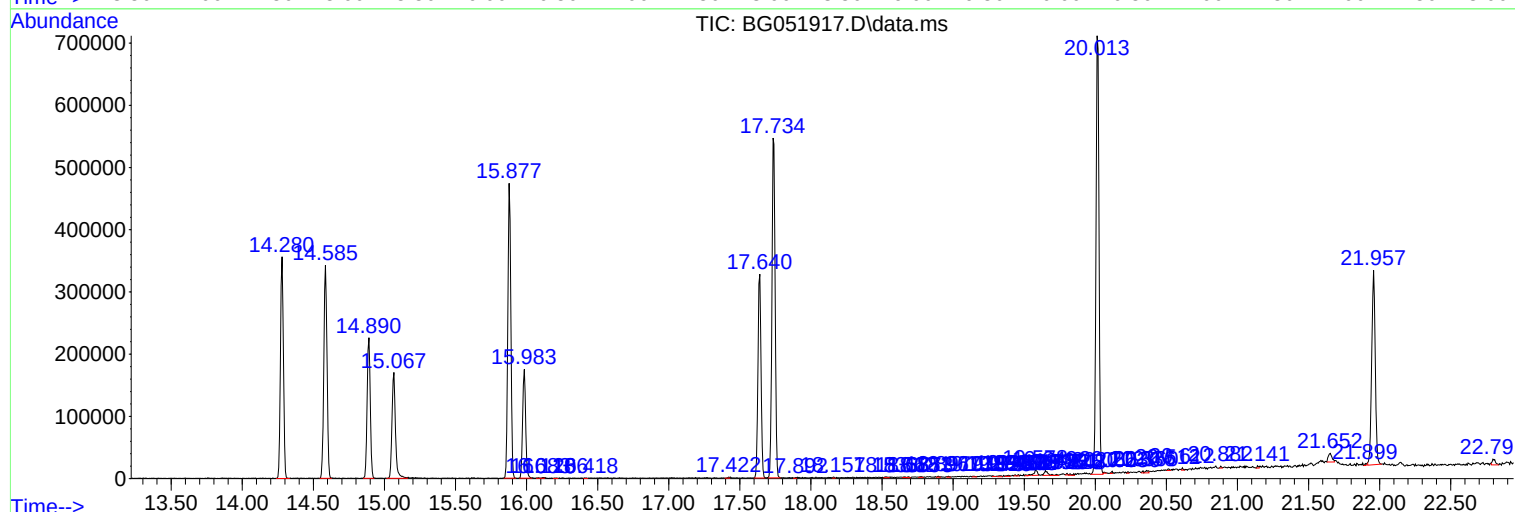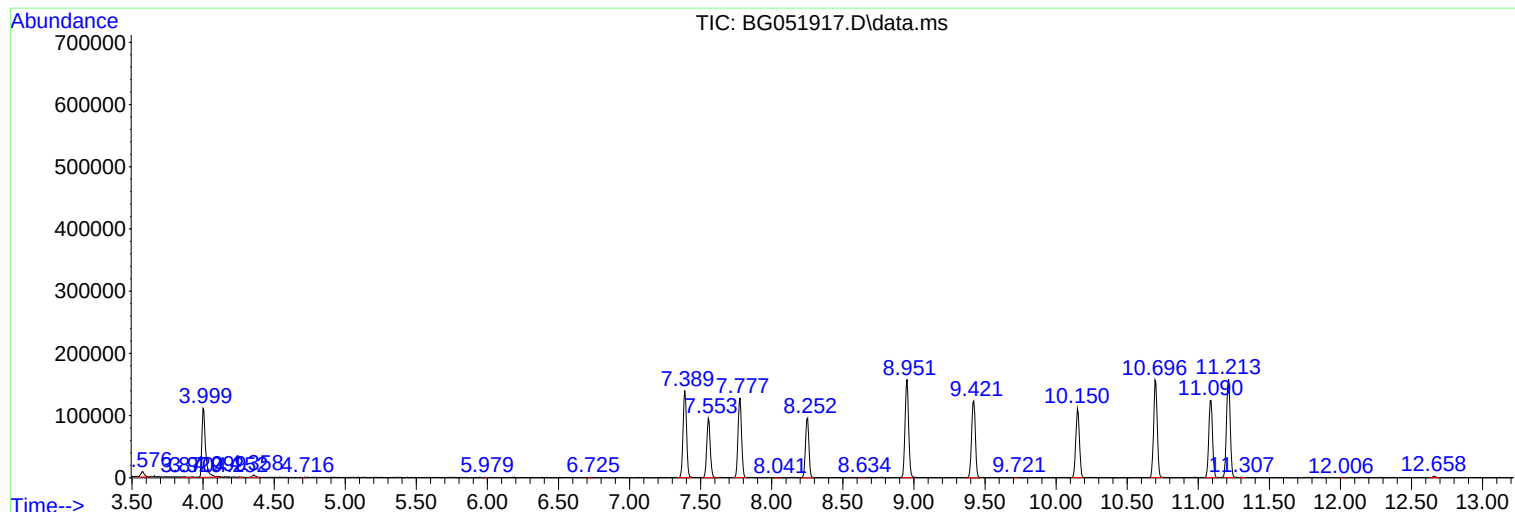

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051917.D
Acq On : 7 Jan 2022 16:20
Operator : CG/JU
Sample : PB141891BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK891

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051917.D
Acq On : 7 Jan 2022 16:20
Operator : CG/JU
Sample : PB141891BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK891

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc