

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051925.D
 Acq On : 7 Jan 2022 21:36
 Operator : CG/JU
 Sample : PB141907BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK907

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.572	8	14	23	rVB4	7655	13130	1.34%	0.152%
2	3.713	35	38	43	rVB2	1051	1815	0.18%	0.021%
3	3.837	57	59	61	rBV2	1281	1223	0.12%	0.014%
4	4.001	82	87	96	rBV	89336	154589	15.73%	1.792%
5	4.066	96	98	101	rVB3	2132	1887	0.19%	0.022%
6	4.354	144	147	150	rBV	1670	1760	0.18%	0.020%
7	4.541	176	179	183	rVB	761	1057	0.11%	0.012%
8	4.994	253	256	259	rBV2	928	1265	0.13%	0.015%
9	5.370	313	320	323	rBV	710	1157	0.12%	0.013%
10	7.385	655	663	671	rBV	117945	200399	20.39%	2.323%
11	7.549	684	691	700	rVV2	82127	134494	13.68%	1.559%
12	7.772	722	729	736	rBV	108093	182804	18.60%	2.119%
13	8.242	803	809	816	rBV	80995	132439	13.47%	1.535%
14	8.554	858	862	864	rBV	664	1088	0.11%	0.013%
15	8.947	919	929	936	rBV2	135155	229913	23.39%	2.665%
16	9.411	998	1008	1017	rVB	108200	194790	19.82%	2.258%
17	10.146	1126	1133	1142	rVB2	90137	162771	16.56%	1.887%
18	10.692	1220	1226	1234	rBV	127031	231065	23.51%	2.679%
19	11.086	1286	1293	1301	rVB	104888	191086	19.44%	2.215%
20	11.209	1307	1314	1322	rBV	131452	242996	24.72%	2.817%
21	12.648	1557	1559	1560	rBV	2068	1548	0.16%	0.018%
22	12.813	1582	1587	1590	rBV	780	1119	0.11%	0.013%
23	13.112	1634	1638	1640	rBV	844	1205	0.12%	0.014%
24	14.275	1829	1836	1844	rBV	301446	425151	43.25%	4.929%
25	14.581	1880	1888	1897	rBV	296471	462819	47.08%	5.365%
26	14.886	1934	1940	1947	rVB	192298	296726	30.19%	3.440%
27	15.063	1963	1970	1981	rBV	135013	232049	23.61%	2.690%
28	15.139	1981	1983	1985	rVB2	1733	1299	0.13%	0.015%
29	15.192	1990	1992	1996	rVB2	930	1210	0.12%	0.014%
30	15.879	2101	2109	2116	rBV	385581	599366	60.97%	6.948%
31	15.979	2120	2126	2135	rVV	124161	180942	18.41%	2.098%
32	16.120	2147	2150	2152	rBV2	1511	1401	0.14%	0.016%
33	16.437	2202	2204	2205	rBV	1463	1073	0.11%	0.012%
34	17.418	2366	2371	2372	rBV3	1540	1598	0.16%	0.019%
35	17.542	2387	2392	2393	rBV	789	1396	0.14%	0.016%
36	17.636	2401	2408	2414	rVB	292548	441441	44.91%	5.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051925.D
 Acq On : 7 Jan 2022 21:36
 Operator : CG/JU
 Sample : PB141907BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK907

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	17.735	2419	2425	2432	rBV	517663	750814	76.38%	8.704%
38	18.111	2488	2489	2492	rVB	1098	1065	0.11%	0.012%
39	18.652	2578	2581	2582	rBV2	1740	1564	0.16%	0.018%
40	18.669	2582	2584	2587	rVB3	1105	1260	0.13%	0.015%
41	18.775	2600	2602	2606	rBV2	1235	1068	0.11%	0.012%
42	19.063	2648	2651	2652	rBV2	951	1037	0.11%	0.012%
43	19.410	2707	2710	2714	rVV4	1211	1717	0.17%	0.020%
44	19.462	2715	2719	2720	rVV3	1347	1596	0.16%	0.019%
45	19.533	2730	2731	2735	rBV4	1675	1552	0.16%	0.018%
46	19.580	2735	2739	2743	rVV3	7666	9905	1.01%	0.115%
47	19.650	2745	2751	2756	rBV3	6699	12485	1.27%	0.145%
48	19.891	2791	2792	2794	rBV2	1635	1429	0.15%	0.017%
49	20.015	2807	2813	2819	rBV	706763	983008	100.00%	11.396%
50	20.209	2844	2846	2847	rBV2	1385	1206	0.12%	0.014%
51	20.256	2852	2854	2857	rVB2	1947	2261	0.23%	0.026%
52	20.344	2867	2869	2870	rVB2	1776	1016	0.10%	0.012%
53	20.361	2870	2872	2873	rBV2	2297	1453	0.15%	0.017%
54	20.379	2873	2875	2878	rBV3	1618	1450	0.15%	0.017%
55	20.414	2879	2881	2882	rVB2	2457	1216	0.12%	0.014%
56	20.443	2884	2886	2889	rBV4	2168	1726	0.18%	0.020%
57	20.755	2935	2939	2940	rBV3	3463	2708	0.28%	0.031%
58	20.772	2940	2942	2944	rBV3	2303	2441	0.25%	0.028%
59	20.949	2970	2972	2973	rBV2	2254	1464	0.15%	0.017%
60	21.648	3089	3091	3095	rVB5	3266	2741	0.28%	0.032%
61	21.953	3137	3143	3151	rBV	311899	540755	55.01%	6.269%
62	22.799	3284	3287	3288	rBV3	4825	4269	0.43%	0.049%
63	23.146	3345	3346	3349	rBV3	4226	2747	0.28%	0.032%
64	23.175	3349	3351	3352	rBV2	3203	2543	0.26%	0.029%
65	23.222	3358	3359	3361	rBV2	3310	1832	0.19%	0.021%
66	23.557	3414	3416	3420	rVB5	5836	5241	0.53%	0.061%
67	23.727	3443	3445	3446	rBV2	2835	2286	0.23%	0.027%
68	23.786	3453	3455	3458	rBV3	3465	4435	0.45%	0.051%
69	24.761	3619	3621	3622	rBV2	3712	2779	0.28%	0.032%
70	24.902	3643	3645	3646	rBV2	2833	1937	0.20%	0.022%
71	25.202	3684	3696	3709	rVB2	327030	946566	96.29%	10.973%
72	25.307	3712	3714	3719	rVB5	3545	3999	0.41%	0.046%
73	25.443	3727	3737	3753	rVB2	174232	536861	54.61%	6.224%
74	25.795	3795	3797	3800	rVB4	3840	3575	0.36%	0.041%
75	25.989	3828	3830	3831	rBV2	3244	2108	0.21%	0.024%
76	26.142	3854	3856	3857	rBV2	2418	1416	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
 Data File : BG051925.D
 Acq On : 7 Jan 2022 21:36
 Operator : CG/JU
 Sample : PB141907BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK907

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	26.518	3918	3920	3923	rBV4	3234	2542	0.26%	0.029%
78	26.670	3944	3946	3947	rBV2	2791	1630	0.17%	0.019%
79	26.952	3993	3994	3996	rBV2	2819	1468	0.15%	0.017%
80	27.528	4090	4092	4094	rBV3	2909	1864	0.19%	0.022%
81	27.575	4097	4100	4104	rBV5	3592	6145	0.63%	0.071%
82	27.769	4131	4133	4134	rBV	4622	2683	0.27%	0.031%
83	28.198	4204	4206	4207	rBV2	3695	2021	0.21%	0.023%
84	28.221	4207	4210	4211	rBV3	7367	6425	0.65%	0.074%
85	28.239	4211	4213	4217	rVB5	4661	5833	0.59%	0.068%
86	29.402	4409	4411	4413	rBV2	2907	3483	0.35%	0.040%
87	30.794	4646	4648	4649	rBV2	3544	1780	0.18%	0.021%
88	31.094	4697	4699	4702	rBV4	2965	2318	0.24%	0.027%
89	31.558	4776	4778	4780	rBV3	3095	2691	0.27%	0.031%
90	32.633	4959	4961	4962	rBV	2633	1473	0.15%	0.017%




Sum of corrected areas: 8625958

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051925.D
Acq On : 7 Jan 2022 21:36
Operator : CG/JU
Sample : PB141907BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK907

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

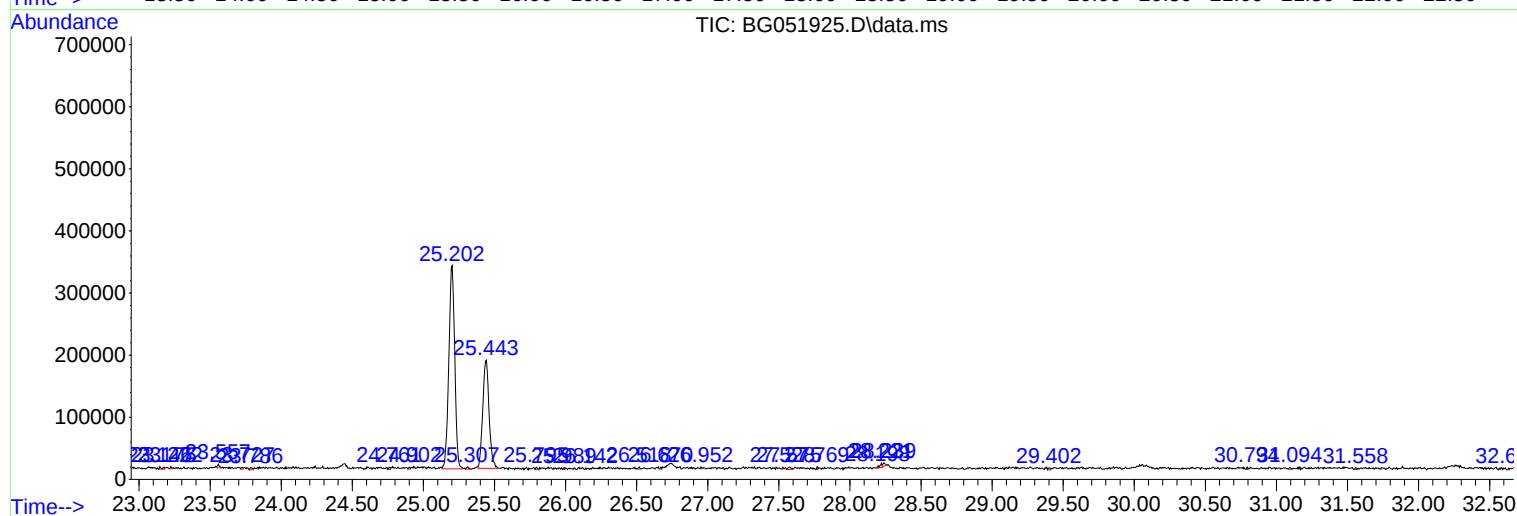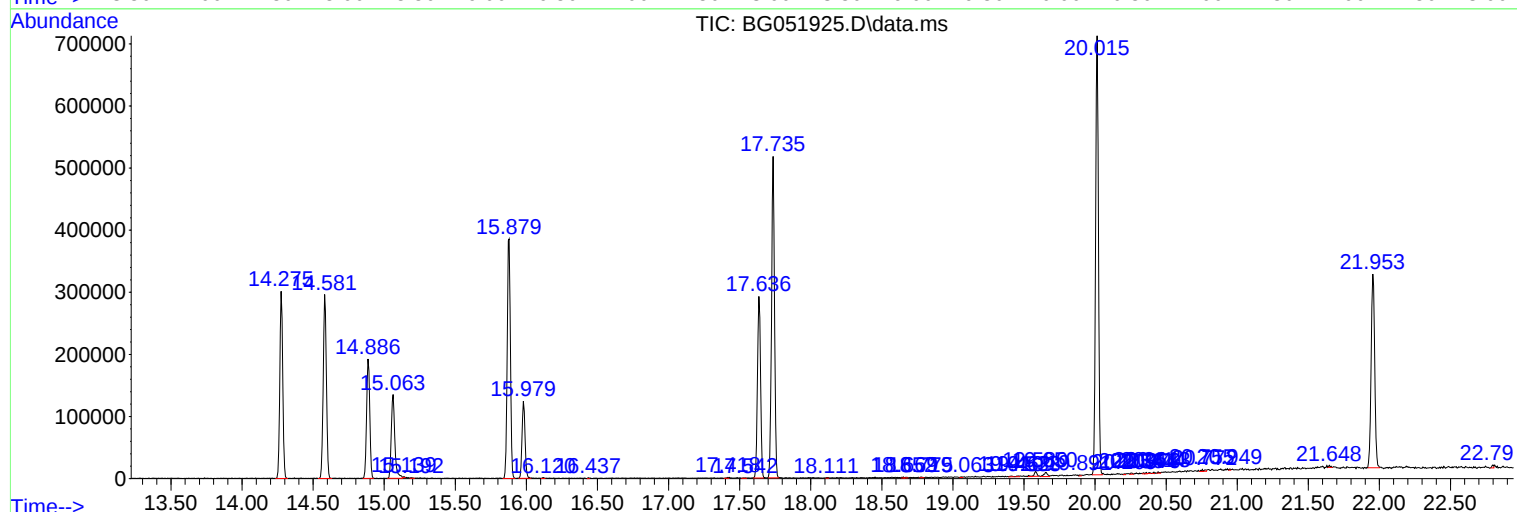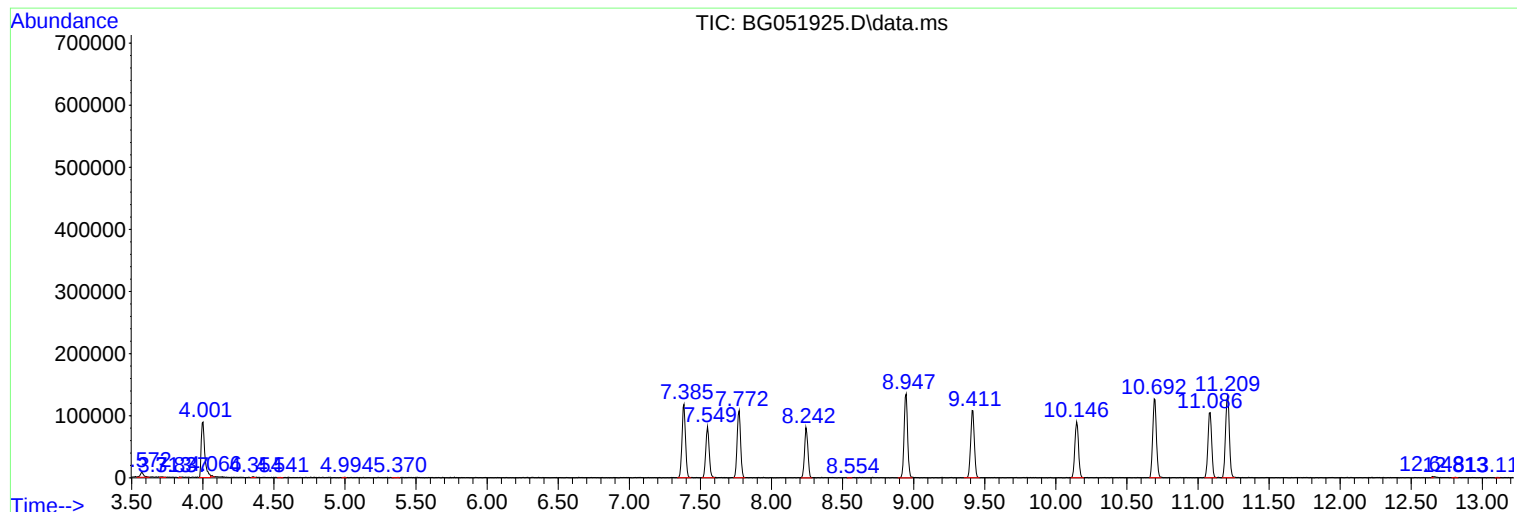

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051925.D
Acq On : 7 Jan 2022 21:36
Operator : CG/JU
Sample : PB141907BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK907

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010622\
Data File : BG051925.D
Acq On : 7 Jan 2022 21:36
Operator : CG/JU
Sample : PB141907BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK907

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc