


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010625\
Data File : BG063932.D
Acq On : 6 Jan 2025 10:05
Operator : RC/JU
Sample : DFTPP451
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP451

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010625.MA.M
Title : SVOA CALIBRATION
Last Update : Mon Jan 06 16:42:18 2025

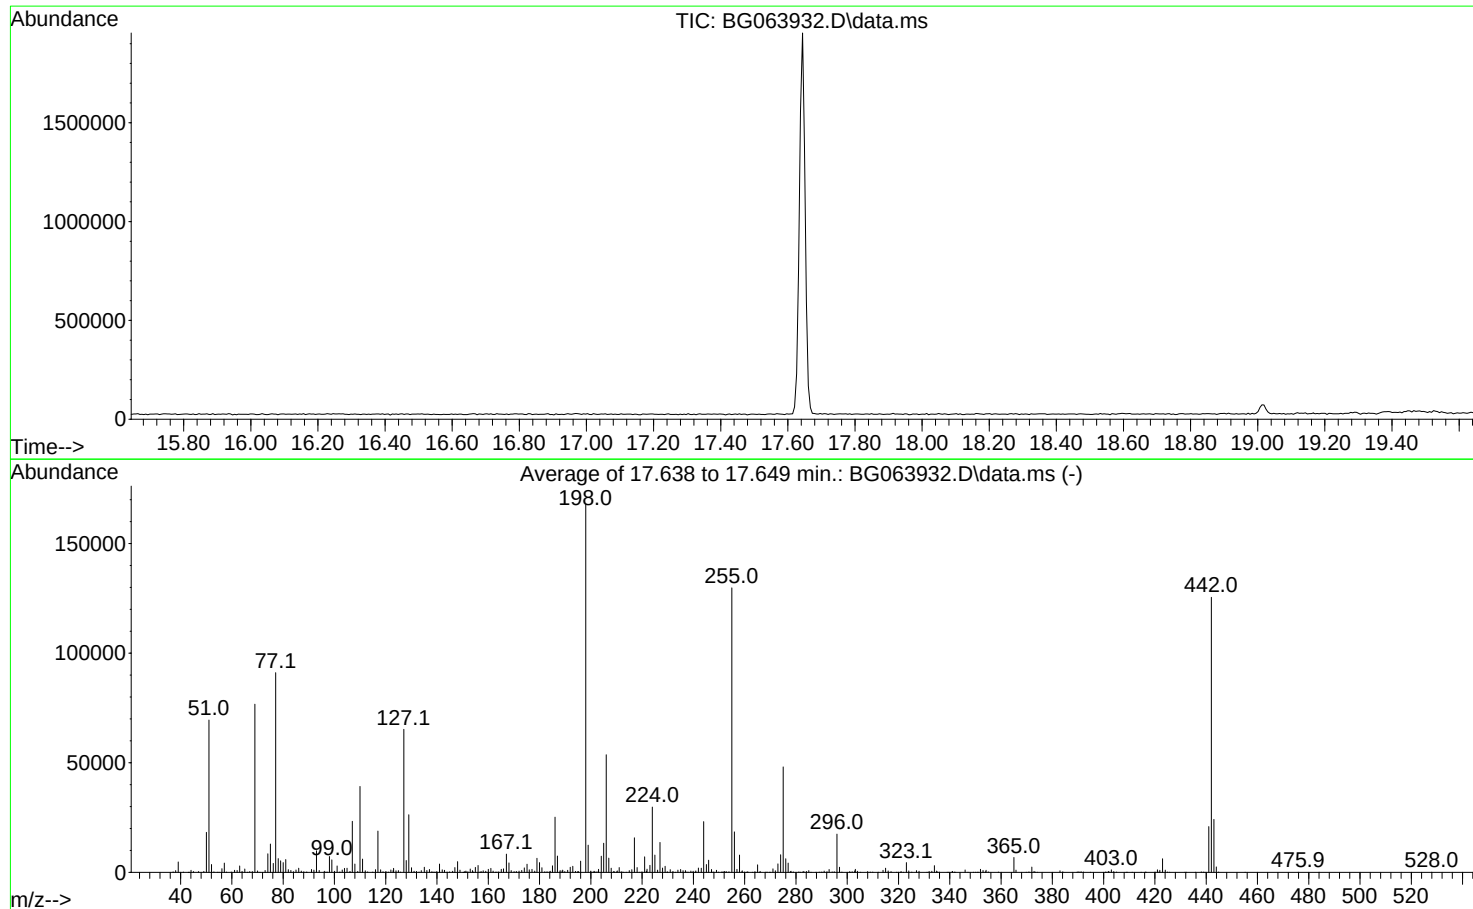

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	69469	PASS
68	69	0.00	2	0.5	400	PASS
69	198	0.00	100	45.7	76693	PASS
70	69	0.00	2	0.8	628	PASS
127	198	10	80	38.9	65221	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	167787	PASS
199	198	5	9	7.4	12441	PASS
275	198	10	60	28.7	48107	PASS
365	198	1	100	4.1	6807	PASS
441	198	0.01	100	12.4	20870	PASS
442	198	50	100	74.8	125459	PASS
443	442	15	24	19.2	24139	PASS

m/z	Abundance
35.90	211.0
40.00	17480.0
43.00	404.0
44.10	3311.0
48.10	150.0
50.90	222.0
55.10	305.0
83.00	341.0
90.00	171.0
95.10	308.0
126.20	281.0
150.30	172.0
158.30	178.0
189.10	172.0
193.50	224.0
194.20	153.0
206.90	332.0
210.10	151.0
226.40	268.0
240.40	164.0
248.10	163.0
276.80	157.0
346.70	205.0
433.70	197.0
463.90	195.0
512.20	293.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

m/z	Abundance
36.00	308.0
37.20	296.0
38.10	668.0
39.10	5885.0
40.10	16448.0
43.10	350.0
44.10	3692.0
45.10	336.0
47.00	254.0
49.10	723.0
50.10	20416.0
51.10	77920.0
52.10	4229.0
53.00	489.0
54.30	247.0
55.00	568.0
56.10	1535.0
57.10	4293.0
58.00	183.0
59.70	245.0
61.00	809.0
62.10	1158.0
63.10	3218.0
64.10	408.0
65.10	1673.0
66.10	203.0
67.10	234.0
68.00	1199.0
69.00	85352.0
70.00	646.0
73.10	710.0
74.10	8725.0
75.00	13322.0
76.10	4575.0
77.10	97600.0
78.10	6884.0
79.00	5593.0
80.00	4485.0
81.00	6182.0
82.00	1428.0
83.10	1151.0
83.90	164.0
85.00	1083.0
86.10	1762.0
87.10	660.0
88.10	380.0
89.00	210.0
91.00	1460.0
92.00	1390.0
93.00	9199.0
94.10	642.0
95.10	263.0
96.10	527.0
96.70	393.0
98.10	8247.0
99.00	5994.0
100.10	536.0
101.00	2558.0
102.00	312.0
103.10	872.0
103.90	1962.0
105.00	1596.0
106.20	847.0
107.00	24832.0
108.00	3877.0
110.00	43144.0
111.00	6622.0
112.10	731.0
113.00	269.0
114.90	221.0
116.10	1122.0
117.00	19088.0
118.00	1344.0
119.00	370.0
120.10	269.0
122.10	1217.0
122.90	2413.0
124.00	464.0
125.00	802.0
127.10	65128.0
128.00	6205.0
129.00	26464.0
130.10	2807.0
131.10	187.0
131.90	197.0
133.90	471.0
135.00	2383.0
136.10	588.0
137.10	1491.0
138.00	245.0
139.30	207.0
140.00	287.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

141.00	3247.0
142.00	1033.0
142.90	978.0
145.00	360.0
146.10	600.0
147.00	2250.0
148.00	3917.0
149.10	1321.0
151.30	430.0
151.70	477.0
153.00	1544.0
153.80	658.0
154.20	547.0
155.00	2327.0
156.10	3747.0
157.10	561.0
158.00	696.0
159.20	425.0
160.00	1450.0
161.00	989.0
161.90	483.0
162.90	331.0
164.00	291.0
164.20	310.0
165.10	1401.0
166.00	1244.0
167.00	7444.0
168.00	4274.0
168.90	844.0
170.00	501.0
171.00	467.0
172.00	602.0
173.10	998.0
174.10	1984.0
175.10	4549.0
176.10	1531.0
177.00	1391.0
178.10	466.0
179.00	5695.0
180.00	4380.0
180.90	1897.0
183.80	738.0
185.00	3082.0
186.10	24888.0
187.00	7044.0
188.10	1016.0
189.10	1943.0
189.90	404.0
191.00	956.0
192.00	1578.0
193.00	2838.0
194.00	661.0
195.20	477.0
196.00	5333.0
198.00	156160.0
198.90	12112.0
199.90	813.0
201.30	781.0
202.90	1552.0
204.00	7596.0
205.00	13475.0
206.00	49520.0
207.00	5176.0
208.00	1955.0
208.90	477.0
210.00	694.0
210.40	1289.0
211.00	1964.0
212.10	487.0
215.00	974.0
216.00	1978.0
217.00	14375.0
218.10	2253.0
219.10	208.0
220.00	377.0
221.00	7593.0
222.00	1561.0
223.00	2531.0
224.00	27320.0
225.00	6797.0
226.00	905.0
227.00	14039.0
228.00	1935.0
229.00	1766.0
229.80	388.0
231.00	1156.0
232.10	586.0
234.10	837.0
235.00	1737.0
236.00	867.0
237.00	537.0
239.10	614.0
240.20	296.0
240.80	778.0
242.00	1731.0
243.00	1558.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

244.00	22464.0
245.00	2865.0
245.90	6218.0
247.00	2003.0
248.00	355.0
249.00	773.0
251.00	382.0
252.10	548.0
252.40	581.0
255.00	115296.0
256.00	16560.0
257.00	1855.0
258.00	7667.0
258.90	977.0
259.90	267.0
261.00	348.0
264.00	283.0
265.00	3798.0
265.80	254.0
266.20	387.0
268.20	170.0
268.70	199.0
271.10	1496.0
271.90	659.0
273.00	2849.0
274.00	6582.0
275.00	41848.0
276.00	6085.0
277.00	3457.0
278.10	831.0
279.00	388.0
281.10	426.0
283.10	643.0
284.10	416.0
285.00	888.0
287.80	297.0
291.00	383.0
291.90	383.0
293.00	1019.0
294.20	222.0
295.00	535.0
296.00	13503.0
297.00	1953.0
298.00	216.0
301.20	246.0
303.10	2111.0
304.00	502.0
308.00	356.0
309.90	176.0
312.10	226.0
314.00	888.0
315.00	1412.0
315.90	228.0
317.10	232.0
319.30	209.0
320.80	310.0
321.90	296.0
323.10	4115.0
323.90	622.0
327.10	751.0
328.00	482.0
331.10	238.0
332.10	243.0
333.00	284.0
334.00	3018.0
334.90	1056.0
340.90	843.0
346.00	794.0
349.20	276.0
351.10	301.0
352.00	894.0
352.90	614.0
353.90	897.0
355.10	195.0
358.90	207.0
365.00	5180.0
365.90	717.0
370.90	154.0
372.00	1769.0
373.30	502.0
383.00	624.0
383.90	164.0
390.10	234.0
390.70	469.0
392.20	173.0
400.70	187.0
401.80	610.0
403.00	1268.0
404.10	155.0
405.10	172.0
411.10	180.0
416.30	379.0
421.00	730.0
421.70	638.0
423.00	6144.0
424.00	1088.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

435.80	196.0
439.00	257.0
441.00	15850.0
442.00	94264.0
443.00	18616.0
443.90	1935.0
484.00	178.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

m/z	Abundance
37.00	384.0
38.10	1026.0
39.10	5077.0
40.00	16440.0
41.10	229.0
43.10	356.0
44.10	5035.0
45.00	419.0
47.00	575.0
49.00	597.0
50.10	20800.0
51.10	79800.0
52.10	4243.0
53.00	290.0
54.90	423.0
56.10	2327.0
57.00	5320.0
57.90	358.0
59.80	250.0
61.10	1133.0
62.00	914.0
63.00	3152.0
63.90	719.0
65.00	1744.0
67.10	444.0
69.00	90208.0
70.00	539.0
72.90	1222.0
74.00	9860.0
75.10	16329.0
76.20	4605.0
77.10	108600.0
78.10	6983.0
79.10	6188.0
80.00	5117.0
81.00	6420.0
82.10	1598.0
83.00	1524.0
84.00	331.0
85.00	713.0
86.00	2052.0
87.10	805.0
88.00	275.0
89.30	325.0
91.00	1301.0
92.00	800.0
93.00	13040.0
94.00	1314.0
96.00	499.0
98.00	8301.0
99.00	7290.0
100.10	676.0
101.00	3787.0
102.20	183.0
103.00	1384.0
104.00	2203.0
105.00	1937.0
105.90	658.0
107.00	27600.0
108.00	5050.0
109.10	1284.0
110.00	45232.0
111.00	7730.0
112.00	778.0
113.00	406.0
115.00	186.0
116.00	1653.0
117.00	21320.0
118.00	1220.0
118.90	293.0
120.10	667.0
121.00	184.0
122.00	1375.0
123.10	3389.0
124.00	964.0
124.90	821.0
127.10	79536.0
128.00	6829.0
129.00	33072.0
130.10	2376.0
131.10	543.0
132.00	696.0
133.10	269.0
133.90	1078.0
135.10	2777.0
136.00	1169.0
137.00	1691.0
138.40	377.0
140.00	512.0
141.00	6048.0
142.00	1600.0
143.00	999.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

143.90	309.0
144.90	363.0
146.10	693.0
147.00	2979.0
148.10	6494.0
148.90	1147.0
150.10	416.0
150.80	845.0
151.30	891.0
152.20	309.0
153.10	1816.0
153.90	1024.0
155.00	2672.0
156.00	3490.0
157.30	816.0
158.00	1051.0
159.00	626.0
160.00	1923.0
161.10	2787.0
161.90	767.0
163.10	162.0
165.10	1666.0
166.00	2345.0
167.10	11280.0
168.10	4909.0
168.90	946.0
170.10	555.0
170.90	561.0
172.00	844.0
173.00	996.0
174.10	2559.0
175.10	4097.0
175.90	1105.0
177.00	1777.0
178.10	613.0
179.00	8757.0
180.00	5087.0
181.00	2454.0
182.00	398.0
182.90	480.0
184.10	922.0
185.00	3095.0
186.00	30248.0
187.00	9612.0
188.00	1145.0
189.00	1763.0
189.80	444.0
190.90	912.0
192.00	3533.0
193.00	3716.0
194.10	592.0
194.90	777.0
195.10	699.0
196.10	5996.0
198.00	205952.0
199.00	13807.0
200.10	1024.0
200.90	379.0
201.50	753.0
202.10	615.0
203.10	2513.0
204.10	8222.0
205.00	15743.0
206.00	65264.0
207.00	9585.0
207.90	2123.0
209.20	688.0
210.00	497.0
211.00	2722.0
212.10	289.0
212.80	187.0
214.90	556.0
216.00	1677.0
217.00	20288.0
218.00	3088.0
221.00	8240.0
221.90	2744.0
223.00	3890.0
224.00	36560.0
225.00	9003.0
226.10	1564.0
227.00	16299.0
228.00	1908.0
229.00	3101.0
230.00	479.0
231.00	1304.0
232.00	624.0
233.00	276.0
233.90	1012.0
235.10	1274.0
236.00	955.0
236.90	1918.0
237.90	377.0
239.00	588.0
239.90	639.0
241.00	1205.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

241.90	2665.0
243.10	2518.0
244.00	27344.0
245.10	5181.0
246.00	5401.0
247.10	1303.0
247.70	526.0
249.00	1357.0
249.90	191.0
251.30	521.0
252.00	710.0
253.00	661.0
255.00	158720.0
256.00	23560.0
257.00	1842.0
258.00	9442.0
259.10	933.0
260.00	239.0
260.60	161.0
261.30	350.0
263.80	311.0
265.00	3648.0
266.00	486.0
268.80	169.0
269.80	330.0
271.00	1696.0
272.00	851.0
273.00	5296.0
274.00	9735.0
275.00	59344.0
276.00	6619.0
277.00	5590.0
277.80	785.0
278.10	737.0
278.90	234.0
282.70	609.0
283.90	469.0
285.00	832.0
289.10	404.0
289.90	476.0
291.00	768.0
292.10	176.0
292.90	1565.0
294.10	391.0
296.00	22128.0
297.00	3250.0
297.80	173.0
300.90	505.0
301.90	442.0
303.20	2139.0
303.90	586.0
305.20	247.0
307.90	594.0
308.90	257.0
313.90	1220.0
314.90	2473.0
316.00	1085.0
317.10	587.0
321.00	749.0
323.00	5781.0
324.00	836.0
325.20	362.0
326.90	922.0
328.00	264.0
331.90	538.0
333.10	771.0
334.10	3382.0
334.90	803.0
335.90	420.0
339.00	214.0
339.60	243.0
341.10	570.0
342.10	254.0
346.00	1204.0
346.90	229.0
350.10	181.0
352.00	1679.0
353.00	820.0
354.20	1202.0
355.00	201.0
359.00	164.0
365.00	8841.0
365.80	1595.0
369.80	304.0
370.80	173.0
372.00	2567.0
372.90	678.0
383.00	870.0
384.10	282.0
390.00	282.0
391.20	430.0
401.00	266.0
402.10	818.0
403.00	1535.0
403.80	653.0
404.90	187.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

408.80	220.0
414.60	156.0
416.60	195.0
420.00	277.0
421.00	1627.0
421.90	1724.0
423.00	6434.0
424.10	1199.0
424.90	315.0
431.70	199.0
432.20	169.0
438.00	291.0
438.80	179.0
441.00	24272.0
442.00	147712.0
443.00	27872.0
444.00	3268.0
444.90	301.0
475.90	179.0
528.00	153.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

m/z	Abundance
38.10	680.0
39.10	3354.0
40.10	17560.0
41.10	221.0
43.00	614.0
44.10	4160.0
45.10	382.0
47.10	253.0
50.10	13473.0
51.10	51352.0
52.10	2204.0
55.00	179.0
56.00	1250.0
57.10	3122.0
61.00	868.0
62.00	498.0
63.00	2423.0
64.10	284.0
65.10	1178.0
66.90	444.0
69.00	54520.0
70.10	700.0
71.00	186.0
72.90	765.0
74.10	6881.0
75.00	9075.0
76.10	3192.0
77.10	66992.0
78.10	5085.0
79.00	3952.0
80.10	3669.0
81.00	4999.0
82.00	713.0
82.90	959.0
84.10	347.0
85.00	1576.0
86.10	1807.0
87.00	343.0
88.20	254.0
89.10	361.0
90.10	235.0
91.10	1307.0
92.00	868.0
93.00	7248.0
94.10	701.0
95.10	287.0
96.10	548.0
97.20	432.0
98.00	5127.0
99.00	3779.0
99.90	236.0
101.10	2374.0
102.10	266.0
103.10	1145.0
104.00	1297.0
104.90	2061.0
107.00	17464.0
108.00	2387.0
110.00	29200.0
111.00	3890.0
112.00	736.0
116.00	950.0
117.00	16162.0
118.10	983.0
118.90	272.0
120.10	409.0
121.00	354.0
122.10	709.0
123.10	2103.0
124.00	740.0
125.00	854.0
125.80	389.0
127.00	51000.0
128.00	3206.0
129.00	19288.0
130.10	1229.0
131.00	776.0
132.00	354.0
132.90	223.0
133.90	884.0
135.00	1930.0
136.10	838.0
137.00	863.0
137.90	385.0
138.90	423.0
139.90	308.0
141.10	2083.0
142.10	927.0
143.00	894.0
144.00	256.0
146.20	166.0
147.00	1324.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

148.00	4340.0
149.00	695.0
150.10	210.0
151.00	473.0
151.30	376.0
152.00	337.0
152.90	1258.0
153.90	796.0
155.00	1878.0
156.10	2084.0
156.80	402.0
158.00	376.0
159.00	590.0
160.10	840.0
161.00	1631.0
161.90	576.0
163.10	216.0
163.80	326.0
165.10	1077.0
165.90	1256.0
167.00	6267.0
168.00	3783.0
169.00	718.0
170.90	227.0
171.90	377.0
173.00	762.0
174.00	1559.0
175.10	2606.0
176.00	849.0
177.10	1115.0
178.10	669.0
179.00	4829.0
180.00	3932.0
181.00	2092.0
182.10	450.0
183.00	363.0
184.20	593.0
185.10	2768.0
186.00	20480.0
187.00	5616.0
187.80	401.0
188.20	345.0
188.80	1903.0
189.90	192.0
191.10	925.0
192.00	1874.0
193.10	1797.0
194.00	496.0
195.00	608.0
196.00	4047.0
198.00	141248.0
199.00	11405.0
200.00	757.0
201.30	824.0
203.00	1705.0
204.00	6280.0
205.00	10627.0
206.00	46168.0
207.10	5811.0
207.90	1597.0
209.00	782.0
210.20	773.0
211.10	1977.0
211.80	705.0
213.80	152.0
215.10	875.0
217.00	12693.0
218.10	1165.0
219.90	388.0
221.00	5484.0
221.70	1749.0
223.10	3152.0
224.00	25472.0
225.00	7979.0
226.00	626.0
227.00	10606.0
228.00	2064.0
229.00	3448.0
229.80	369.0
231.00	1307.0
232.10	178.0
234.00	1279.0
235.00	930.0
235.90	674.0
237.10	594.0
239.10	572.0
239.90	807.0
240.90	703.0
241.90	1629.0
243.10	1615.0
244.00	19640.0
245.00	2738.0
245.90	4986.0
247.10	707.0
247.90	289.0
249.10	670.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

249.90	178.0
251.80	507.0
252.80	305.0
253.90	794.0
255.00	115280.0
256.00	15324.0
256.80	489.0
258.00	6505.0
259.00	1385.0
261.10	310.0
263.10	169.0
264.20	404.0
265.10	2890.0
266.00	433.0
270.00	304.0
271.10	1547.0
272.10	671.0
273.00	3410.0
274.00	7771.0
275.00	43128.0
276.00	5921.0
277.00	4143.0
277.90	265.0
281.20	178.0
281.80	221.0
283.00	660.0
284.10	536.0
285.00	793.0
285.90	315.0
288.90	165.0
290.20	315.0
291.00	605.0
292.20	582.0
293.00	1364.0
294.90	423.0
296.00	16664.0
297.00	1870.0
301.00	376.0
302.00	441.0
302.90	1944.0
304.10	536.0
307.90	217.0
309.00	236.0
310.00	293.0
314.00	829.0
314.90	1841.0
315.90	731.0
317.10	372.0
319.90	309.0
321.00	454.0
323.00	3554.0
324.10	613.0
327.00	708.0
328.00	693.0
332.00	518.0
332.90	566.0
333.90	2742.0
335.10	694.0
341.00	666.0
341.80	484.0
346.00	1208.0
347.10	216.0
350.70	280.0
351.90	1696.0
352.90	1174.0
354.10	1627.0
354.90	331.0
365.00	6399.0
365.90	746.0
370.90	256.0
372.00	2804.0
372.90	648.0
374.10	195.0
383.00	680.0
384.10	297.0
389.60	233.0
390.10	302.0
391.20	423.0
392.10	166.0
394.90	166.0
400.80	214.0
401.90	713.0
402.90	694.0
404.00	602.0
405.10	166.0
409.20	177.0
420.20	156.0
421.00	1251.0
422.00	1229.0
423.00	5978.0
424.00	733.0
424.90	258.0
425.80	216.0
438.10	480.0
439.50	170.0
441.00	22488.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451

442.00	134400.0
443.00	25928.0
443.90	2271.0
444.90	261.0
455.20	210.0

Instrument :
BNA_G
ClientSampleId :
DFTPP451