
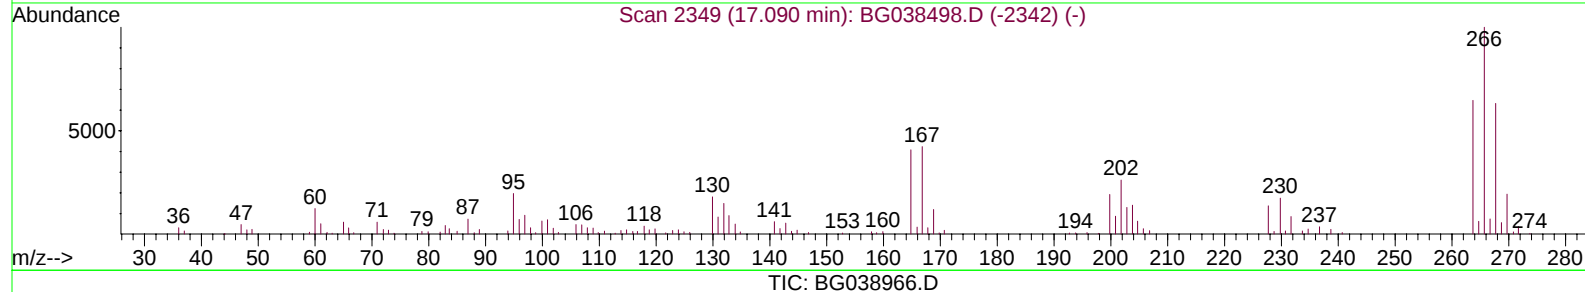
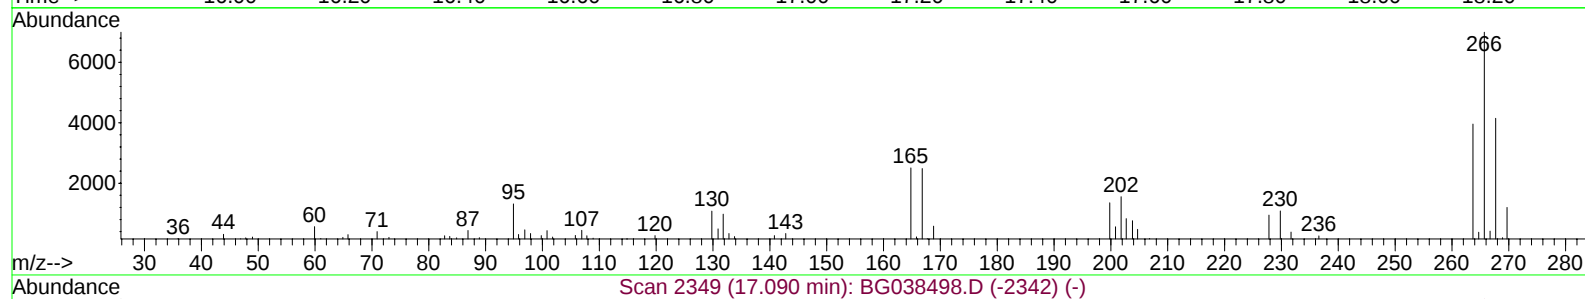


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010719\
Data File : BG038966.D
Acq On : 7 Jan 2019 14:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 17:54:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

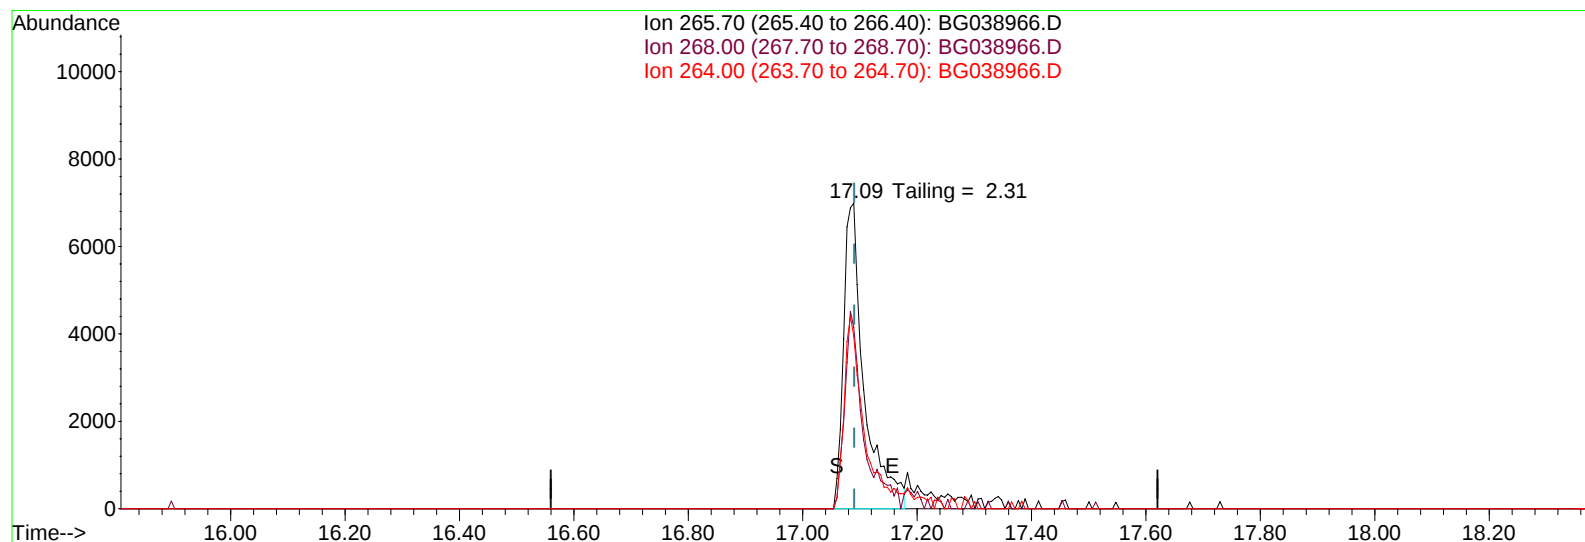

(70) Pentachlorophenol (C)




17.089min (-0.001) 39917.99ng

response 17636

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	59.27
264.00	70.90	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010719\
Data File : BG038966.D
Acq On : 7 Jan 2019 14:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 17:54:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

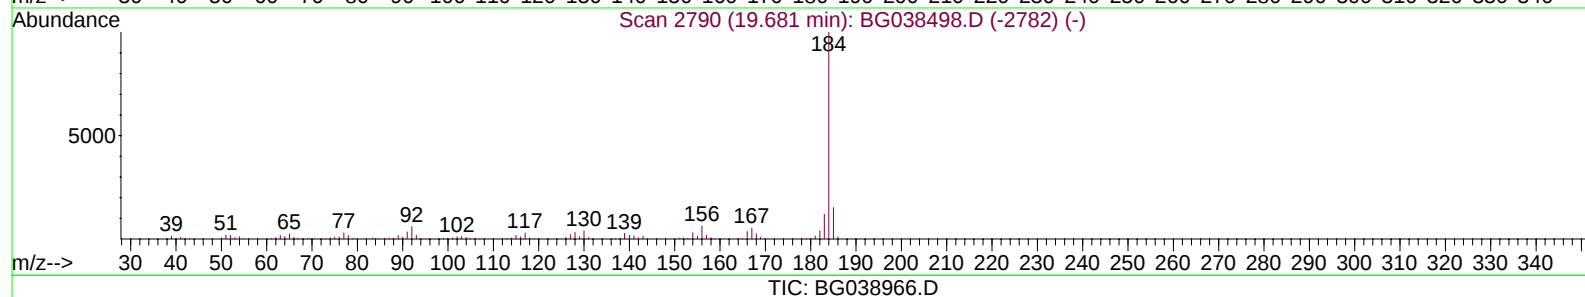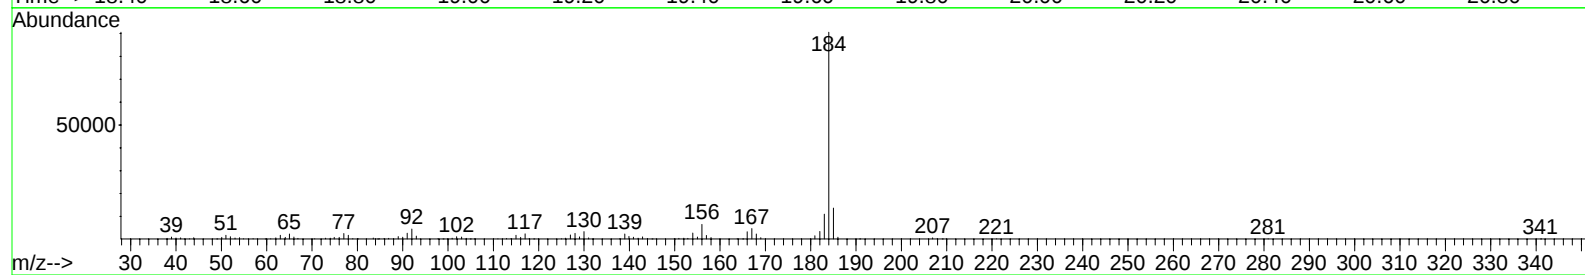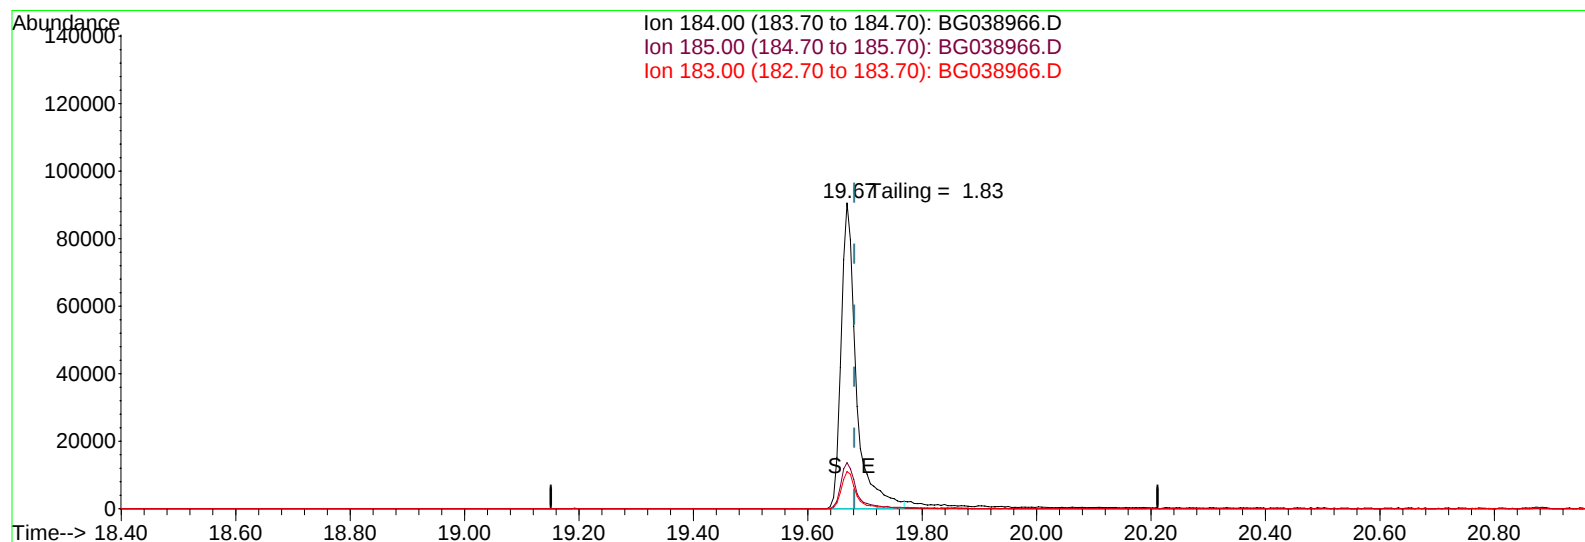

(77) Benzidine

19.668min (-0.013) 0.00ng

response 172526

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.09
183.00	12.00	12.12
0.00	0.00	0.00