
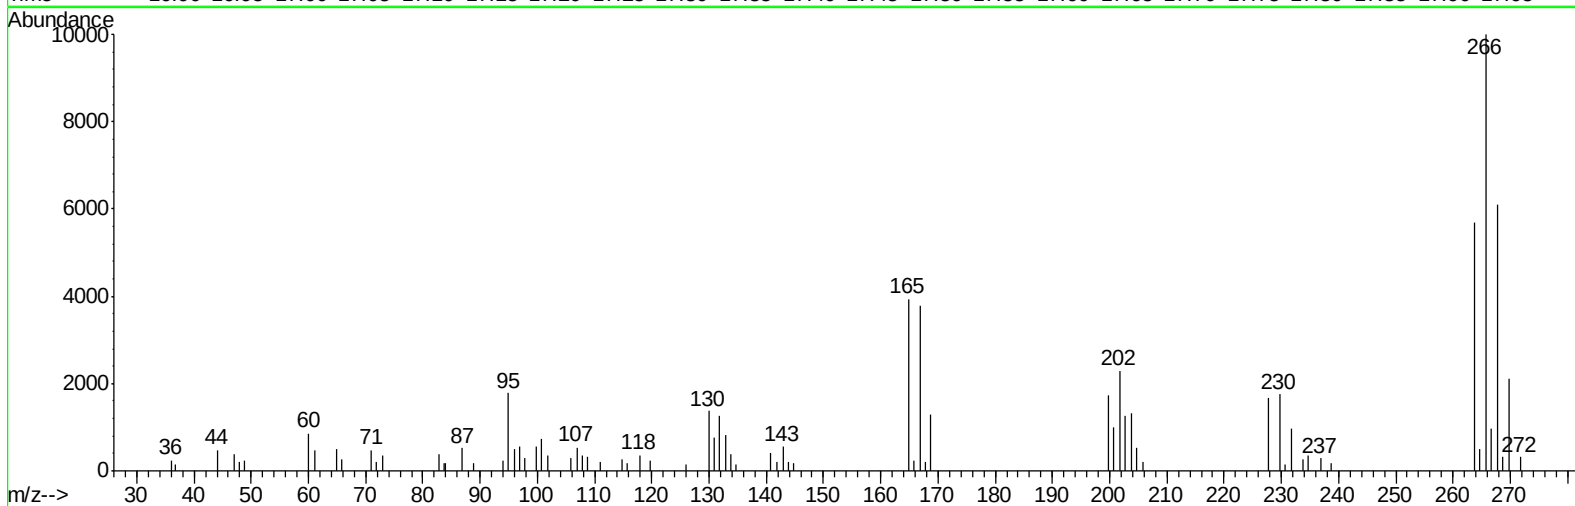


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010719\  
Data File : BG038985.D  
Acq On : 8 Jan 2019 5:03  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 08 08:14:31 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 12 15:26:27 2018  
Response via : Initial Calibration

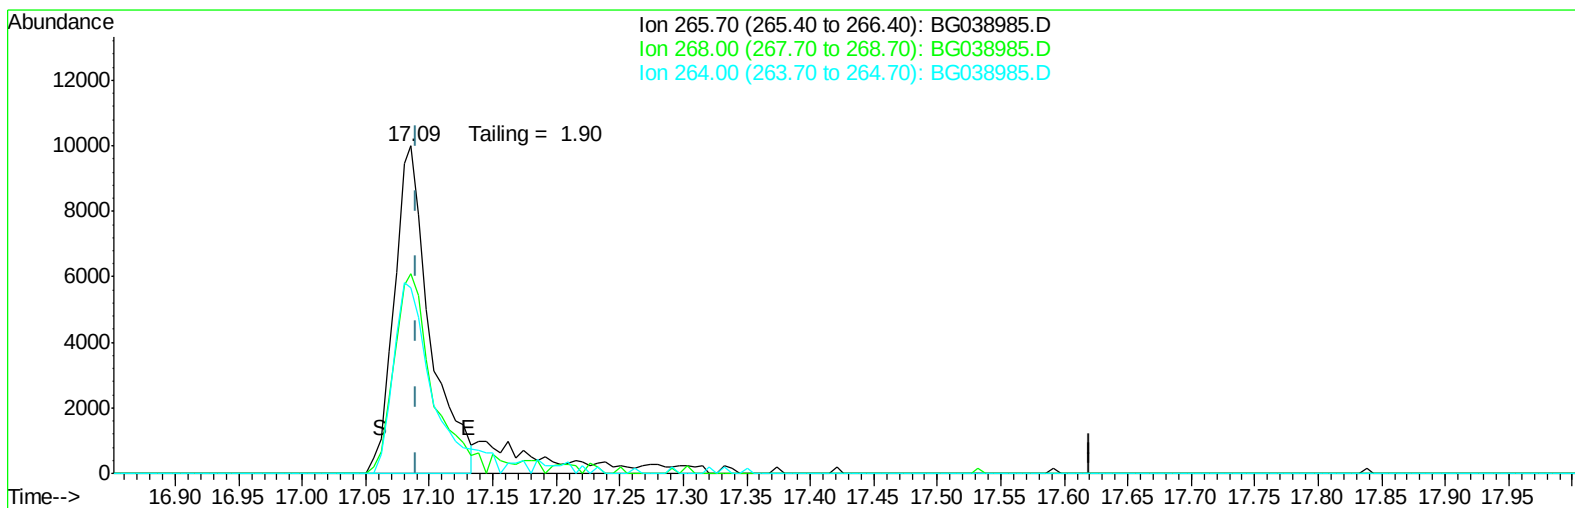

TIC: BG038985.D

(70) Pentachlorophenol (C)



17.086min (-0.004) 35120.08ng

response 20776

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 68.80 | 64.34 |
| 264.00 | 70.90 | 61.91 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010719\  
 Data File : BG038985.D  
 Acq On : 8 Jan 2019 5:03  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 08 08:14:31 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 12 15:26:27 2018  
 Response via : Initial Calibration

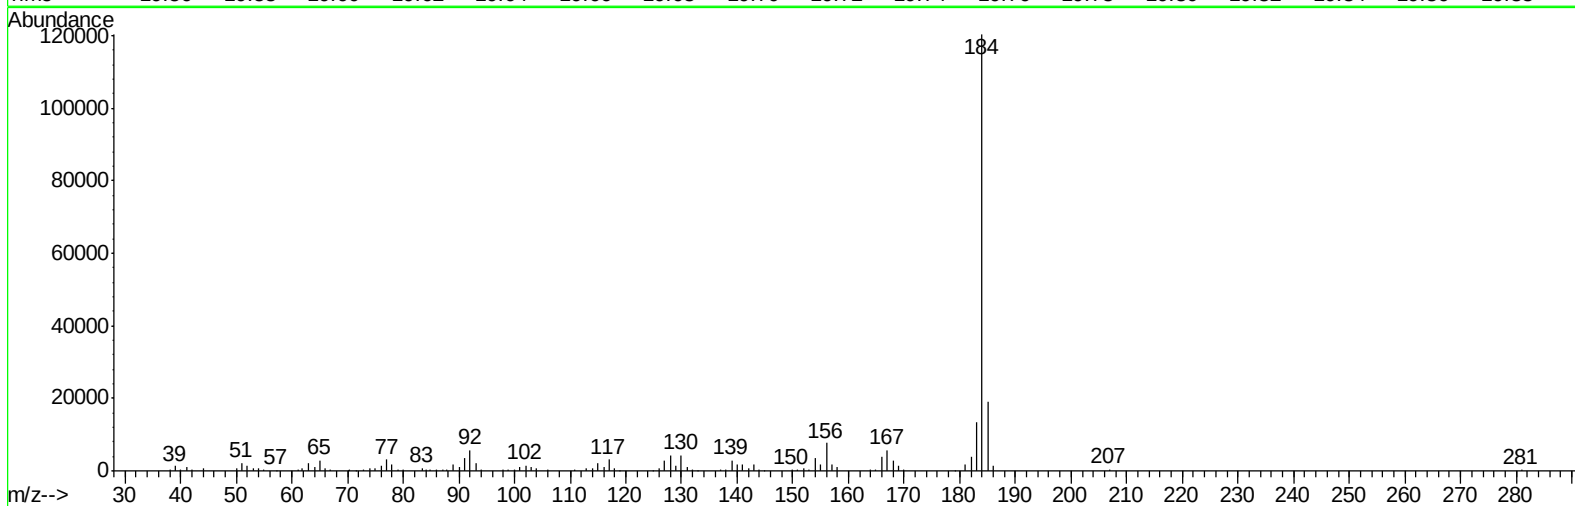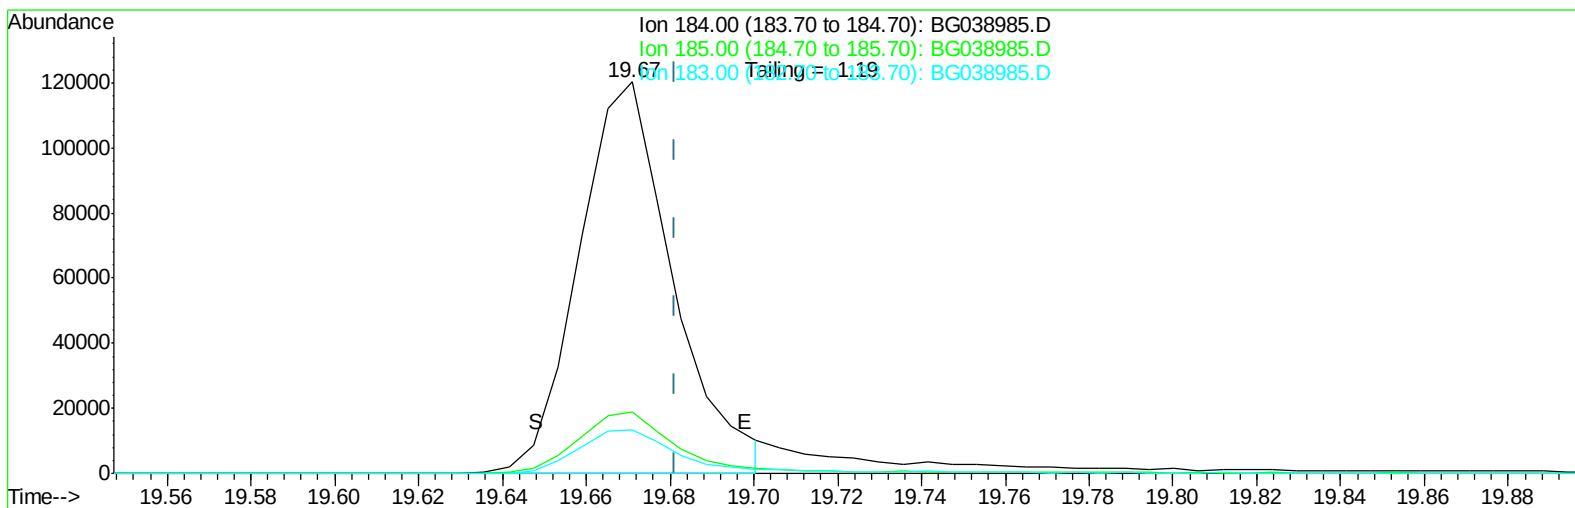

TIC: BG038985.D

(77) Benzidine

19.671min (-0.010) 0.00ng

response 207167

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.20 | 15.71 |
| 183.00 | 12.00 | 11.15 |
| 0.00   | 0.00  | 0.00  |