

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010719\
 Data File : BG038972.D
 Acq On : 7 Jan 2019 18:33
 Operator : JU/SJ
 Sample : K1036-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 13-D

Quant Time: Jan 08 03:42:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	39661	20.00	ng	-0.01
21) Naphthalene-d8	10.86	136	157319	20.00	ng	-0.02
39) Acenaphthene-d10	14.69	164	100154	20.00	ng	-0.01
64) Phenanthrene-d10	17.43	188	216303	20.00	ng	-0.01
76) Chrysene-d12	21.71	240	222621	20.00	ng	-0.02
87) Perylene-d12	25.00	264	229828	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	188796	84.43	ng	0.00
7) Phenol-d6	7.21	99	265271	86.41	ng	0.00
23) Nitrobenzene-d5	9.22	82	164041	53.27	ng	-0.02
42) 2,4,6-Tribromophenol	16.18	330	123509	89.48	ng	-0.01
45) 2-Fluorobiphenyl	13.30	172	449541	61.58	ng	-0.02
79) Terphenyl-d14	20.03	244	665167	65.03	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010719\
Data File : BG038972.D
Acq On : 7 Jan 2019 18:33
Operator : JU/SJ
Sample : K1036-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
13-D

Quant Time: Jan 08 03:42:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

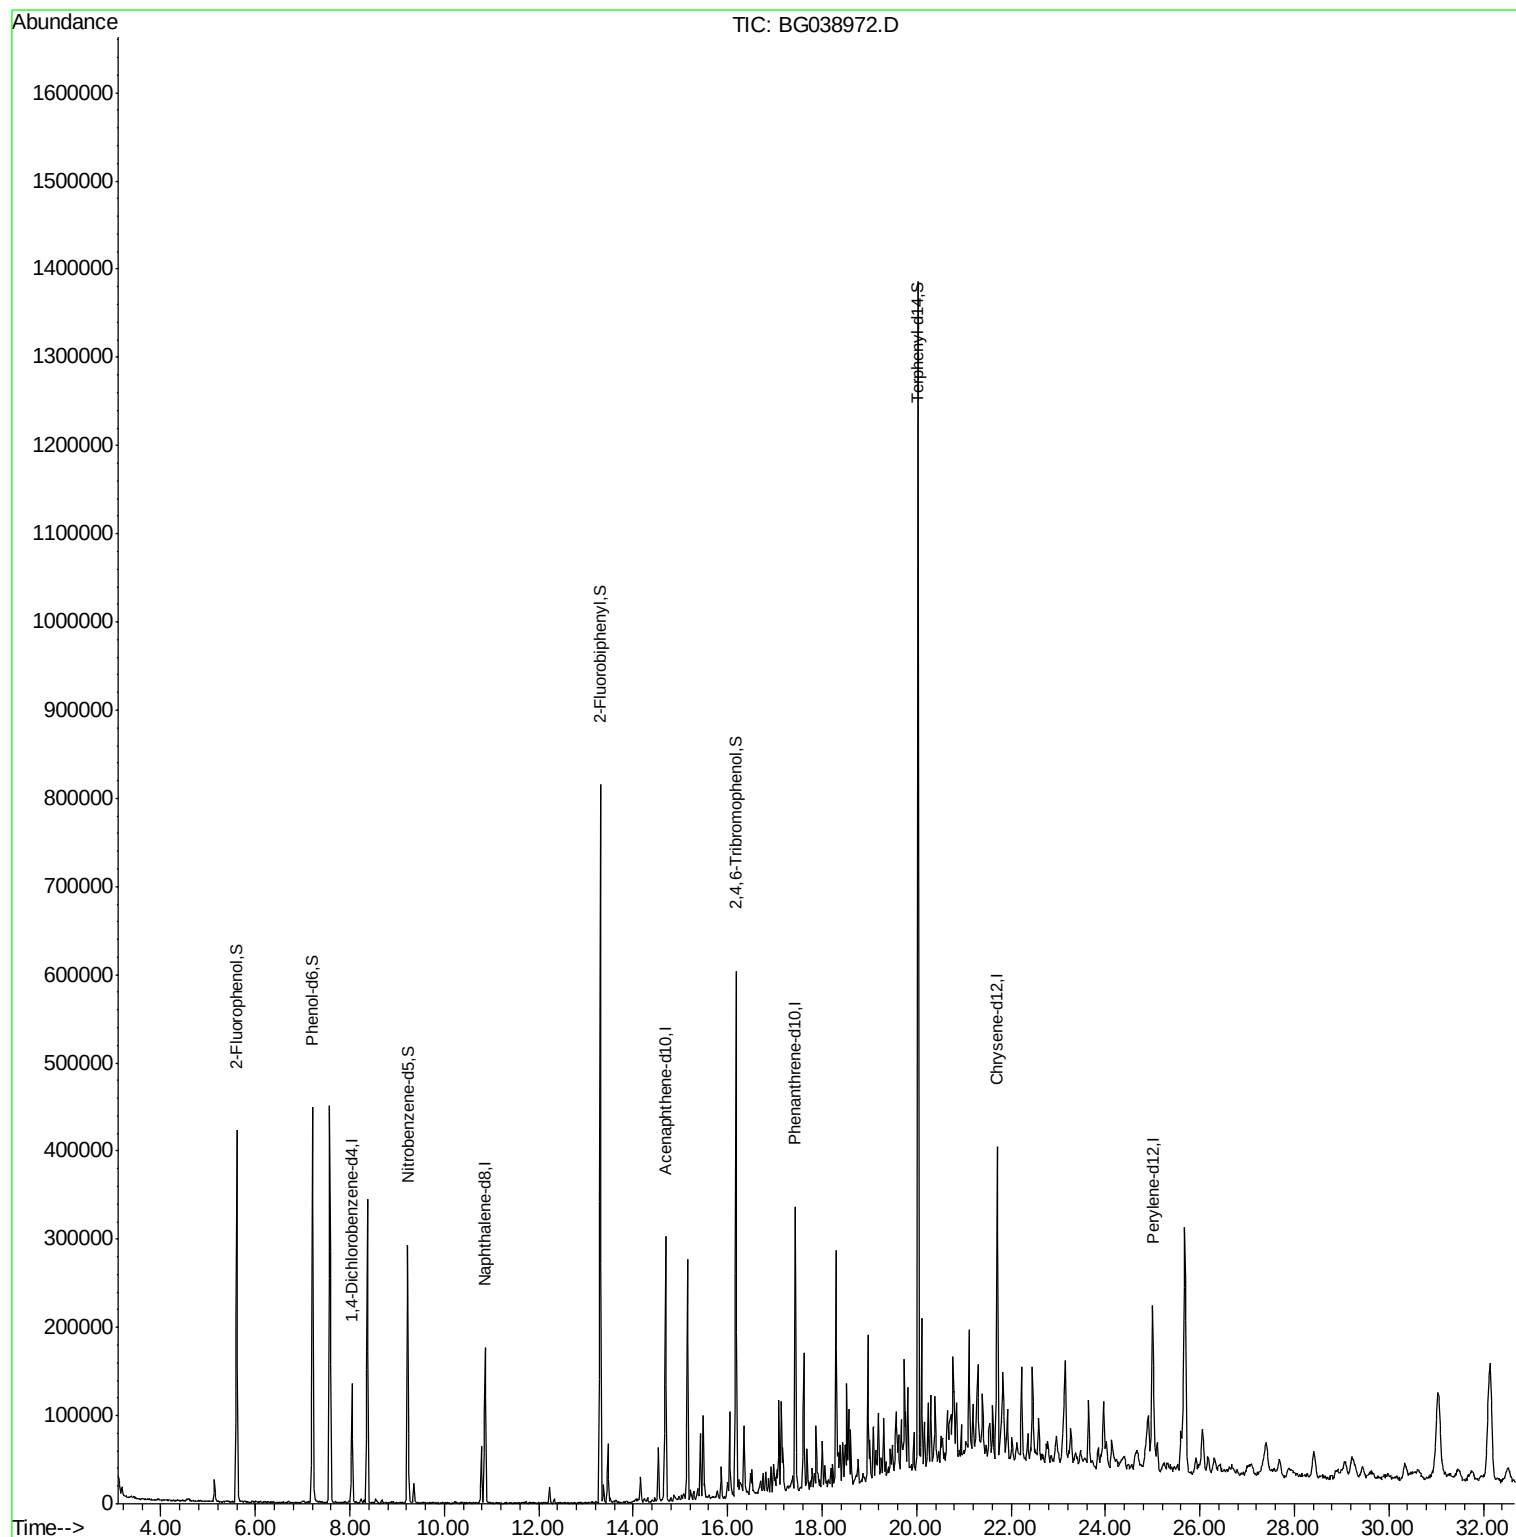

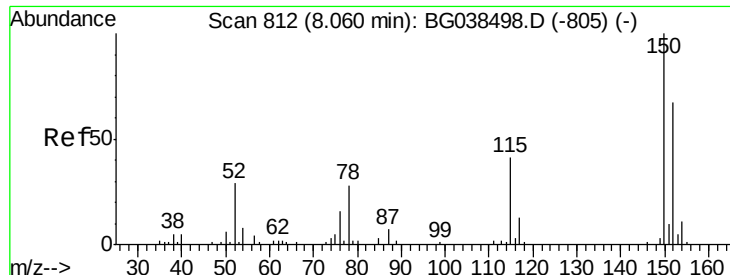


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 844
Delta R.T. -0.01 min
Lab File: BG038972.D
Acq: 7 Jan 2019 18:33

Instrument :
BNA_G
ClientSampleId :
13-D

Tot Ion:152 Resp: 39661
Ion Ratio Lower Upper
152 100
150 155.4 119.5 179.3
115 57.1 49.6 74.4

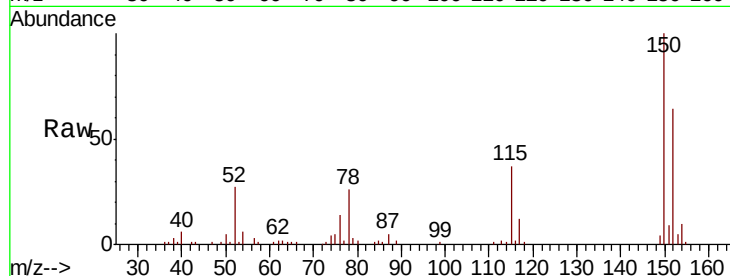


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

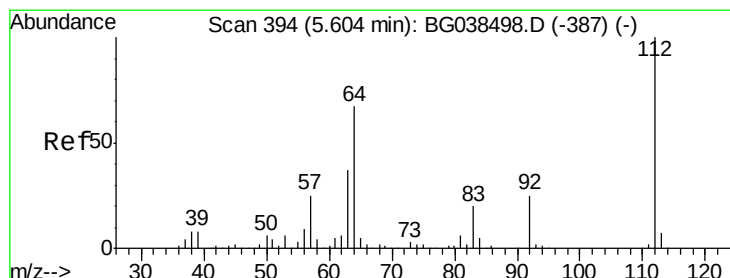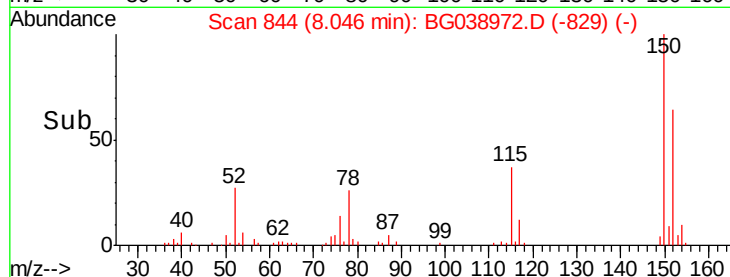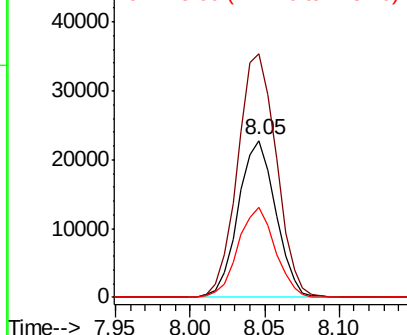



#5


2-Fluorophenol
Concen: 84.430 ng
RT: 5.60 min Scan# 428
Delta R.T. -0.00 min
Lab File: BG038972.D
Acq: 7 Jan 2019 18:33

Tgt Ion:112 Resp: 188796
Ion Ratio Lower Upper
112 100
64 65.7 53.4 80.2
63 38.7 29.3 43.9

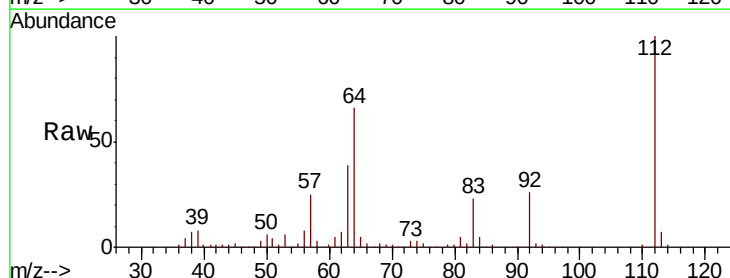

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

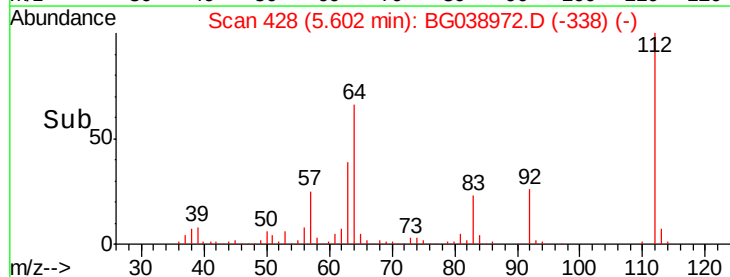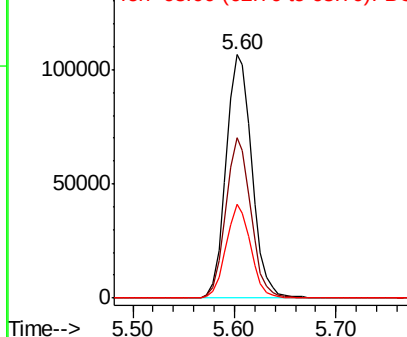

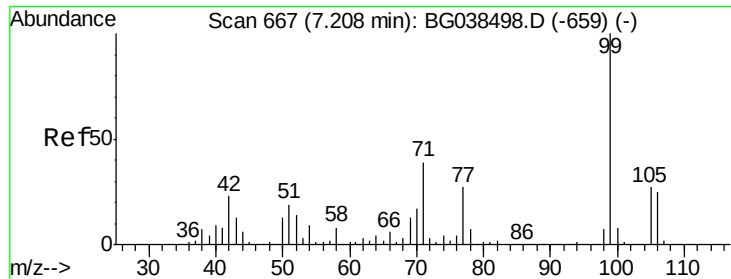

#7

Phenol-d6

Concen: 86.414 ng

RT: 7.21 min Scan# 701

Delta R.T. -0.00 min

Lab File: BG038972.D

Acq: 7 Jan 2019 18:33

Instrument :

BNA_G

ClientSampleId :

13-D


Tot Ion: 99 Resp: 265271

Ion Ratio Lower Upper

99 100

42 22.5 18.5 27.7

71 38.8 31.1 46.7



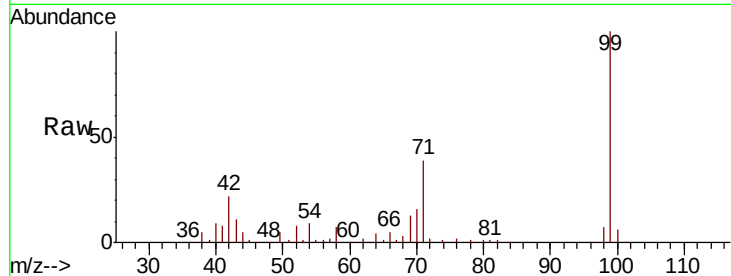


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

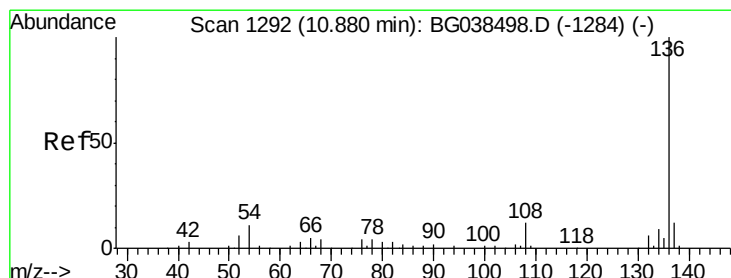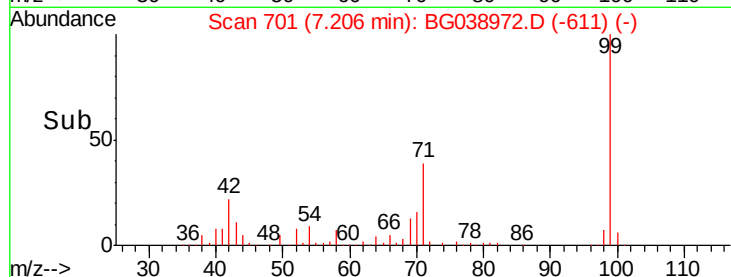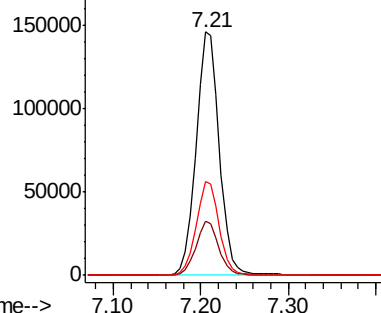

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BG038972.D

Acq: 7 Jan 2019 18:33

Tgt Ion: 136 Resp: 157319


Ion Ratio Lower Upper

136 100

137 11.5 9.3 13.9

54 9.4 8.5 12.7

68 4.4 3.5 5.3

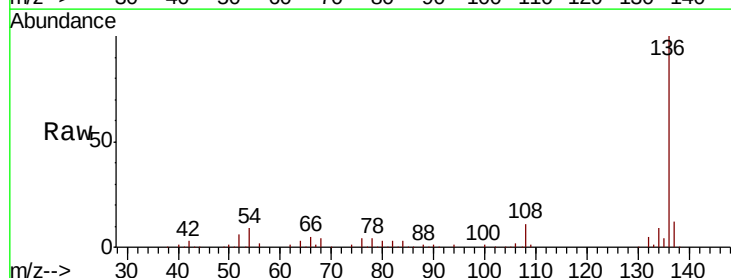



Abundance


Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



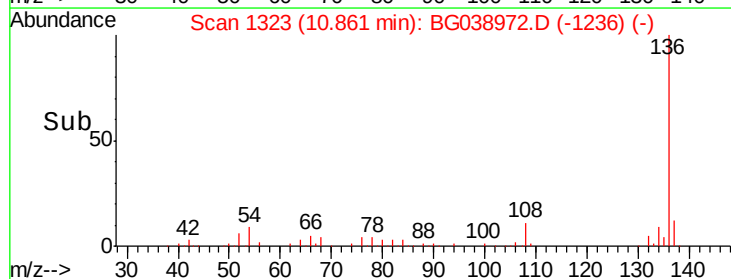
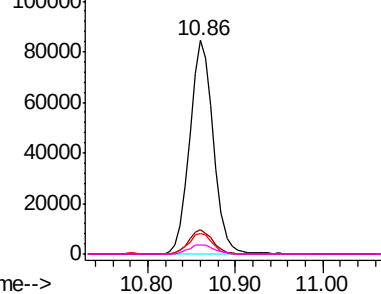


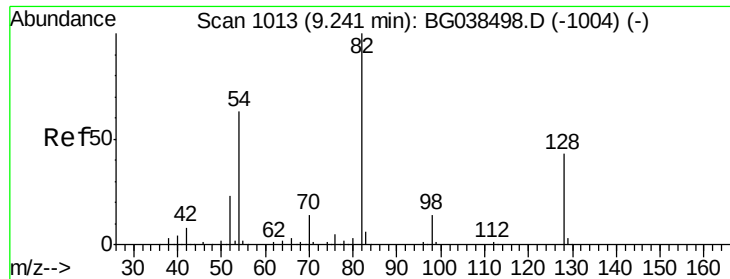

#23
 Nitrobenzene-d5
 Concen: 53.270 ng
 RT: 9.22 min Scan# 1044
 Delta R.T. -0.02 min
 Lab File: BG038972.D
 Acq: 7 Jan 2019 18:33




Instrument :
 BNA_G
 ClientSampleID :
 13-D


Tot Ion: 82 Resp: 164041
 Ion Ratio Lower Upper
 82 100
 128 45.9 34.6 52.0
 54 59.9 50.6 76.0

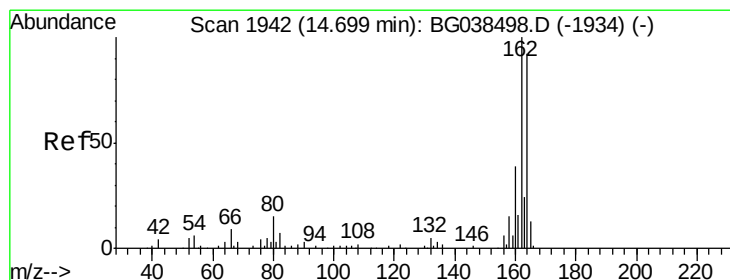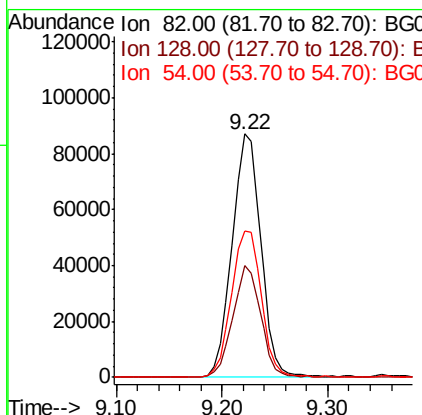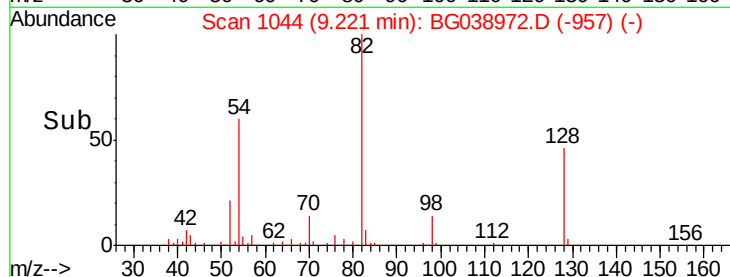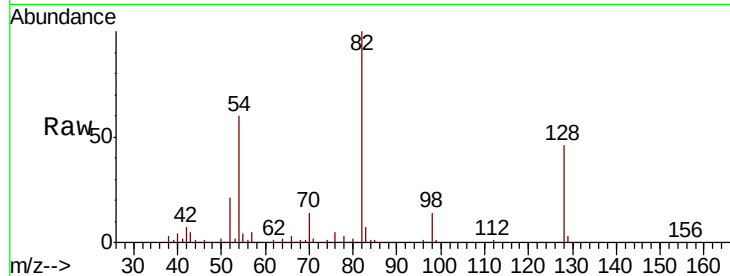

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.69 min Scan# 1974
 Delta R.T. -0.01 min
 Lab File: BG038972.D
 Acq: 7 Jan 2019 18:33

Tgt Ion:164 Resp: 100154
 Ion Ratio Lower Upper
 164 100
 162 102.0 86.6 130.0
 160 41.9 34.2 51.2

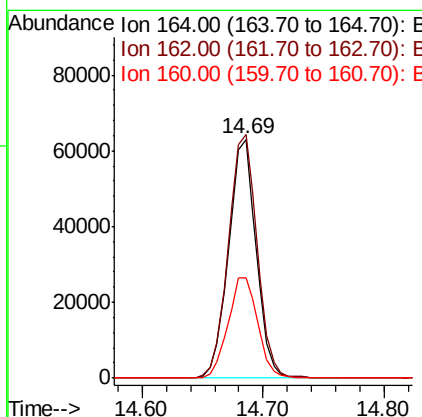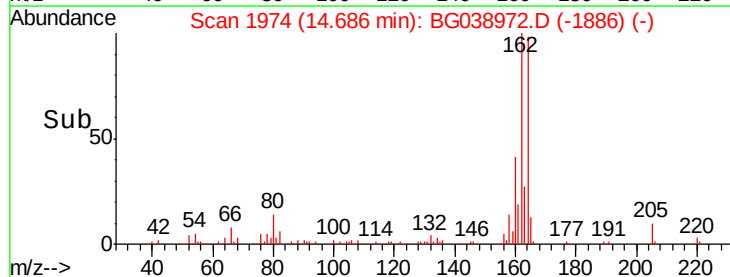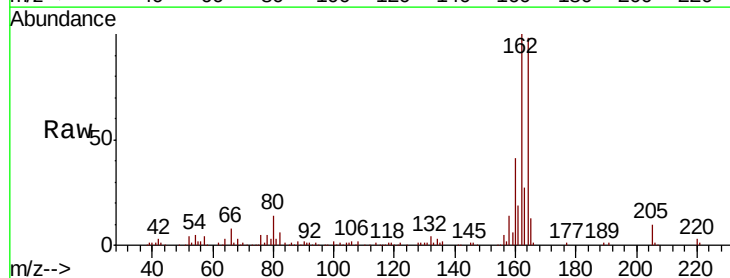


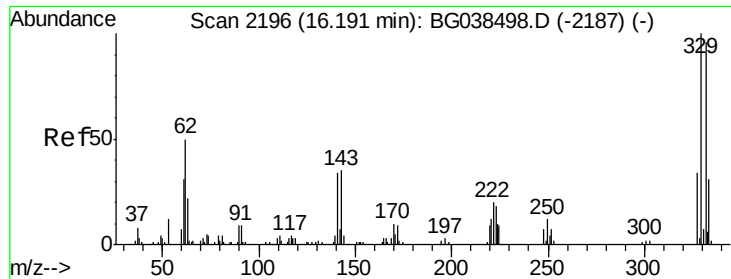

#42
 2,4,6-Tribromophenol
 Concen: 89.480 ng
 RT: 16.18 min Scan# 2228
 Delta R.T. -0.01 min
 Lab File: BG038972.D
 Acq: 7 Jan 2019 18:33

Instrument :
 BNA_G
 ClientSampled :
 13-D

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.4	76.9	115.3
141	33.6	28.8	43.2



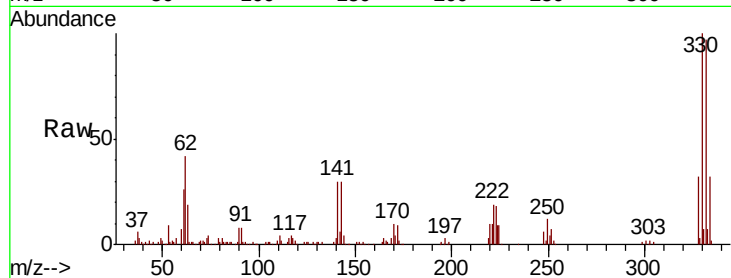


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

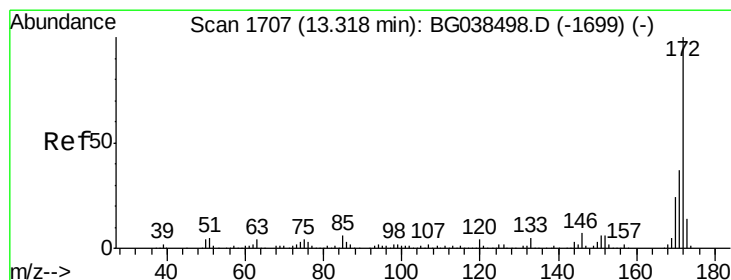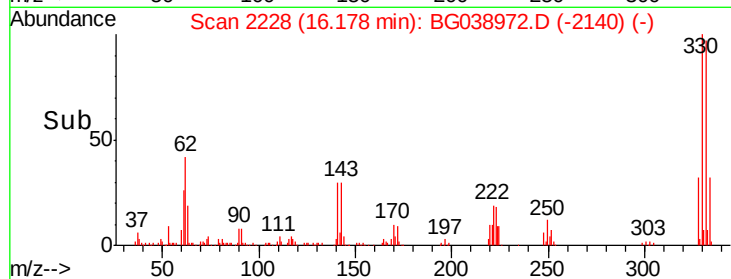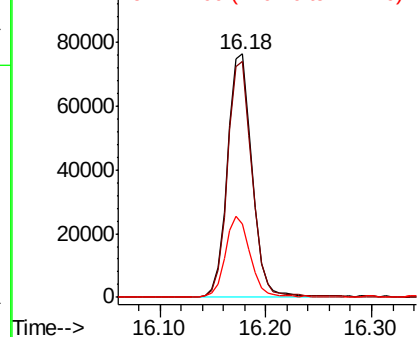

#45
 2-Fluorobiphenyl
 Concen: 61.575 ng
 RT: 13.30 min Scan# 1738
 Delta R.T. -0.02 min
 Lab File: BG038972.D
 Acq: 7 Jan 2019 18:33

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.8	44.6
170	24.3	19.5	29.3


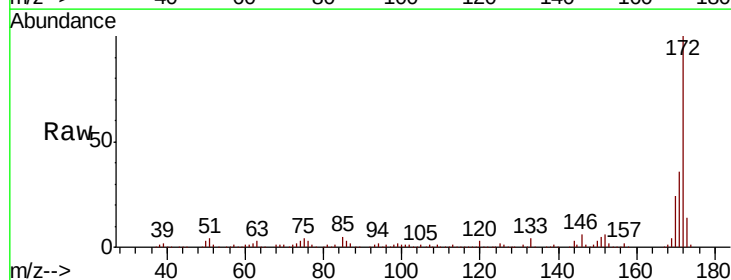



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

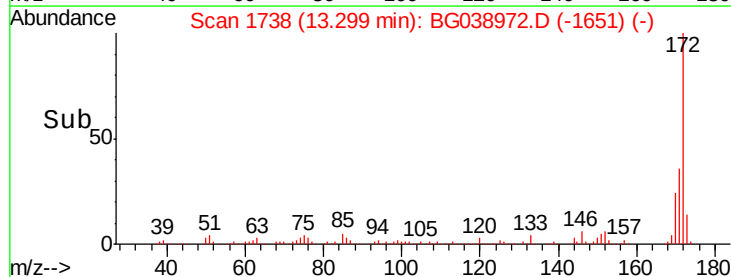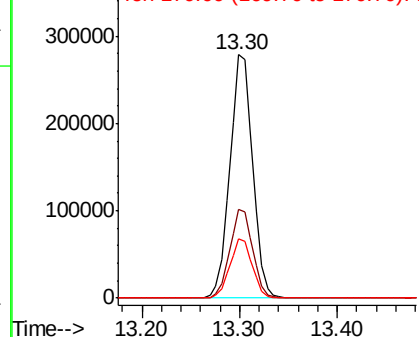


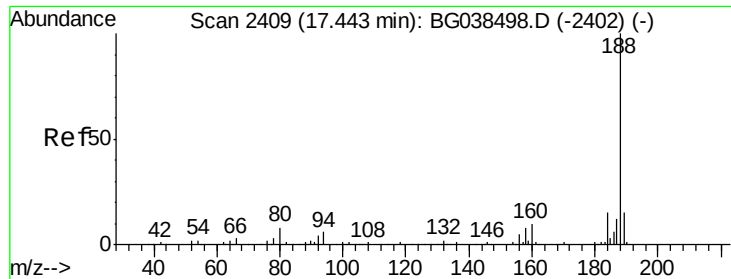




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.43 min Scan# 2441
Delta R.T. -0.01 min
Lab File: BG038972.D
Acq: 7 Jan 2019 18:33

Instrument :
BNA_G
ClientSampleId :
13-D

Tot Ion:188 Resp: 216303
Ion Ratio Lower Upper
188 100
94 5.4 5.1 7.7
80 6.6 6.1 9.1

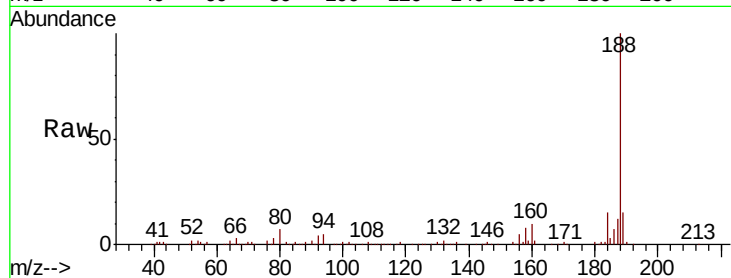


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

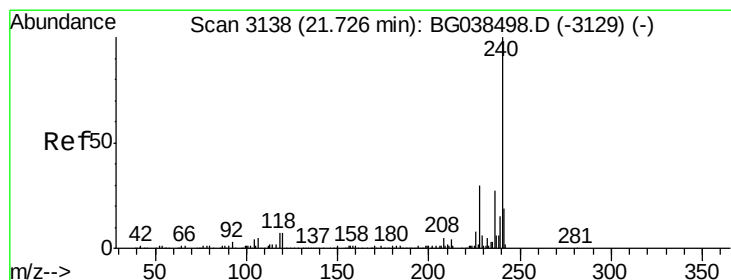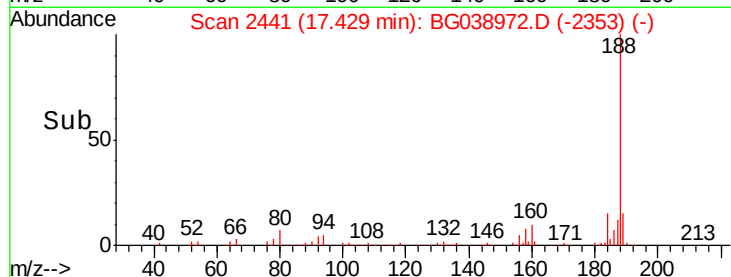
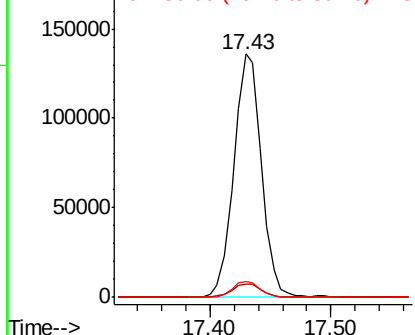



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.71 min Scan# 3169
Delta R.T. -0.02 min
Lab File: BG038972.D
Acq: 7 Jan 2019 18:33

Tgt Ion:240 Resp: 222621
Ion Ratio Lower Upper
240 100
120 6.1 5.3 7.9
236 26.4 21.4 32.2

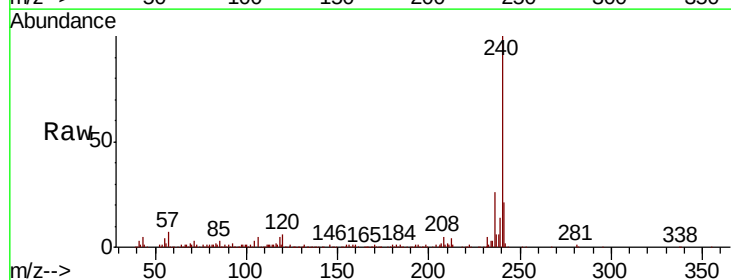

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

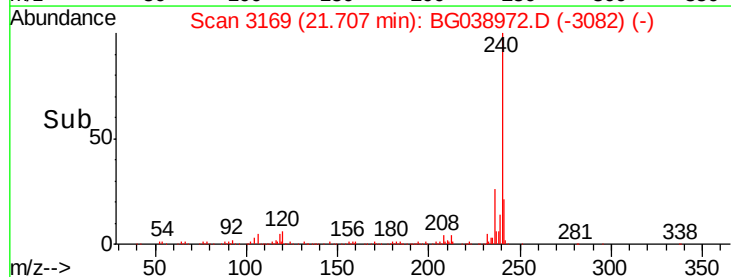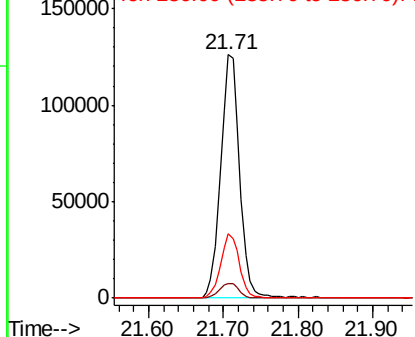

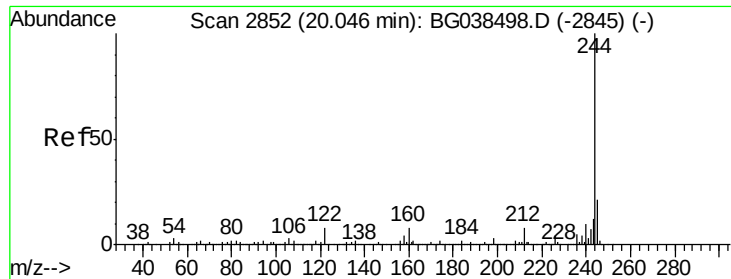

#79

Terphenyl-d14

Concen: 65.026 ng

RT: 20.03 min Scan# 2884

Delta R.T. -0.01 min

Lab File: BG038972.D

Acq: 7 Jan 2019 18:33

Instrument :

BNA_G

ClientSampleId :

13-D


Tot Ion:244 Resp: 665167

Ion Ratio Lower Upper

244 100

212 7.6 6.2 9.2




122 6.8 6.3 9.5

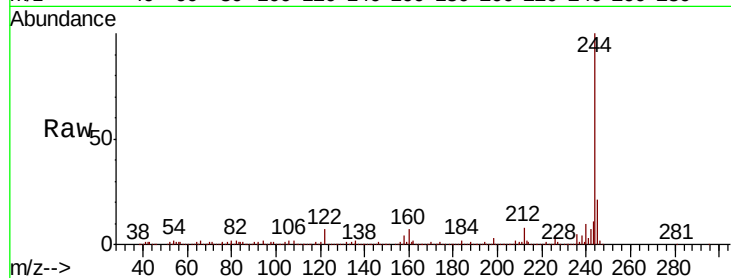

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

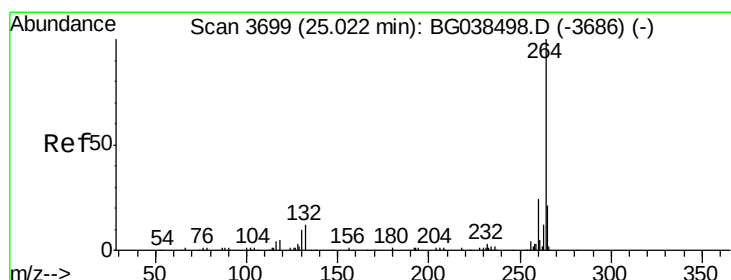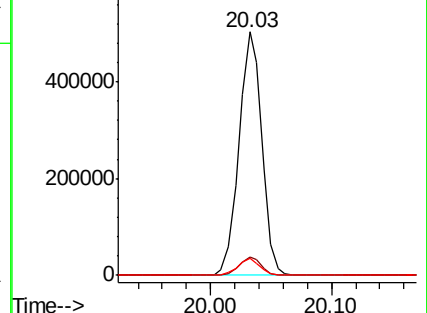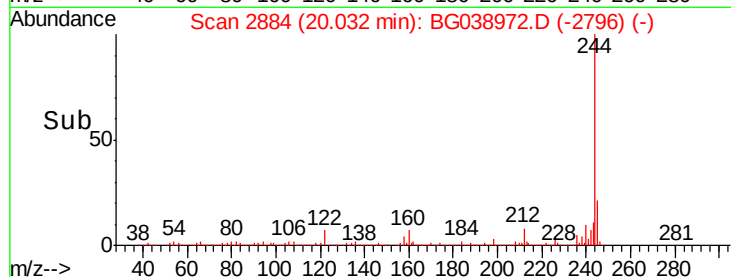

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.00 min Scan# 3729

Delta R.T. -0.03 min

Lab File: BG038972.D

Acq: 7 Jan 2019 18:33


Tgt Ion:264 Resp: 229828

Ion Ratio Lower Upper

264 100

260 23.0 18.9 28.3

265 20.6 17.0 25.4

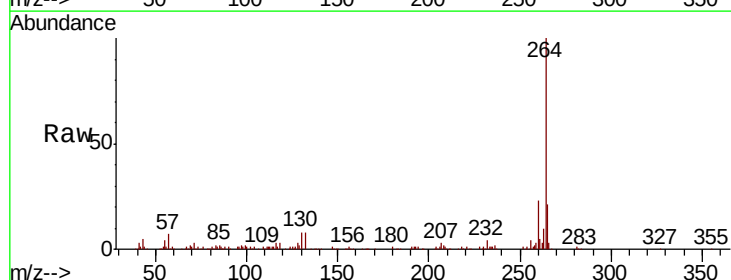

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

