

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010719\
 Data File : BG038992.D
 Acq On : 8 Jan 2019 12:13
 Operator : JU/SJ
 Sample : K1034-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-3

Quant Time: Jan 08 13:11:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	28352	20.00	ng	-0.01
21) Naphthalene-d8	10.86	136	110072	20.00	ng	-0.02
39) Acenaphthene-d10	14.68	164	72181	20.00	ng	-0.02
64) Phenanthrene-d10	17.43	188	176295	20.00	ng	-0.01
76) Chrysene-d12	21.71	240	176807	20.00	ng	-0.02
87) Perylene-d12	25.00	264	186345	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	114596	71.69	ng	0.00
7) Phenol-d6	7.21	99	157798	71.91	ng	0.00
23) Nitrobenzene-d5	9.22	82	96356	44.72	ng	-0.02
42) 2,4,6-Tribromophenol	16.18	330	76896	77.30	ng	-0.01
45) 2-Fluorobiphenyl	13.30	172	263371	50.06	ng	-0.02
79) Terphenyl-d14	20.03	244	457129	56.27	ng	-0.01
Target Compounds						
10) Phenol	7.23	94	7324	3.141	ng	90
50) Dimethylphthalate	14.13	163	35522	6.026	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010719\
Data File : BG038992.D
Acq On : 8 Jan 2019 12:13
Operator : JU/SJ
Sample : K1034-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

Quant Time: Jan 08 13:11:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

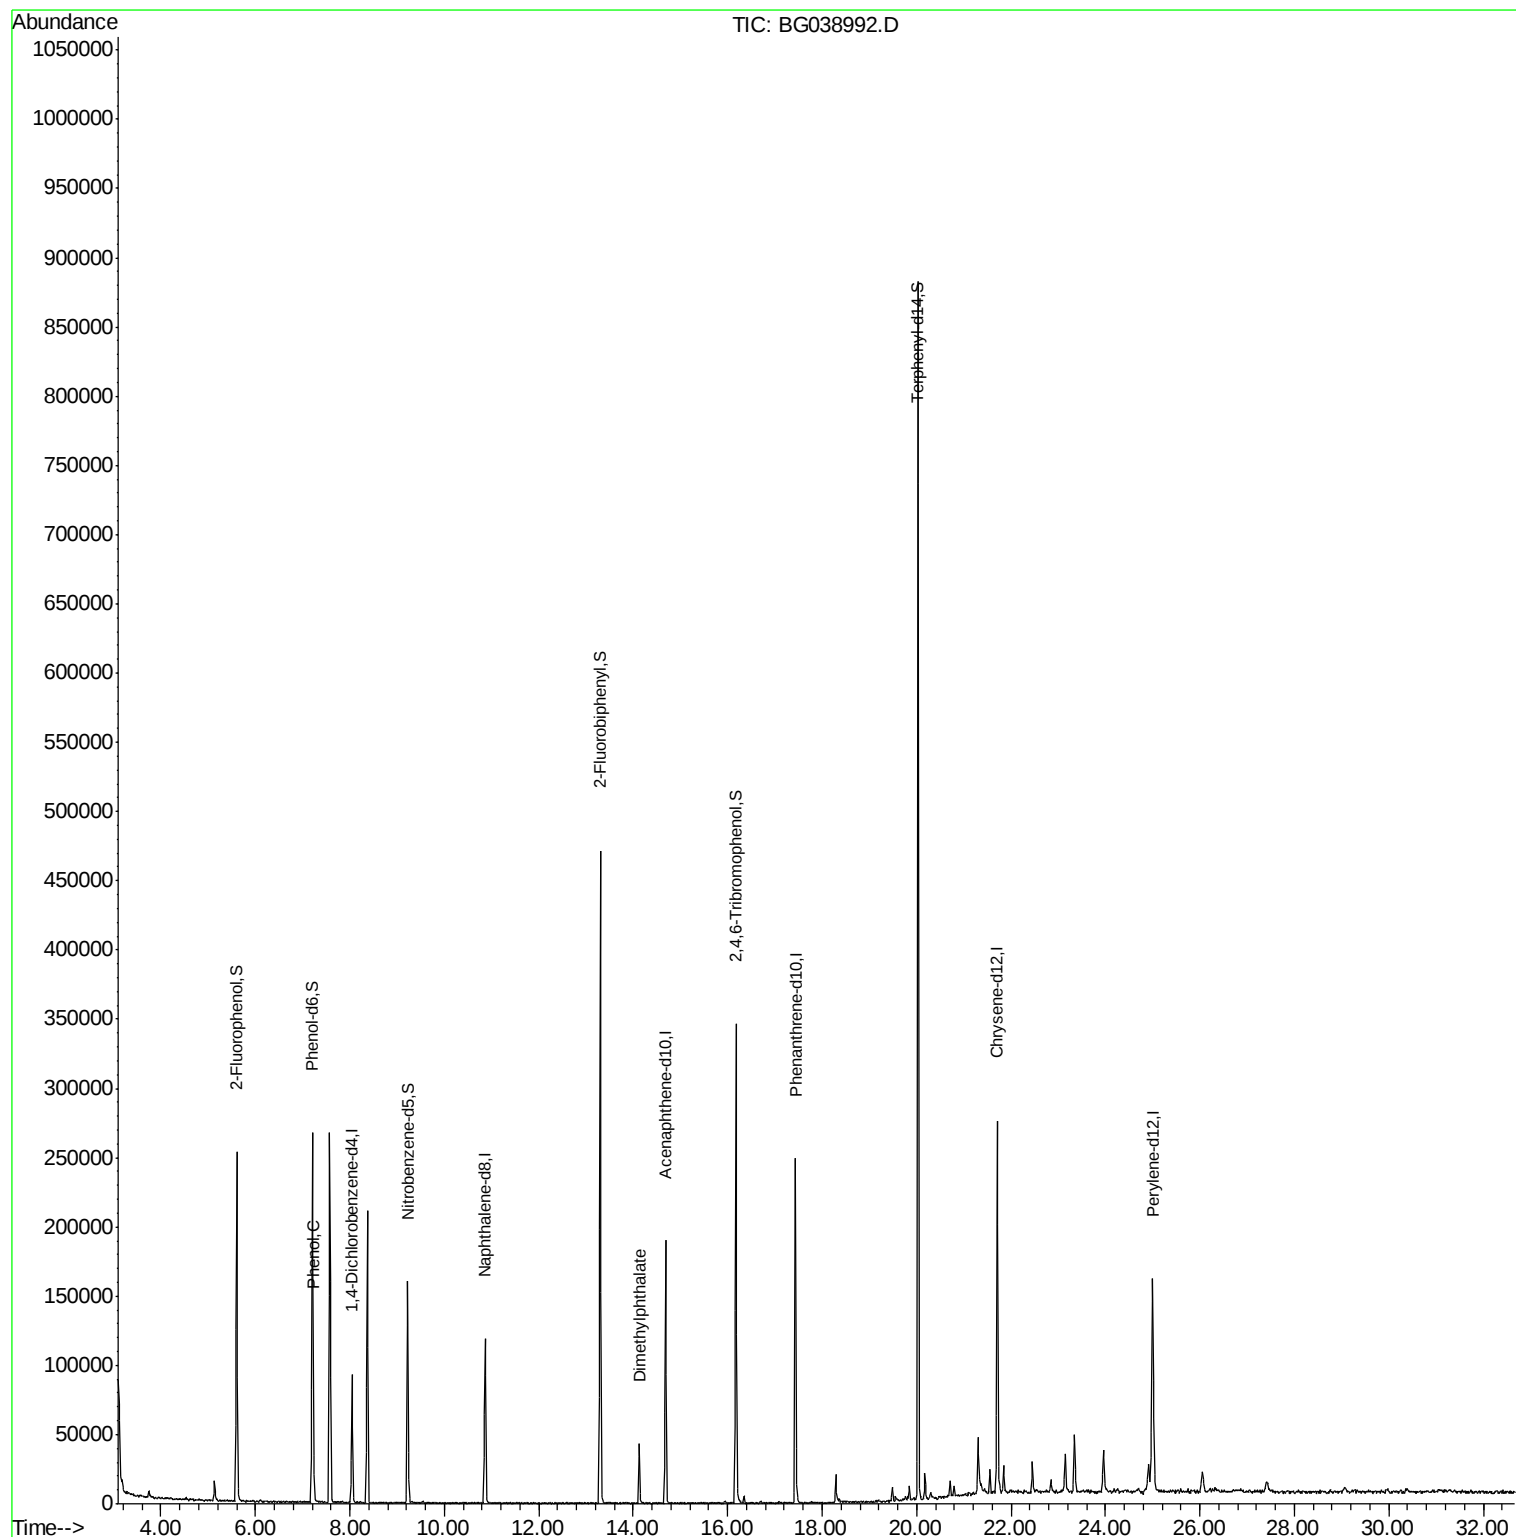




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 844
Delta R.T. -0.01 min
Lab File: BG038992.D
Acq: 8 Jan 2019 12:13

Instrument :
BNA_G
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

Tot Ion:152 Resp: 28352
Ion Ratio Lower Upper
152 100
150 156.1 119.5 179.3
115 52.5 49.6 74.4

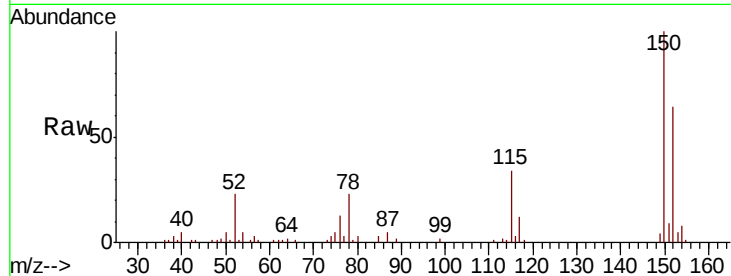


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

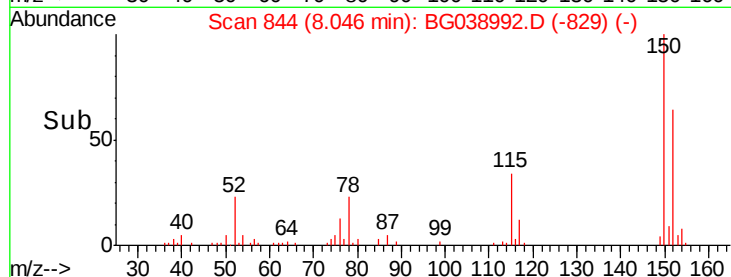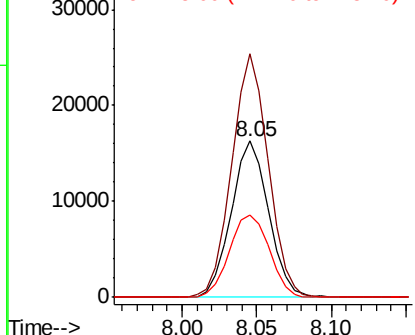



#5

2-Fluorophenol
Concen: 71.689 ng
RT: 5.60 min Scan# 428
Delta R.T. -0.00 min
Lab File: BG038992.D
Acq: 8 Jan 2019 12:13

Tgt Ion:112 Resp: 114596
Ion Ratio Lower Upper
112 100
64 62.5 53.4 80.2
63 37.1 29.3 43.9

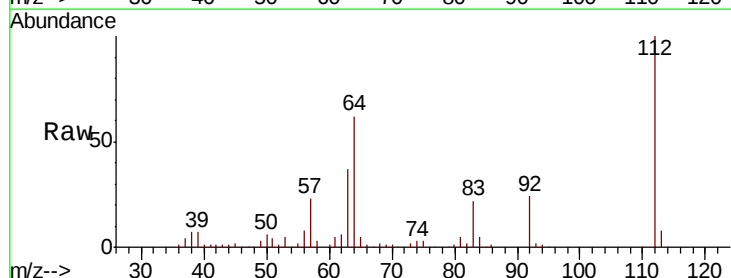

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

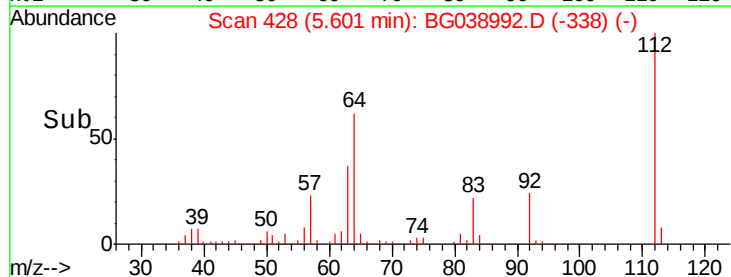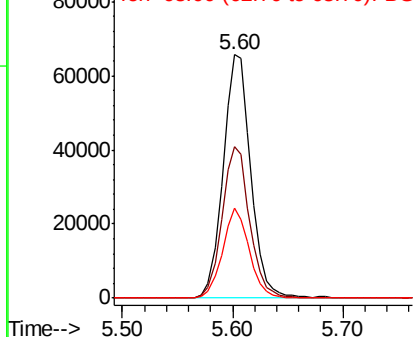



#7

Phenol-d6

Concen: 71.908 ng

RT: 7.21 min Scan# 701

Delta R.T. -0.00 min

Lab File: BG038992.D

Acq: 8 Jan 2019 12:13

Instrument :

BNA_G

ClientSampleId :

CONTROL-HOUSE-WALL-1-3


Tot Ion: 99 Resp: 157798

Ion Ratio Lower Upper



99 100

42 20.9 18.5 27.7

71 38.4 31.1 46.7

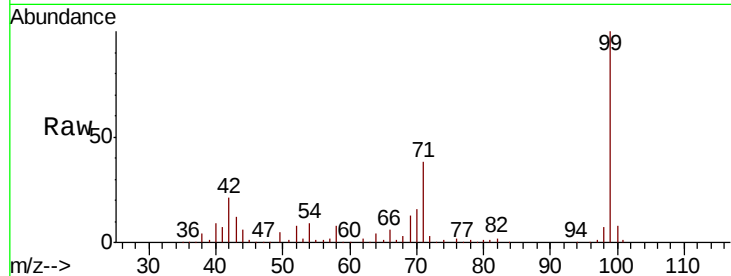

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

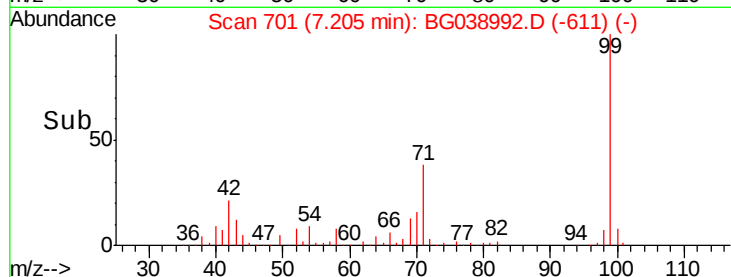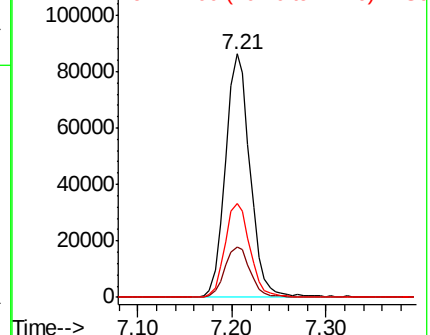

#10

Phenol

Concen: 3.141 ng

RT: 7.23 min Scan# 705

Delta R.T. -0.01 min

Lab File: BG038992.D

Acq: 8 Jan 2019 12:13


Tgt Ion: 94 Resp: 7324

Ion Ratio Lower Upper



94 100


65 35.0 12.6 52.6

66 53.3 24.1 64.1

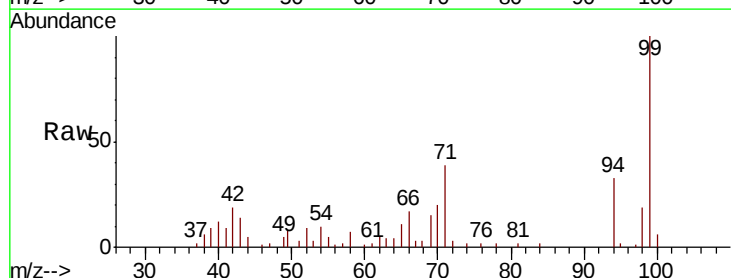

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC



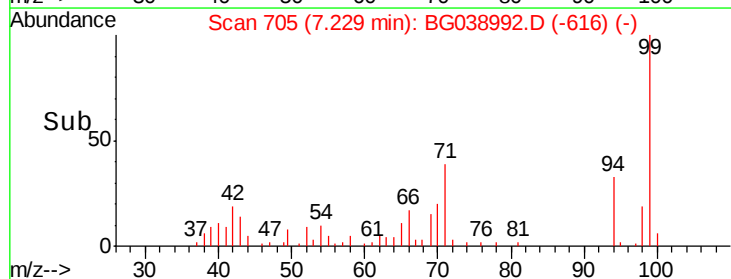
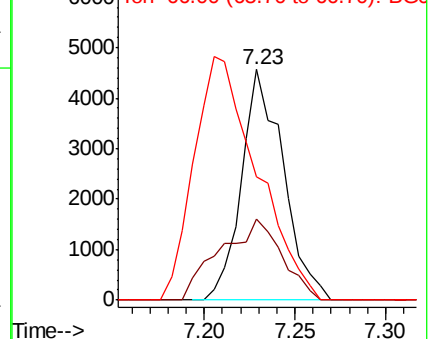


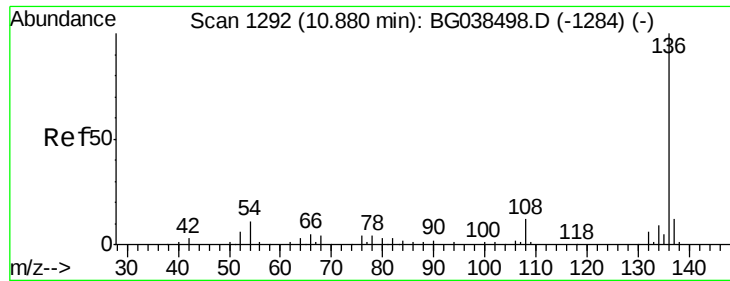

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.86 min Scan# 1323
Delta R.T. -0.02 min
Lab File: BG038992.D
Acq: 8 Jan 2019 12:13




Instrument :
BNA_G
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

Tot Ion:136	Resp:	110072
Ion	Ratio	Lower Upper
136	100	
137	12.1	9.3 13.9
54	10.2	8.5 12.7
68	3.9	3.5 5.3

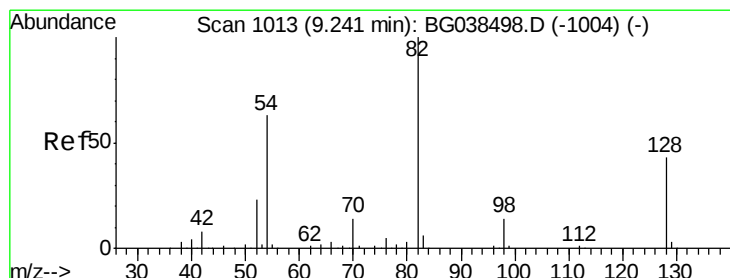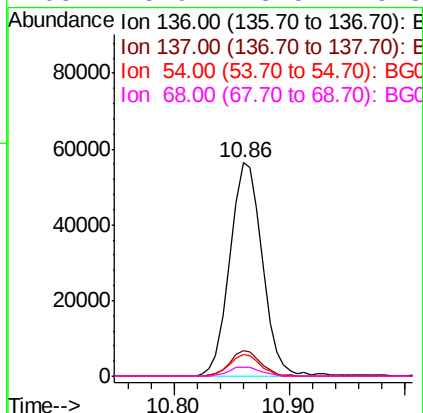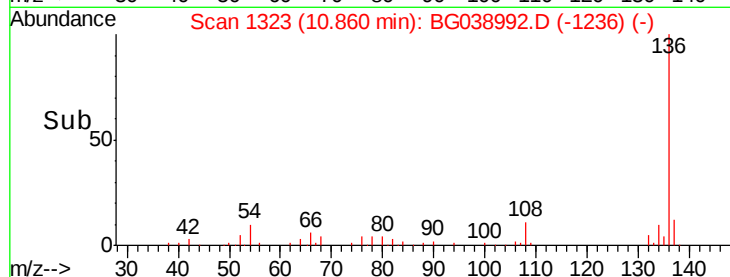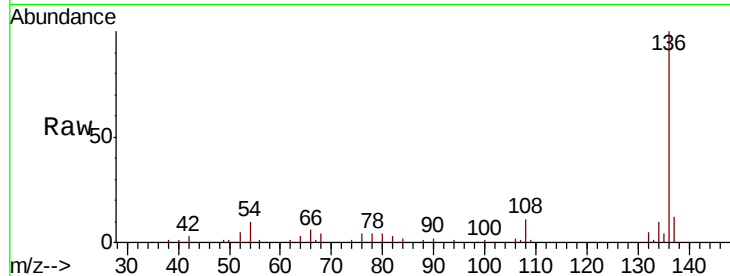

#23
Nitrobenzene-d5
Concen: 44.721 ng
RT: 9.22 min Scan# 1044
Delta R.T. -0.02 min
Lab File: BG038992.D
Acq: 8 Jan 2019 12:13

Tgt Ion: 82	Resp:	96356
Ion	Ratio	Lower Upper
82	100	
128	43.1	34.6 52.0
54	60.8	50.6 76.0

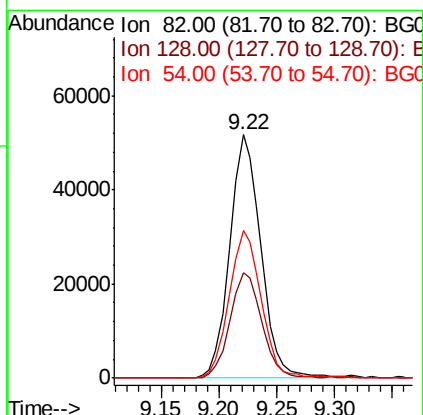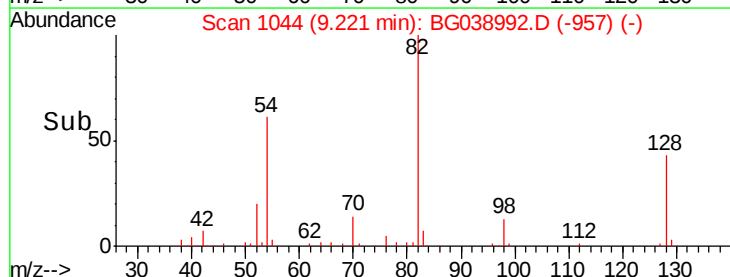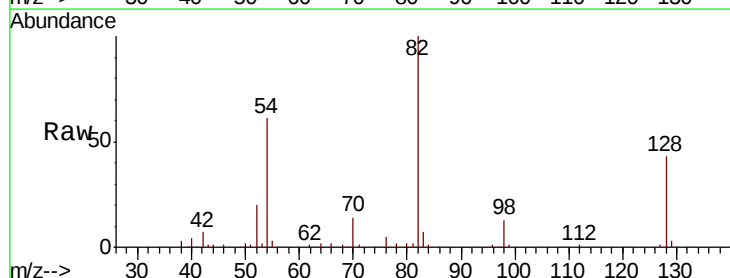



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.68 min Scan# 1973

Delta R.T. -0.02 min

Lab File: BG038992.D

Acq: 8 Jan 2019 12:13

Instrument :

BNA_G

ClientSampleId :

CONTROL-HOUSE-WALL-1-3


Tot Ion:164 Resp: 72181

Ion Ratio Lower Upper

164 100

162 100.2 86.6 130.0




160 43.5 34.2 51.2

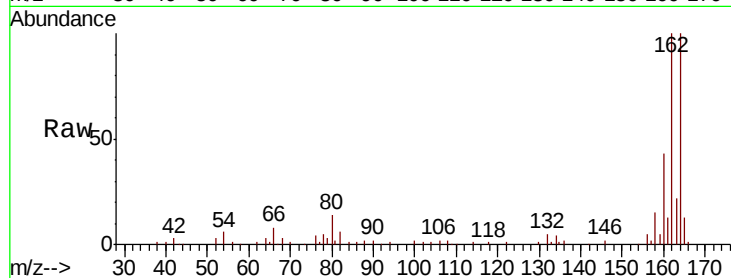

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

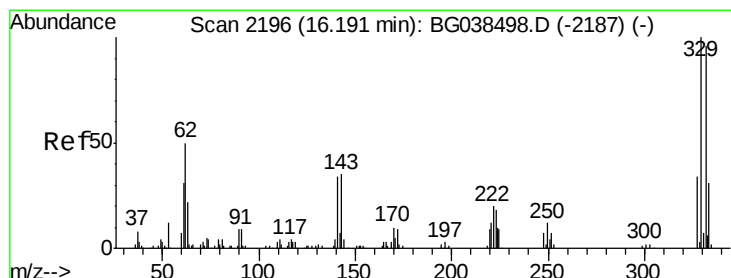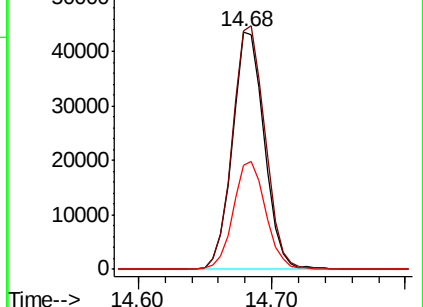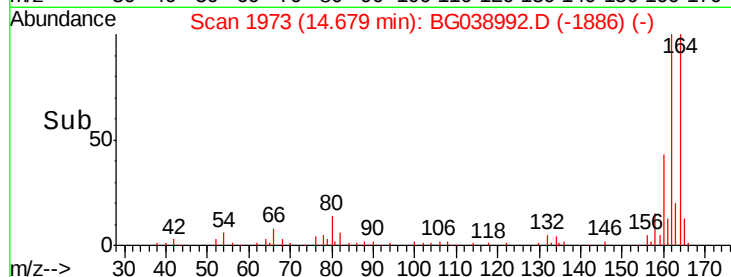

#42

2,4,6-Tribromophenol

Concen: 77.299 ng

RT: 16.18 min Scan# 2228

Delta R.T. -0.01 min

Lab File: BG038992.D

Acq: 8 Jan 2019 12:13


Tgt Ion:330 Resp: 76896

Ion Ratio Lower Upper

330 100

332 97.6 76.9 115.3



141 32.8 28.8 43.2

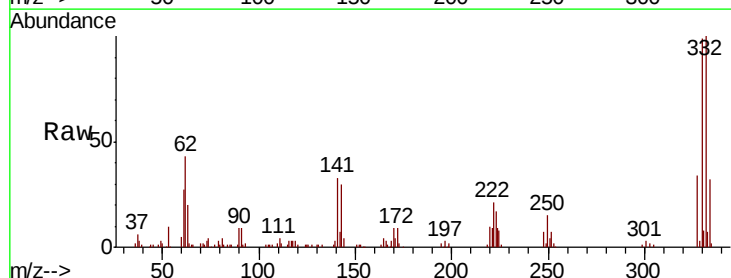


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



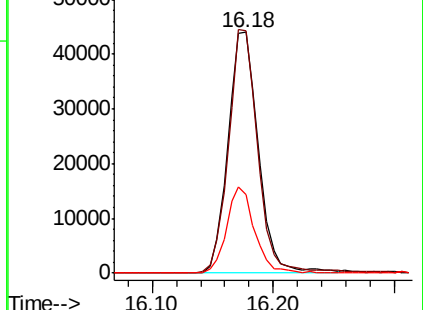
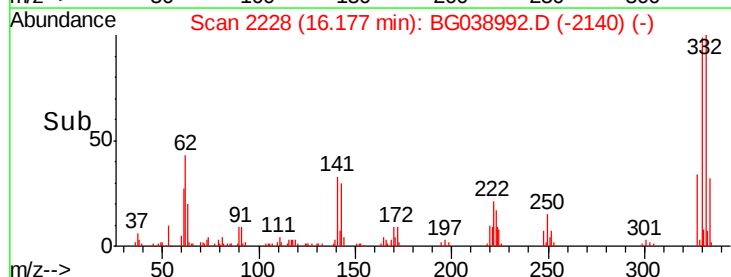


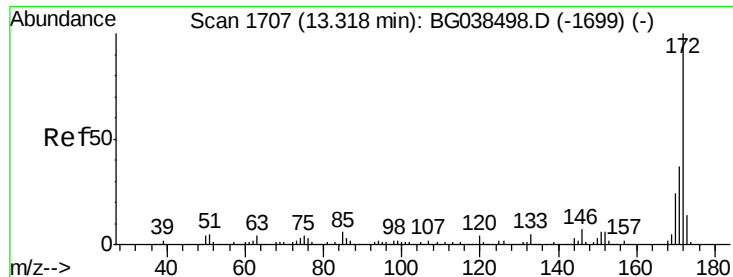

#45
2-Fluorobiphenyl
Concen: 50.055 ng
RT: 13.30 min Scan# 1738
Delta R.T. -0.02 min
Lab File: BG038992.D
Acq: 8 Jan 2019 12:13




Instrument :
BNA_G
ClientSampleId :
CONTROL-HOUSE-WALL-1-3


Tot Ion:172 Resp: 263371
Ion Ratio Lower Upper
172 100
171 36.7 29.8 44.6
170 23.8 19.5 29.3

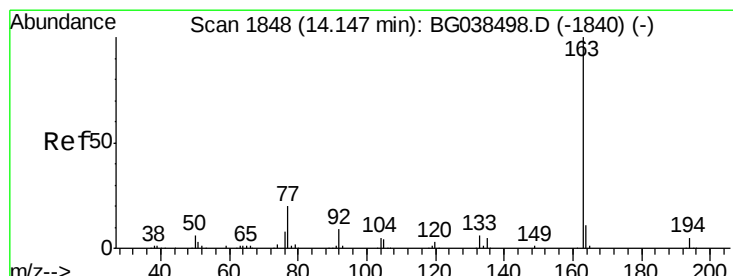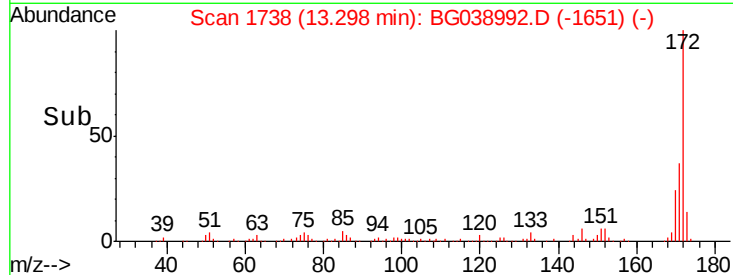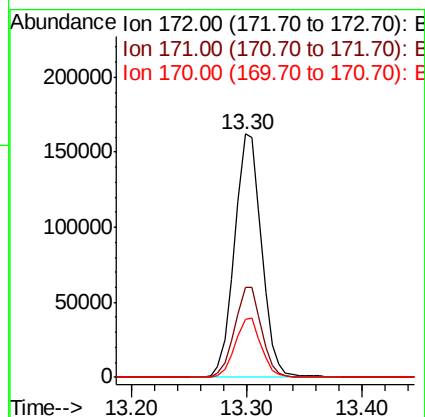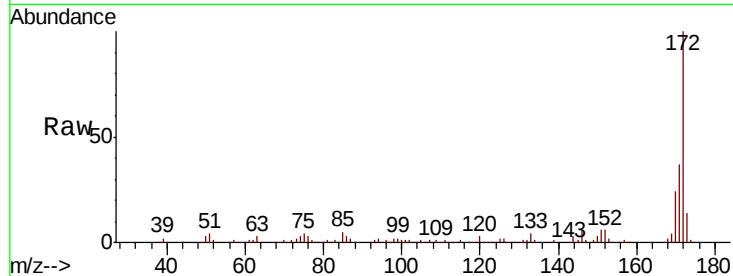

#50
Dimethylphthalate
Concen: 6.026 ng
RT: 14.13 min Scan# 1879
Delta R.T. -0.02 min
Lab File: BG038992.D
Acq: 8 Jan 2019 12:13

Tgt Ion:163 Resp: 35522
Ion Ratio Lower Upper
163 100
194 5.2 3.7 5.5
164 9.7 8.6 12.8

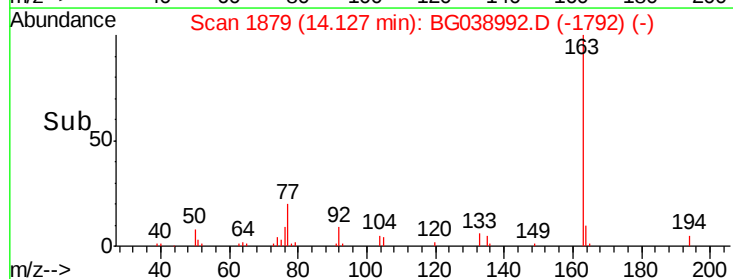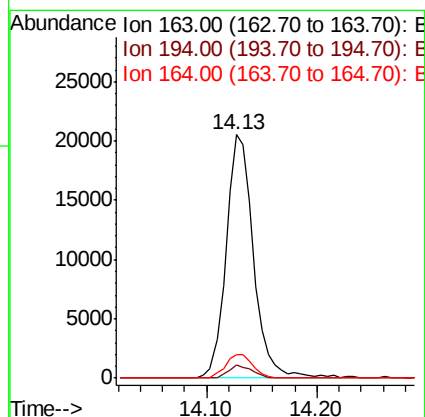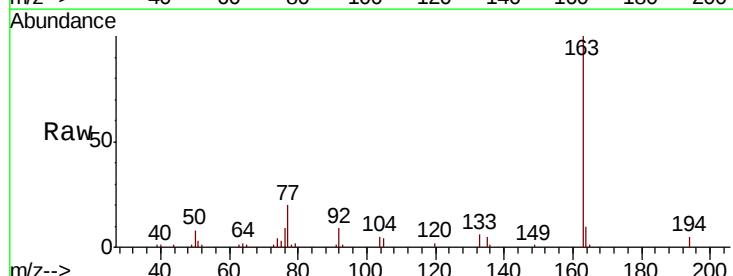


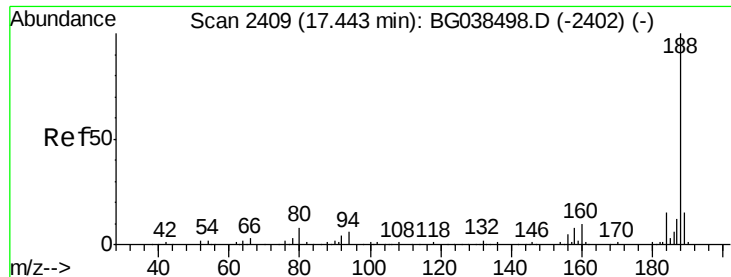




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.43 min Scan# 2441
Delta R.T. -0.01 min
Lab File: BG038992.D
Acq: 8 Jan 2019 12:13

Instrument :
BNA_G
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

Tot Ion:188 Resp: 176295
Ion Ratio Lower Upper
188 100
94 5.6 5.1 7.7
80 6.7 6.1 9.1

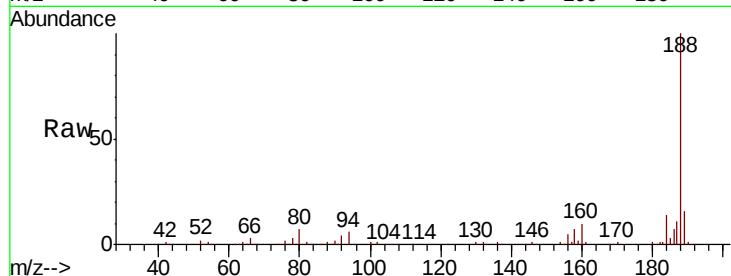


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

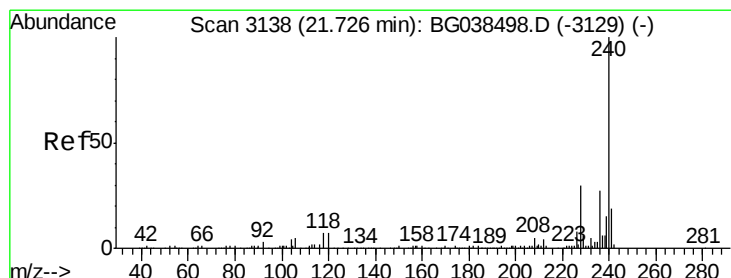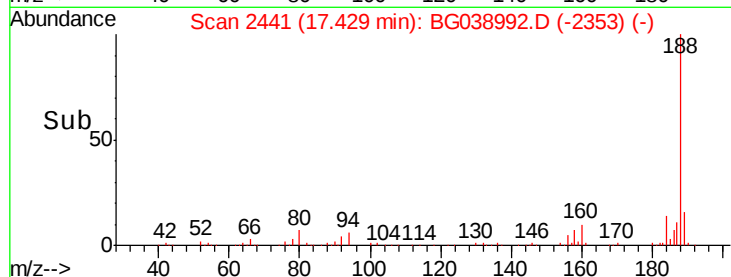
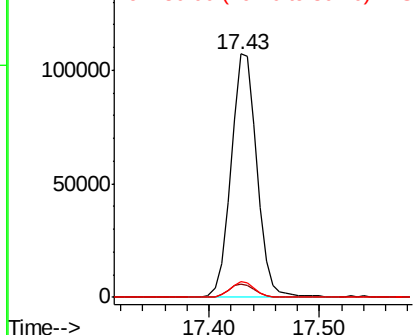



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.71 min Scan# 3169
Delta R.T. -0.02 min
Lab File: BG038992.D
Acq: 8 Jan 2019 12:13

Tgt Ion:240 Resp: 176807
Ion Ratio Lower Upper
240 100
120 6.5 5.3 7.9
236 26.3 21.4 32.2

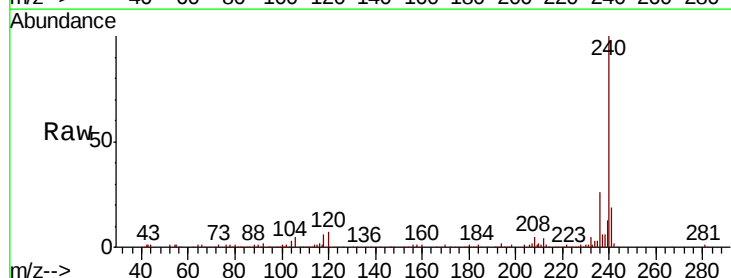

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

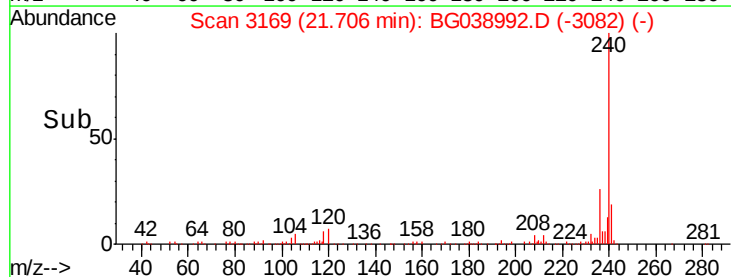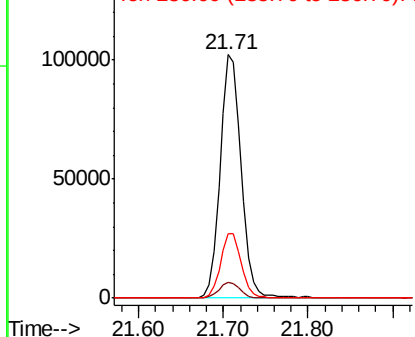

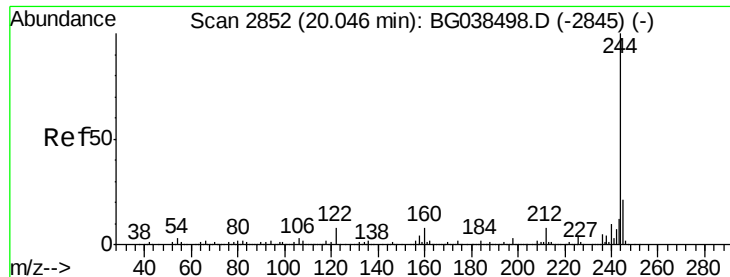

#79

Terphenyl-d14

Concen: 56.268 ng

RT: 20.03 min Scan# 2884

Delta R.T. -0.01 min

Lab File: BG038992.D

Acq: 8 Jan 2019 12:13

Instrument :

BNA_G

ClientSampleId :

CONTROL-HOUSE-WALL-1-3


Tot Ion:244 Resp: 457129

Ion Ratio Lower Upper

244 100

212 7.3 6.2 9.2




122 7.1 6.3 9.5

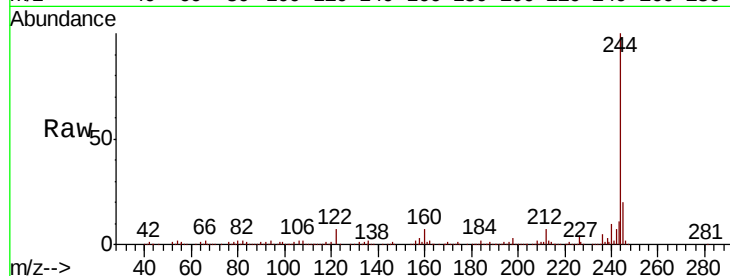

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

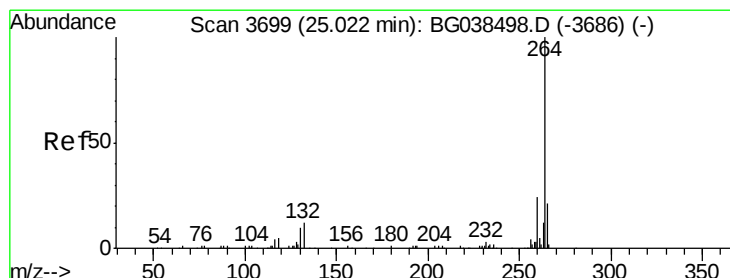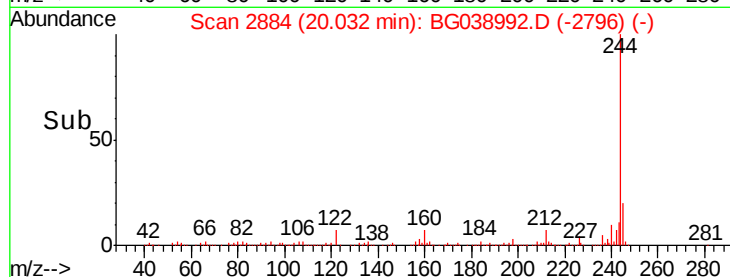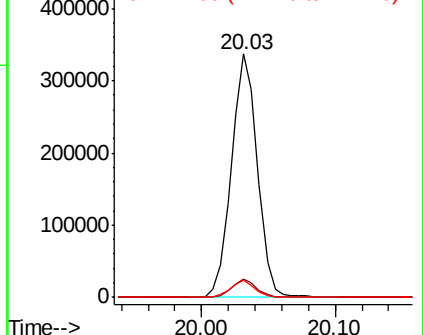

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.00 min Scan# 3729

Delta R.T. -0.03 min

Lab File: BG038992.D

Acq: 8 Jan 2019 12:13


Tgt Ion:264 Resp: 186345

Ion Ratio Lower Upper

264 100

260 24.2 18.9 28.3

265 22.0 17.0 25.4

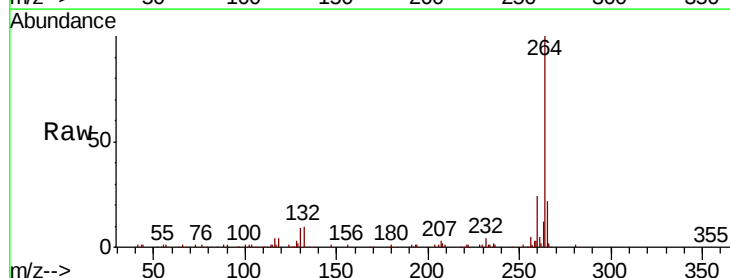

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

