


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010719\
 Data File : BG038966.D
 Acq On : 7 Jan 2019 14:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

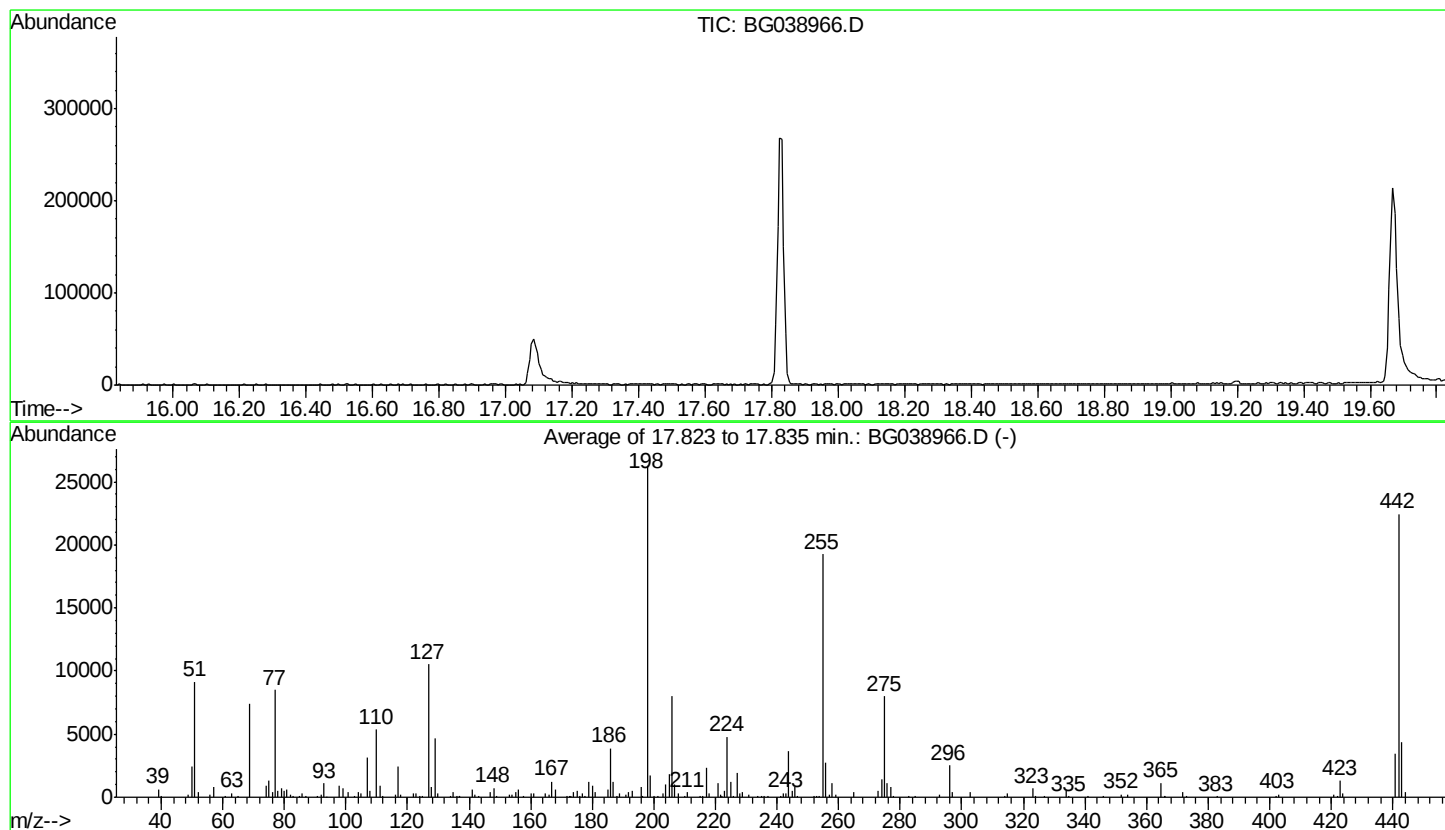

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	9133	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.3	7434	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.0	10505	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26272	PASS
199	198	5	9	6.5	1700	PASS
275	198	10	60	30.4	7996	PASS
365	198	1	100	4.4	1159	PASS
441	198	0.01	100	13.2	3479	PASS
442	198	50	100	85.5	22464	PASS
443	442	15	24	19.3	4339	PASS