


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG010719\
 Data File : BG038985.D
 Acq On : 8 Jan 2019 5:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

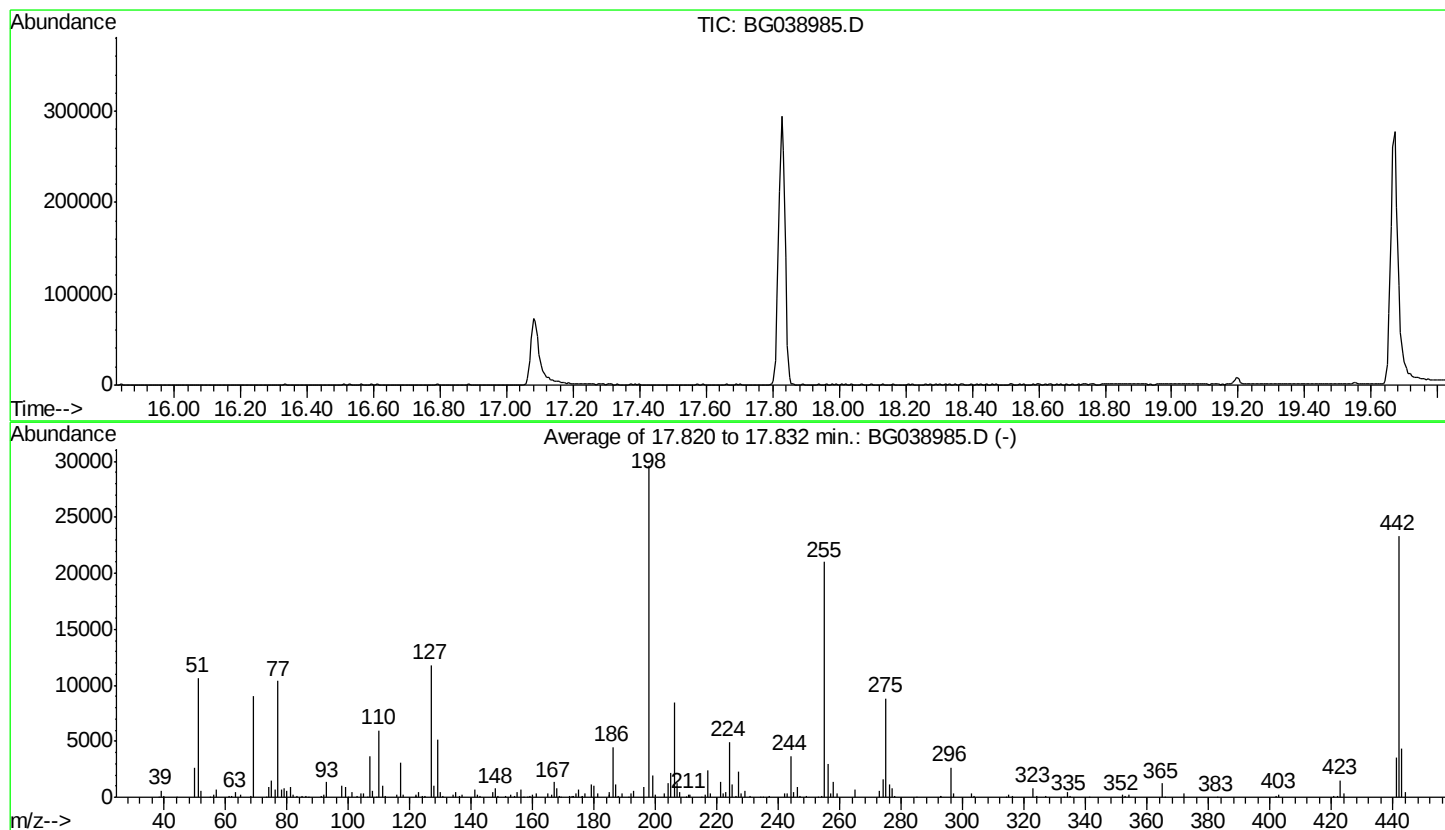

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	10648	PASS
68	69	0.00	2	1.7	158	PASS
69	198	0.00	100	30.5	9037	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.9	11823	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29629	PASS
199	198	5	9	6.6	1951	PASS
275	198	10	60	29.9	8853	PASS
365	198	1	100	4.2	1254	PASS
441	198	0.01	100	12.1	3591	PASS
442	198	50	100	78.9	23389	PASS
443	442	15	24	18.5	4323	PASS