
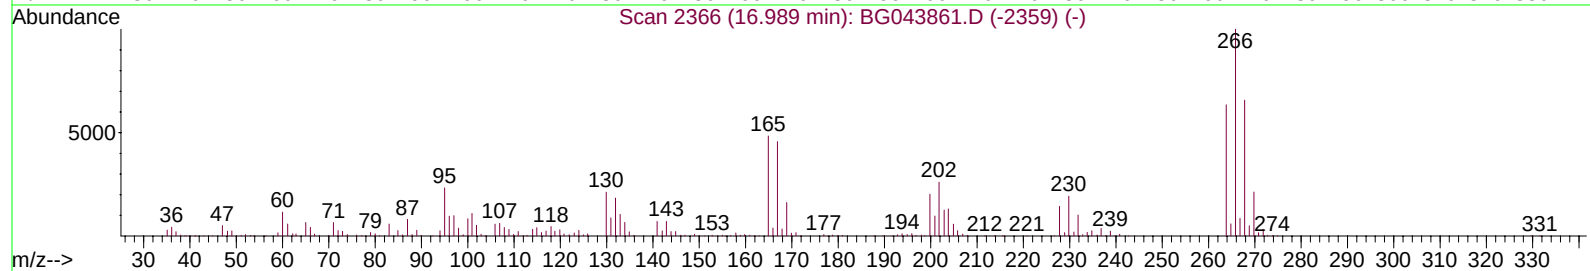
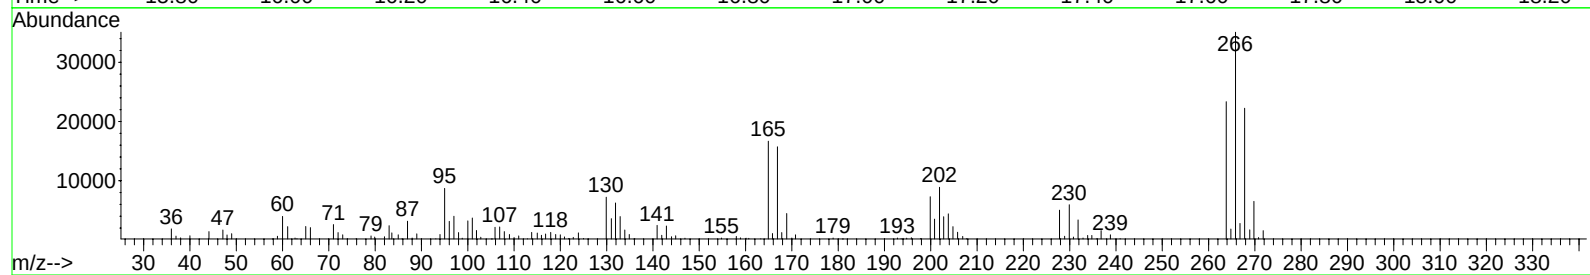


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010720\
Data File : BG043947.D
Acq On : 7 Jan 2020 9:20
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 17:56:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

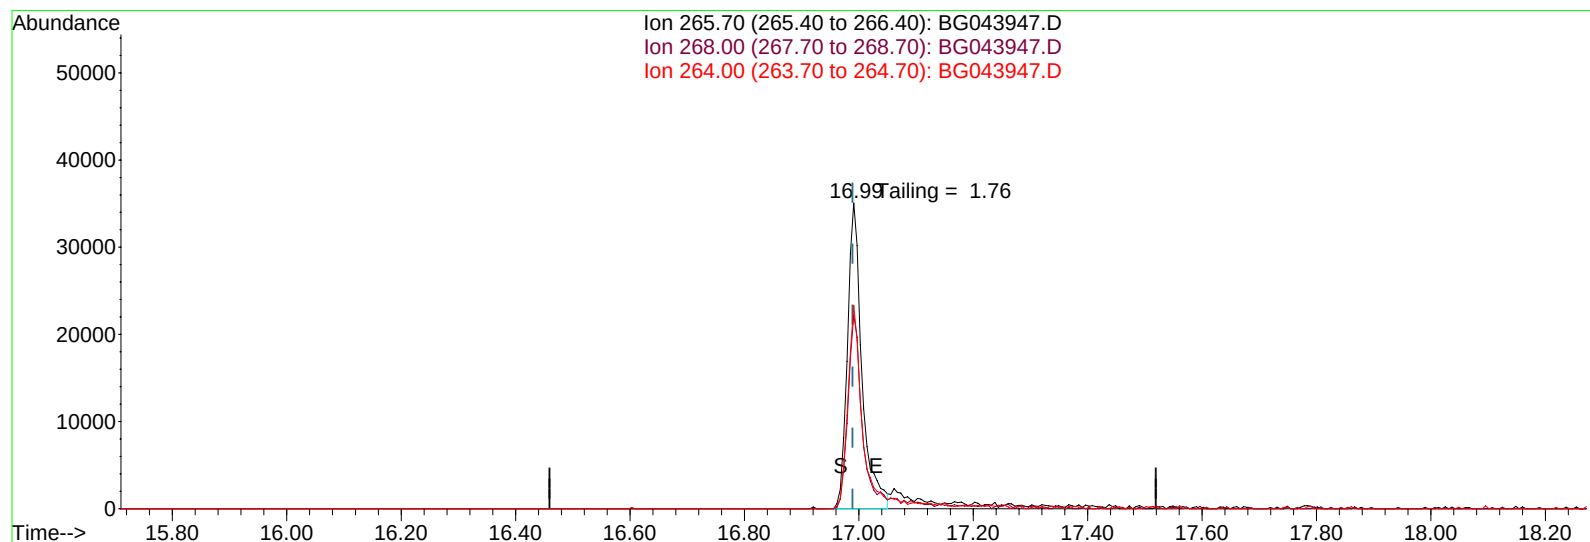

TIC: BG043947.D

(70) Pentachlorophenol (C)




16.991min (+0.002) 22860.66ng

response 63227

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	63.39
264.00	63.50	66.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010720\
Data File : BG043947.D
Acq On : 7 Jan 2020 9:20
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 17:56:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

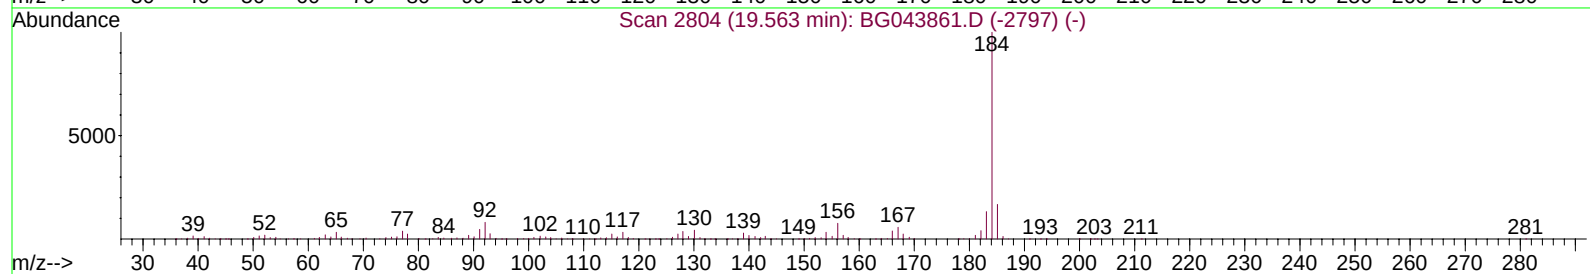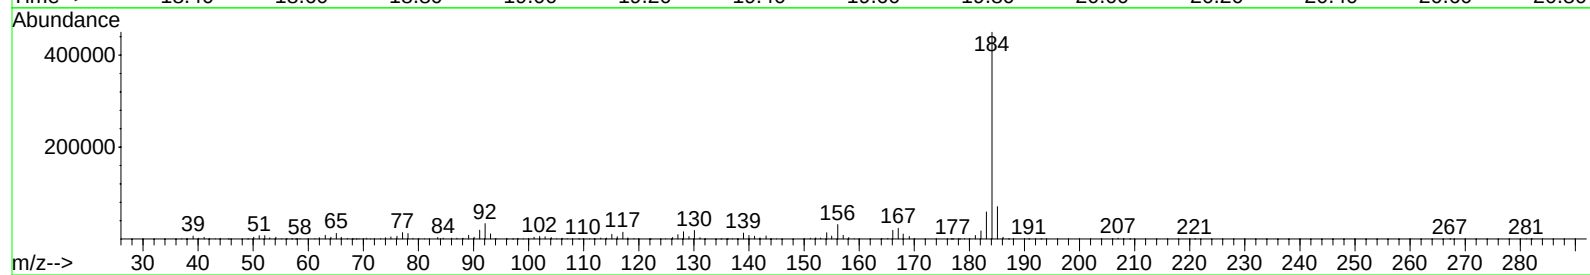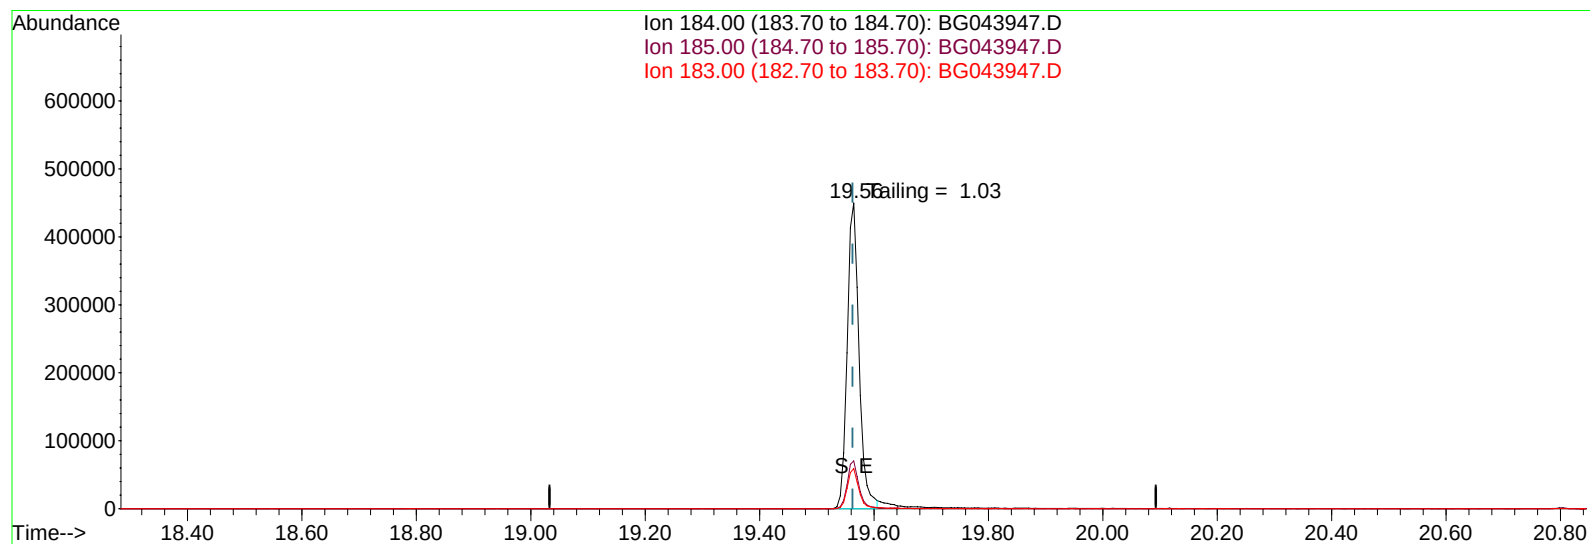

TIC: BG043947.D

(77) Benzidine

19.564min (+0.002) 115204.51ng

response 668916

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.63
183.00	13.20	13.11
0.00	0.00	0.00