
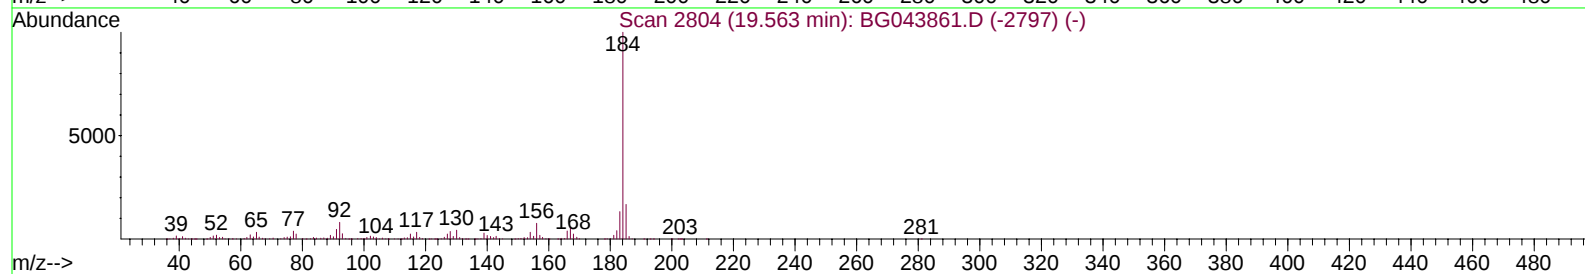
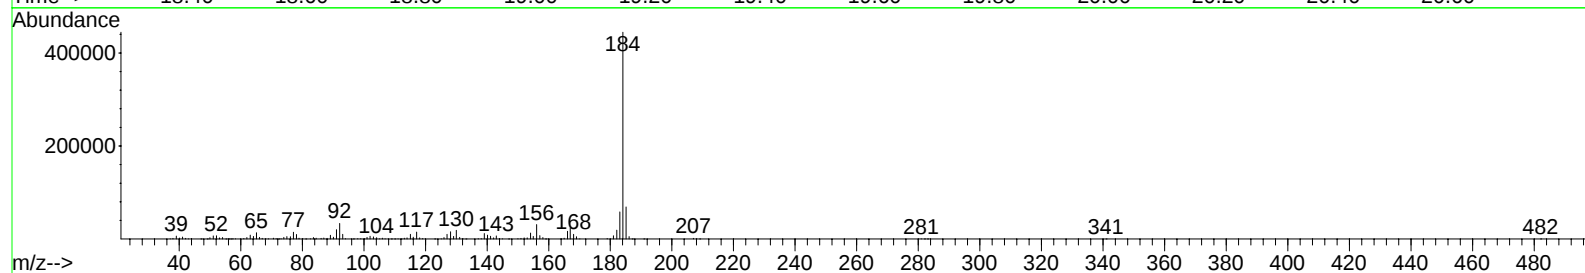


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010720\
Data File : BG043955.D
Acq On : 7 Jan 2020 15:05
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 17:58:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

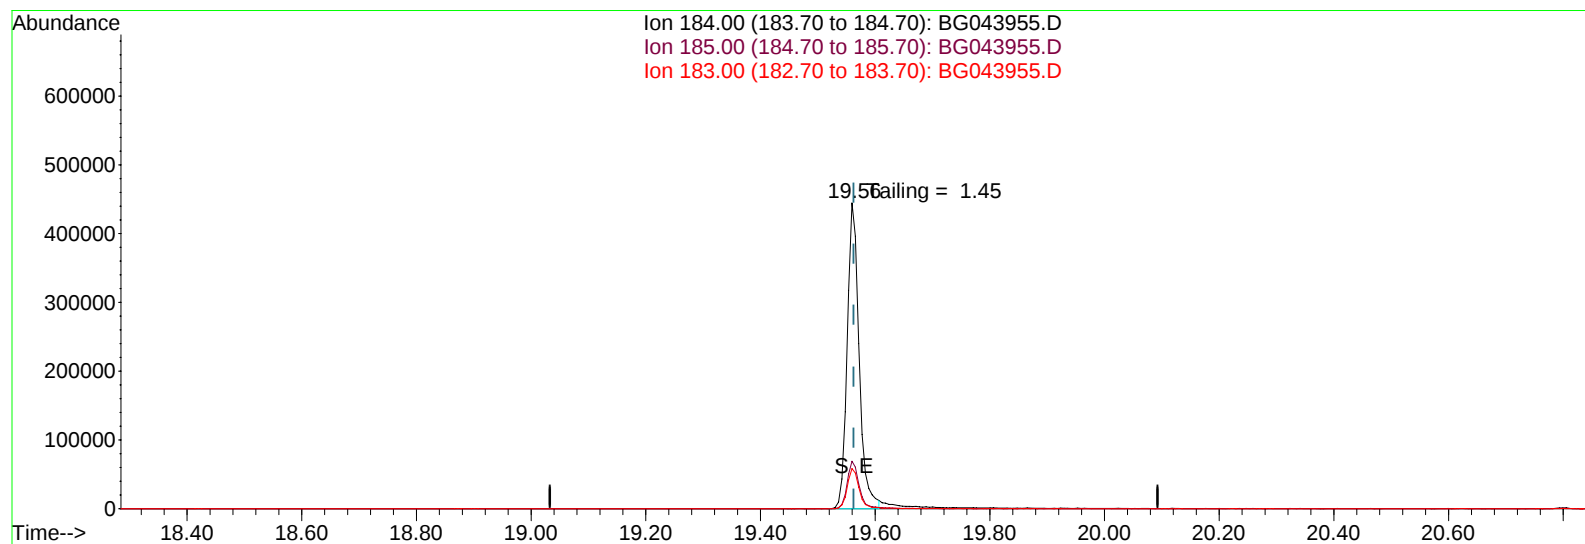

TIC: BG043955.D

(77) Benzidine




19.560min (-0.003) 424784.00ng

response 672665

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.54
183.00	13.20	13.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010720\
Data File : BG043955.D
Acq On : 7 Jan 2020 15:05
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 17:58:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

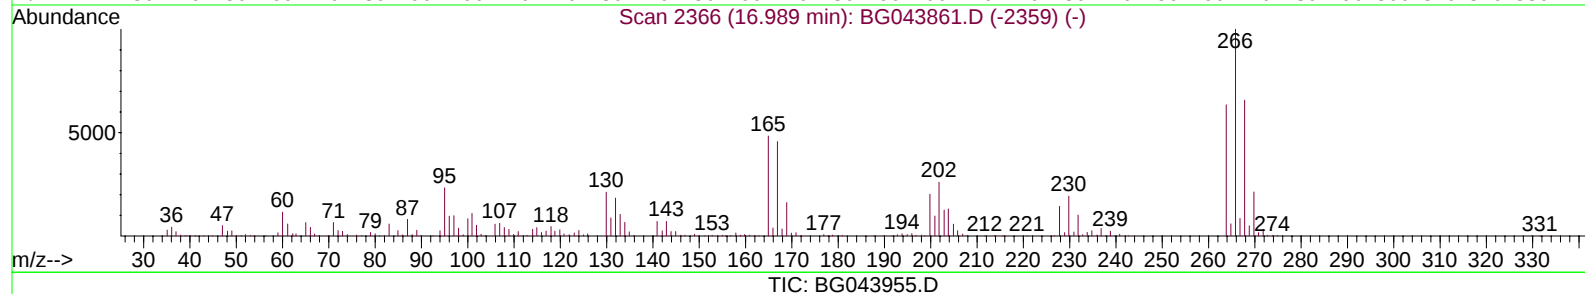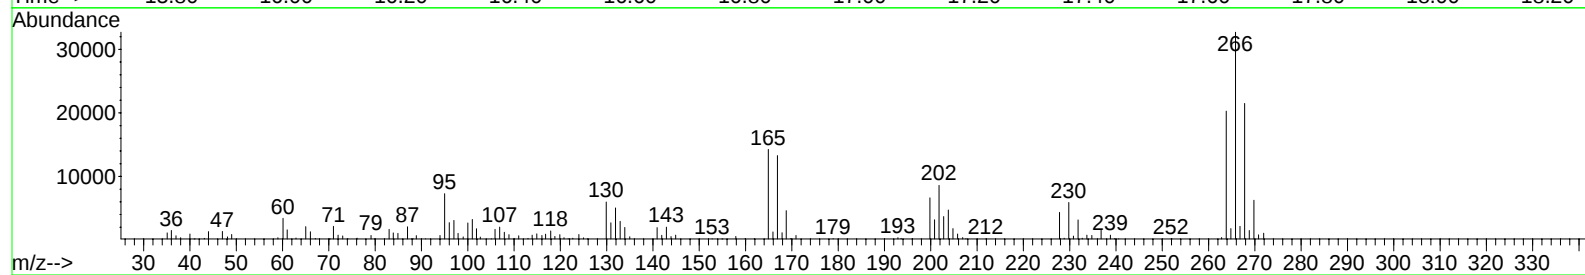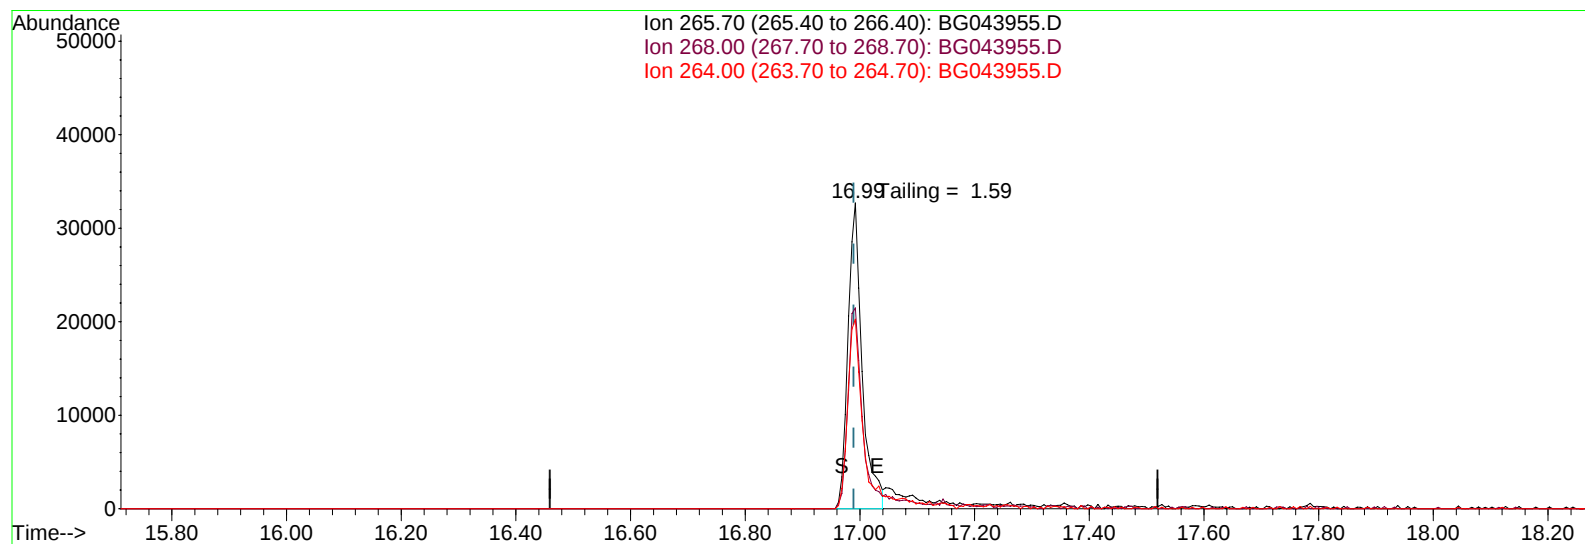

(70) Pentachlorophenol (C)

16.992min (+0.003) 159606.65ng

response 60777

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	65.70
264.00	63.50	62.03
0.00	0.00	0.00