


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010720\
 Data File : BG043947.D
 Acq On : 7 Jan 2020 9:20
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

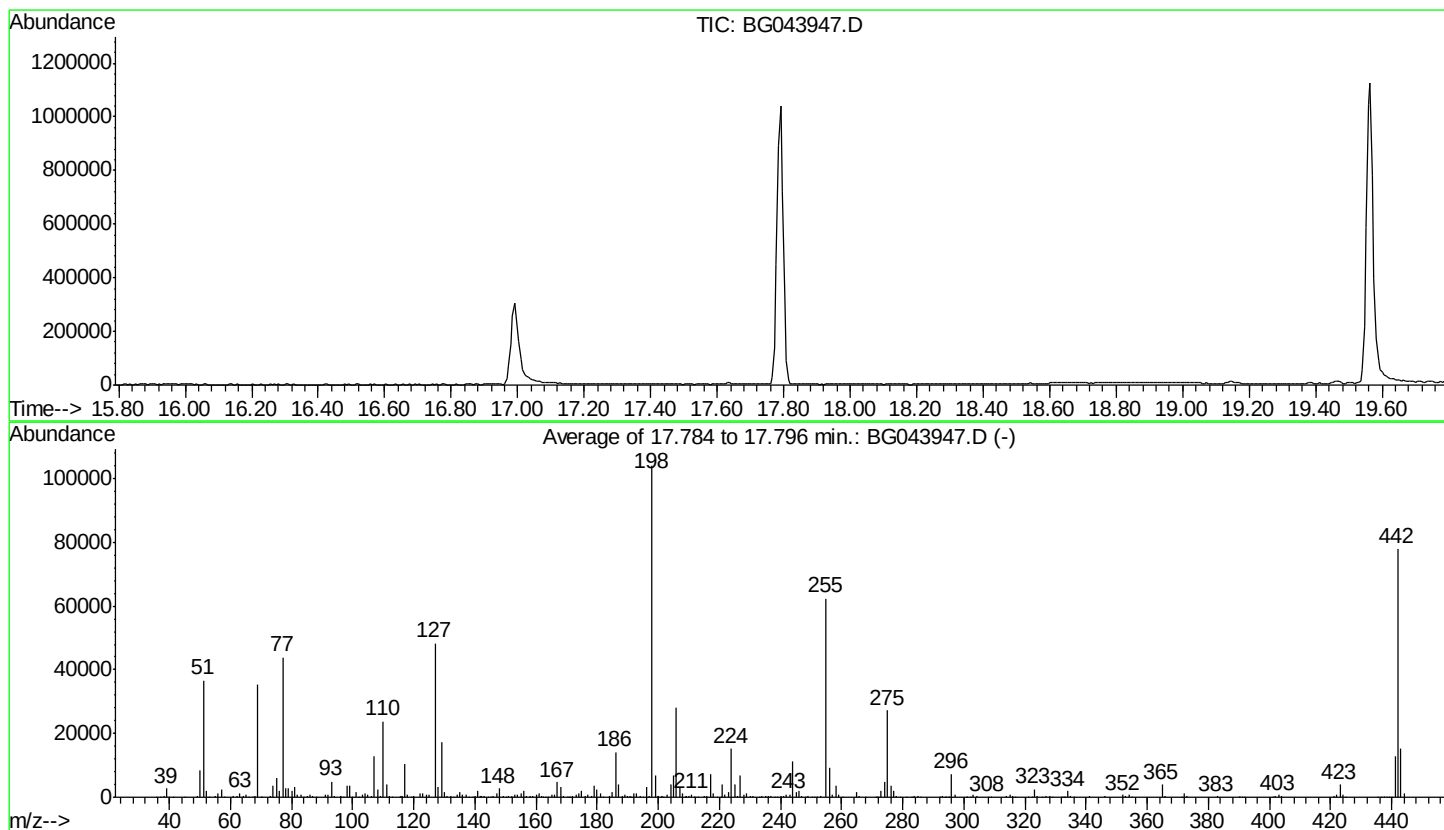

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	36562	PASS
68	69	0.00	2	1.2	422	PASS
69	198	0.00	100	34.0	35408	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	46.5	48336	PASS
197	198	0.00	2	0.3	357	PASS
198	198	100	100	100.0	104042	PASS
199	198	5	9	6.6	6837	PASS
275	198	10	60	26.2	27221	PASS
365	198	1	100	3.7	3886	PASS
441	198	0.01	100	12.3	12839	PASS
442	198	50	100	75.1	78088	PASS
443	442	15	24	19.4	15130	PASS