


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG010720\
 Data File : BG043955.D
 Acq On : 7 Jan 2020 15:05
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

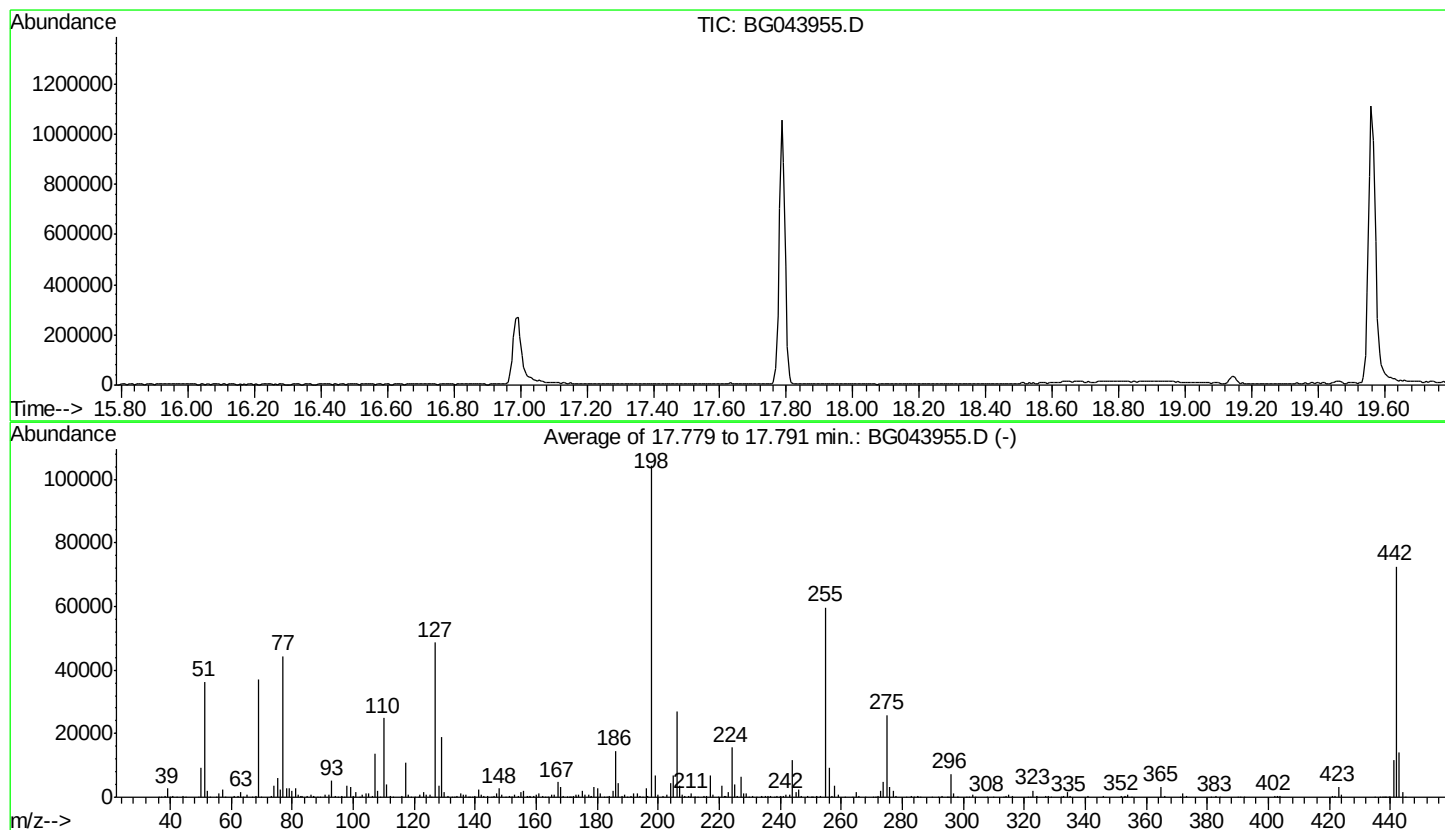

AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	36354	PASS
68	69	0.00	2	0.7	245	PASS
69	198	0.00	100	35.5	37021	PASS
70	69	0.00	2	0.5	196	PASS
127	198	10	80	46.6	48650	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	104304	PASS
199	198	5	9	6.6	6917	PASS
275	198	10	60	24.8	25821	PASS
365	198	1	100	3.2	3353	PASS
441	198	0.01	100	11.2	11670	PASS
442	198	50	100	69.6	72626	PASS
443	442	15	24	19.5	14143	PASS