

Data File : BG043965.D

Acq On : 8 Jan 2020 13:29

Operator : JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1



Quant Time: Jan 09 08:26:17 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 31 13:32:23 2019

Response via : Initial Calibration

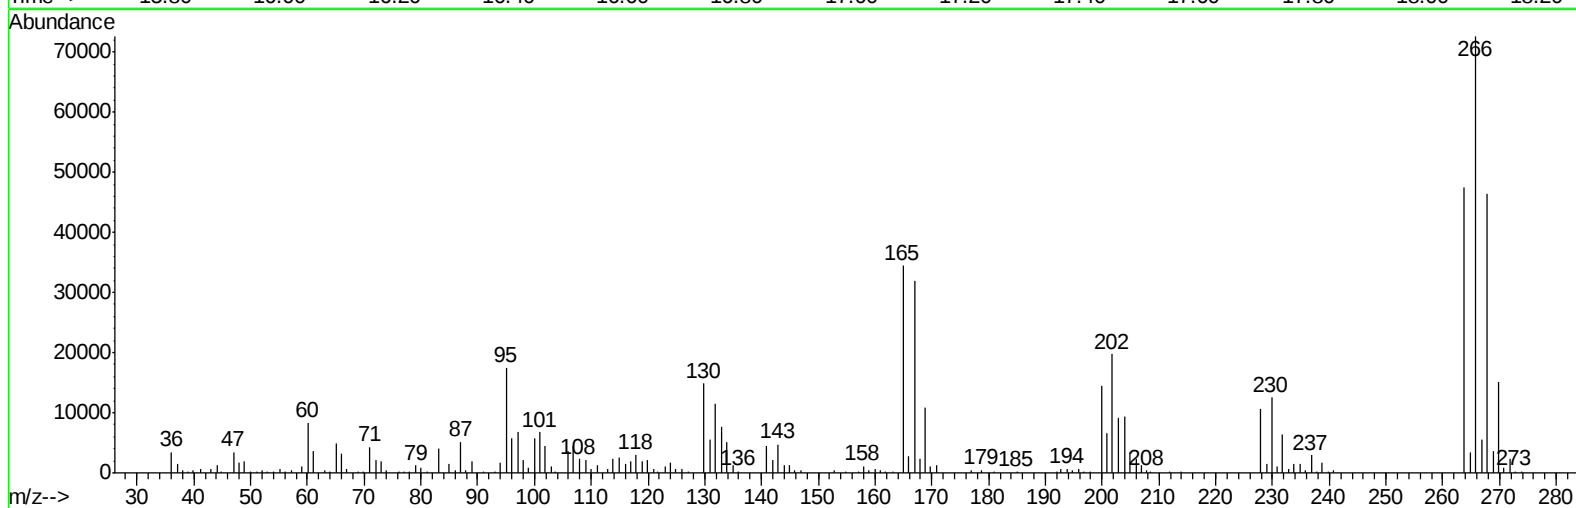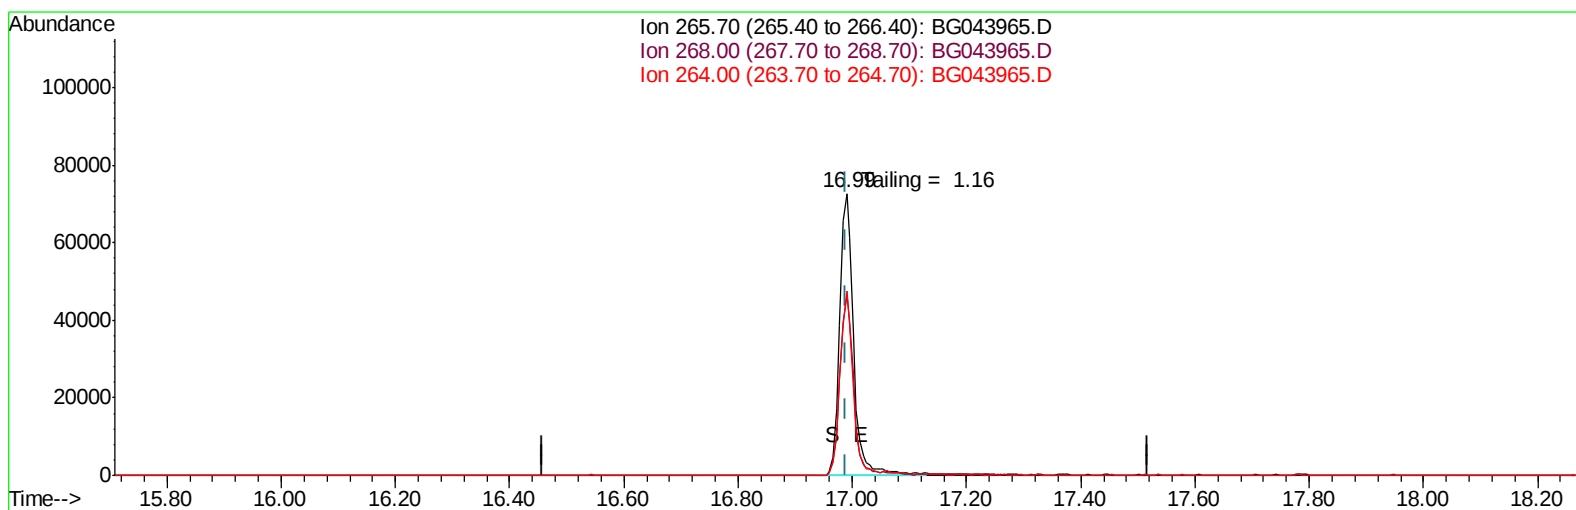

TIC: BG043965.D

(70) Pentachlorophenol (C)



16.990min (+0.000) 26373.92ng

response 122454

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	63.99
264.00	63.50	65.36
0.00	0.00	0.00

Data File : BG043965.D
Acq On : 8 Jan 2020 13:29
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 08:26:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

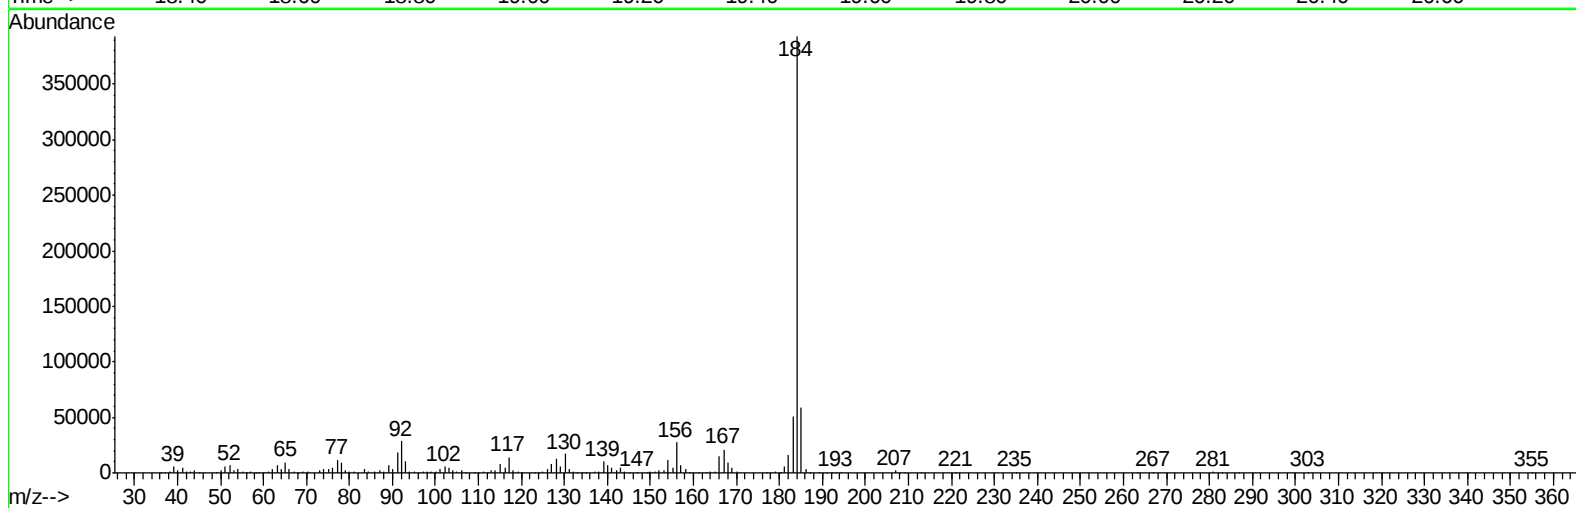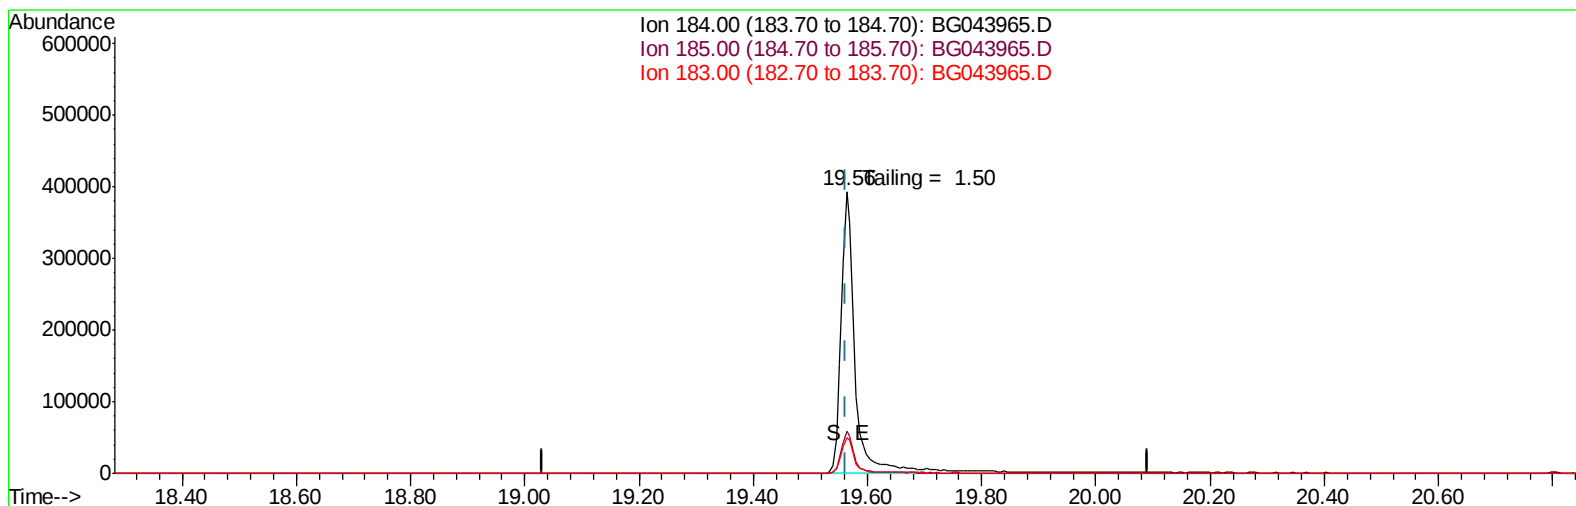

TIC: BG043965.D

(77) Benzidine

19.563min (+0.000) 220650.74ng

response 637813

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.05
183.00	13.20	12.80
0.00	0.00	0.00