

Data File : BG043978.D

Acq On : 8 Jan 2020 22:38

Operator : JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1



Quant Time: Jan 09 08:27:03 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG123019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 31 13:32:23 2019

Response via : Initial Calibration

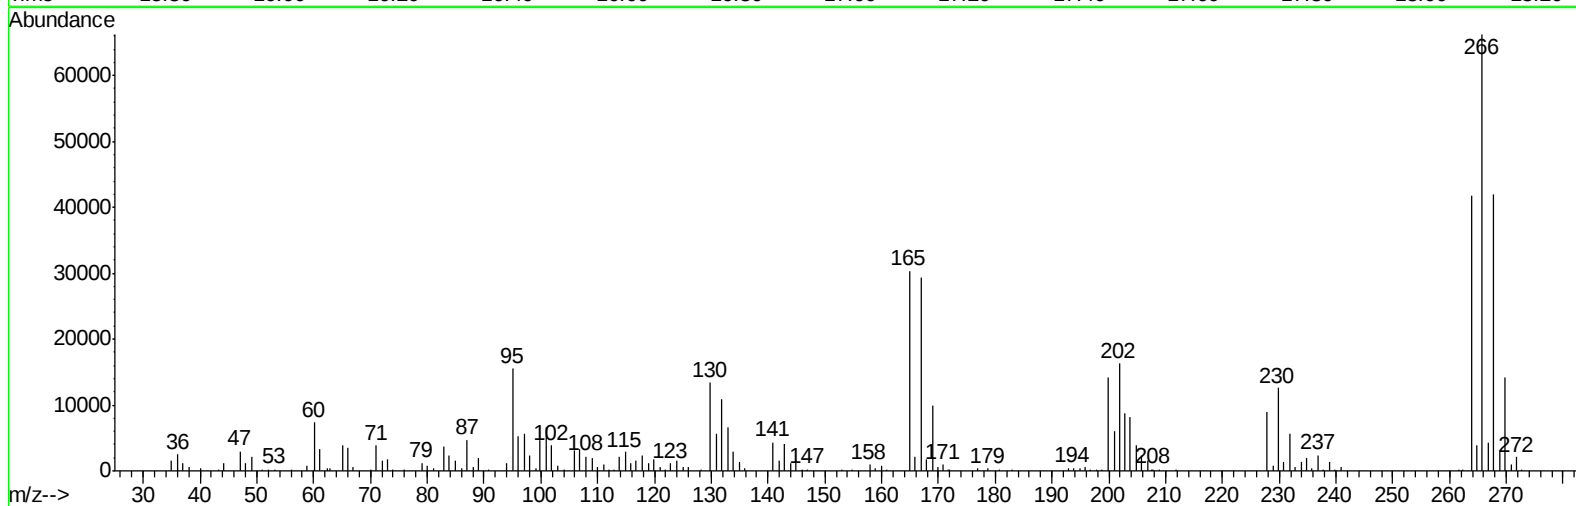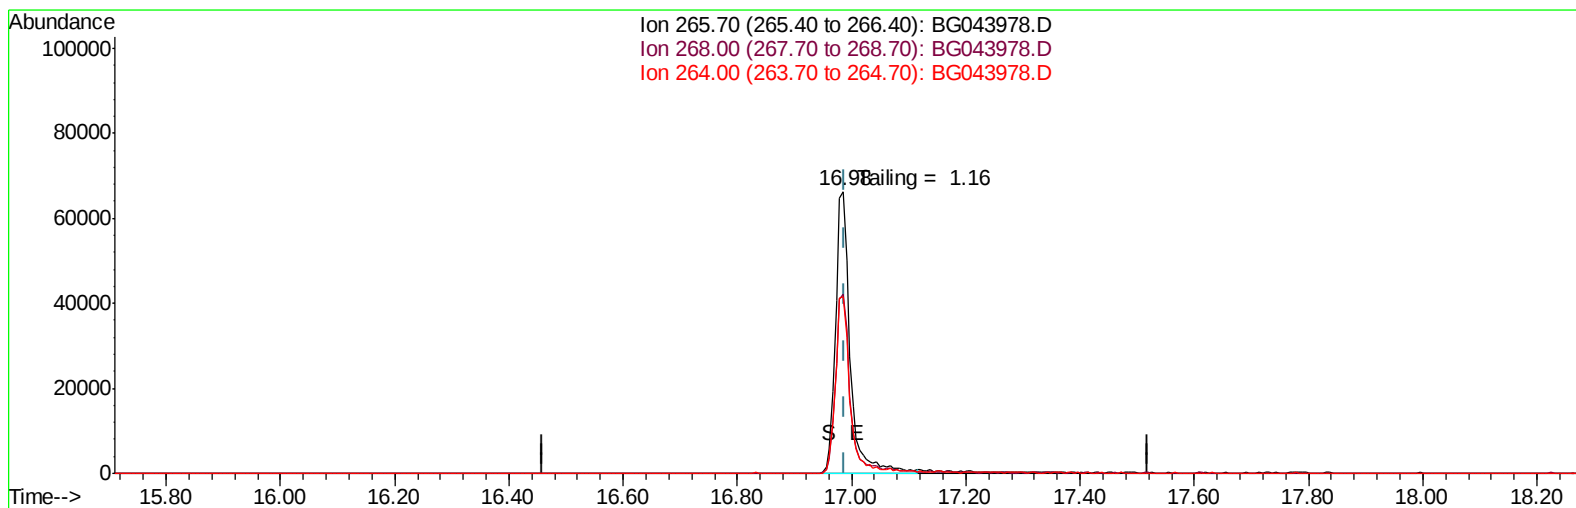

TIC: BG043978.D

(70) Pentachlorophenol (C)

16.985min (-0.004) 146942.34ng

response 117799

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.80 | 63.49 |
| 264.00 | 63.50 | 62.92 |
| 0.00   | 0.00  | 0.00  |

Data File : BG043978.D

Acq On : 8 Jan 2020 22:38

Operator : JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1



Quant Time: Jan 09 08:27:03 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG123019.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 31 13:32:23 2019

Response via : Initial Calibration

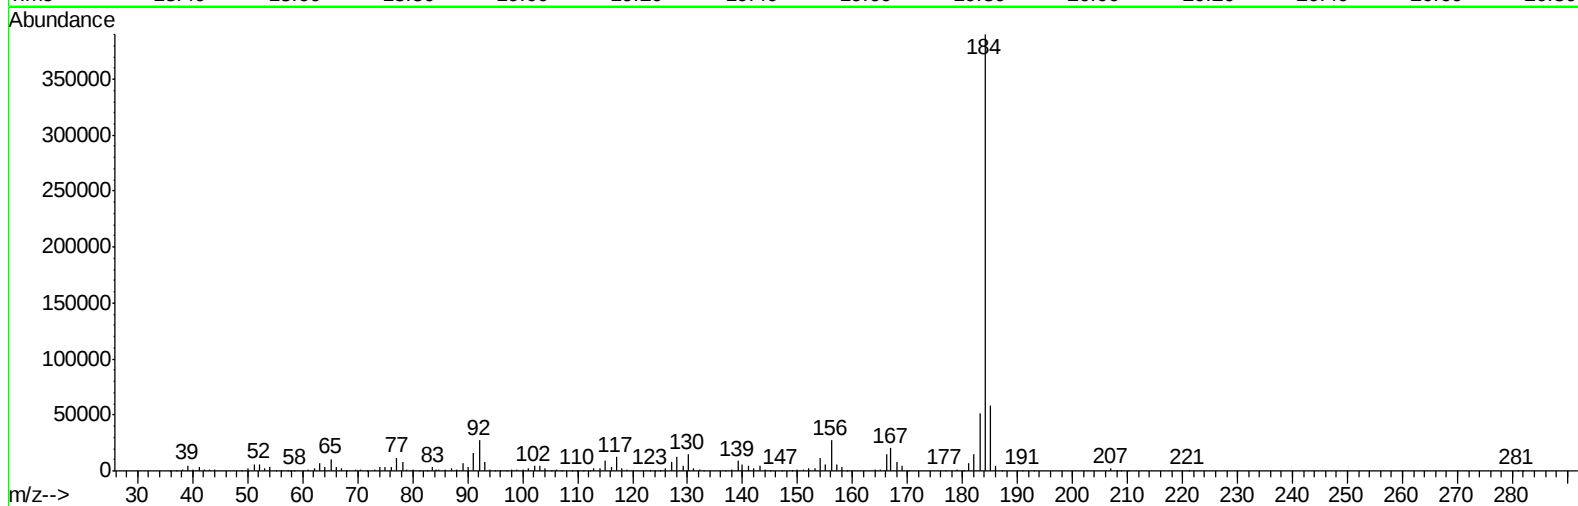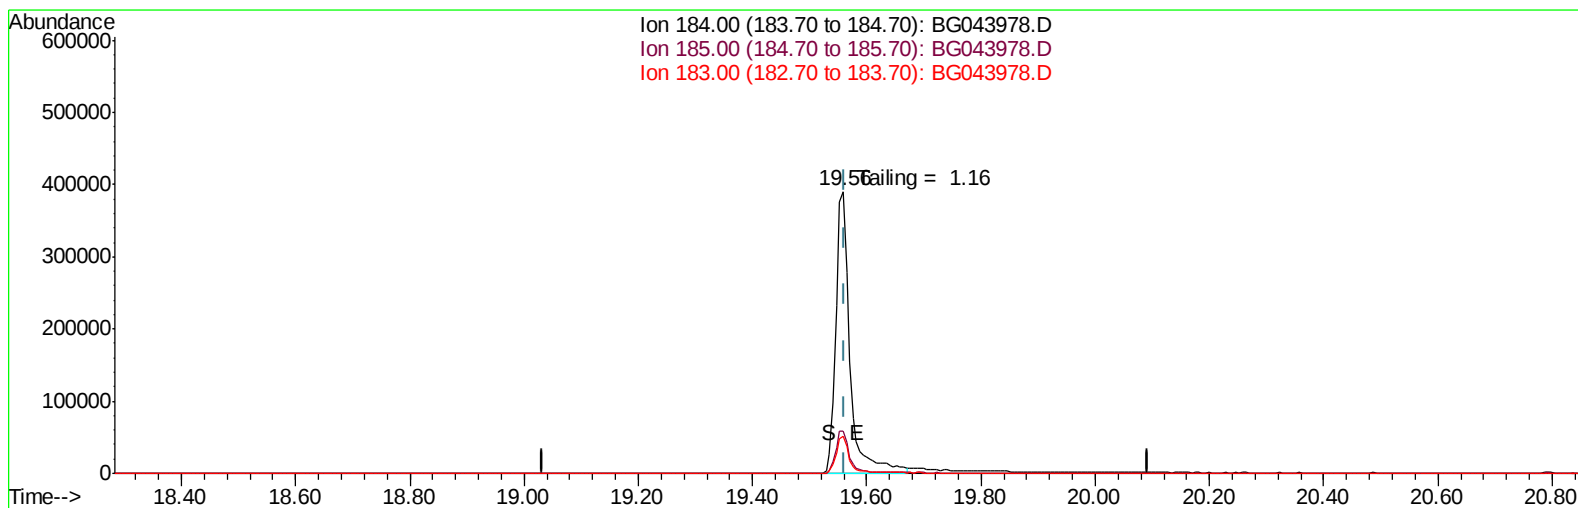

TIC: BG043978.D

(77) Benzidine

19.558min (-0.004) 18853.75ng

response 696161

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.70 | 15.04 |
| 183.00 | 13.20 | 13.24 |
| 0.00   | 0.00  | 0.00  |