


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG010820\
 Data File : BG043978.D
 Acq On : 8 Jan 2020 22:38
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

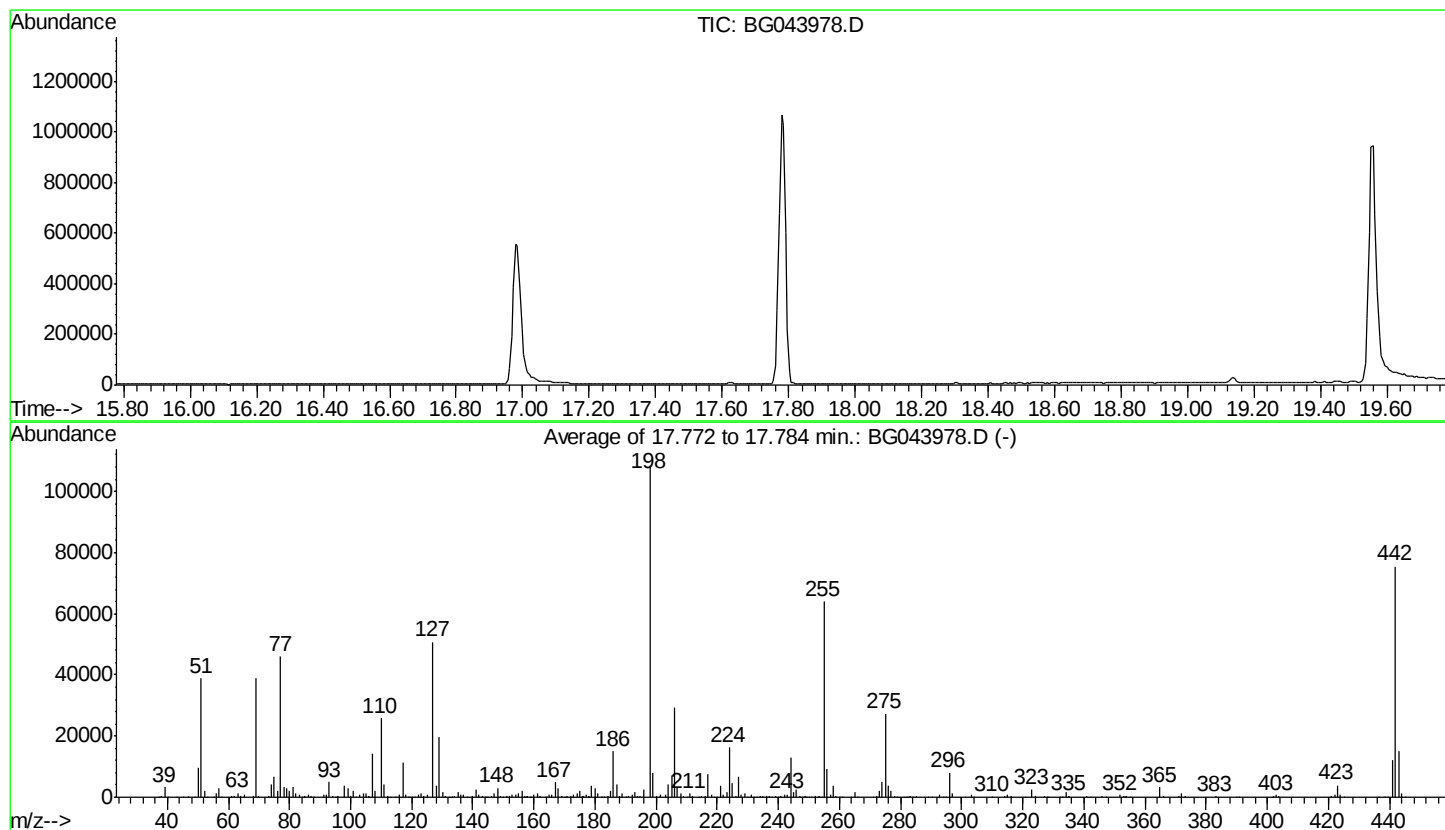

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	38797	PASS
68	69	0.00	2	0.7	278	PASS
69	198	0.00	100	35.9	38909	PASS
70	69	0.00	2	0.7	255	PASS
127	198	10	80	46.9	50818	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	108413	PASS
199	198	5	9	7.3	7880	PASS
275	198	10	60	25.2	27306	PASS
365	198	1	100	2.9	3195	PASS
441	198	0.01	100	11.2	12122	PASS
442	198	50	100	69.6	75405	PASS
443	442	15	24	20.3	15277	PASS