


Data Path : Z:\HPCHEM1\BNA_G\Data\BG010915\
Data File : BGTUNE2.D
Acq On : 9 Jan 2015 23:14
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG010515.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 06 08:46:19 2015

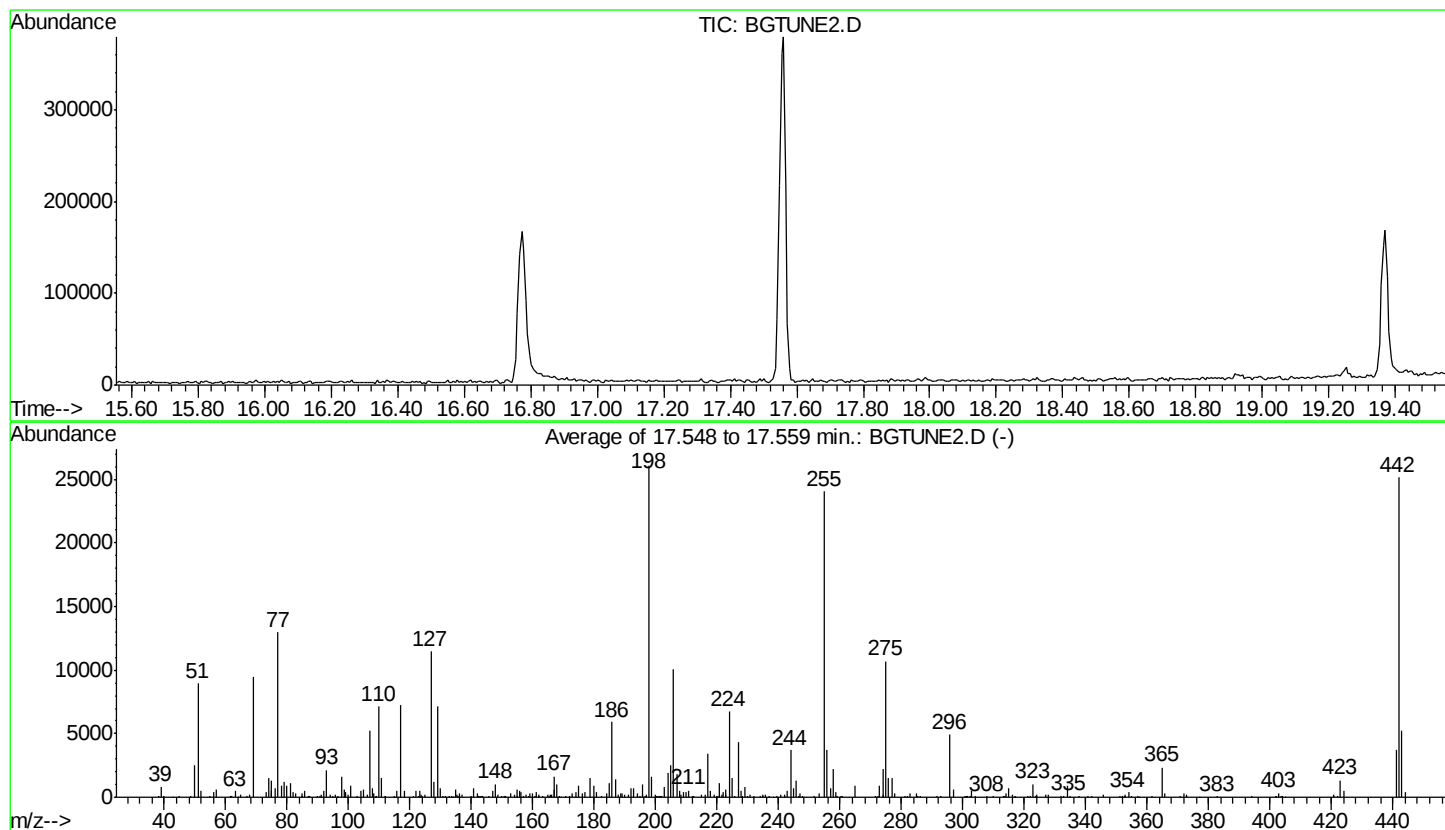

AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	8933	PASS
68	69	0.00	2	1.7	164	PASS
69	198	0.00	100	36.4	9503	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.0	11474	PASS
197	198	0.00	2	0.7	178	PASS
198	198	100	100	100.0	26082	PASS
199	198	5	9	6.2	1627	PASS
275	198	10	60	41.0	10704	PASS
365	198	1	100	9.1	2364	PASS
441	442	0.01	24	15.0	3768	PASS
442	198	50	100	96.4	25147	PASS
443	442	15	24	20.8	5219	PASS