


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG010915\
 Data File : BG015863.D
 Acq On : 9 Jan 2015 10:21
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG010515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 06 08:46:19 2015

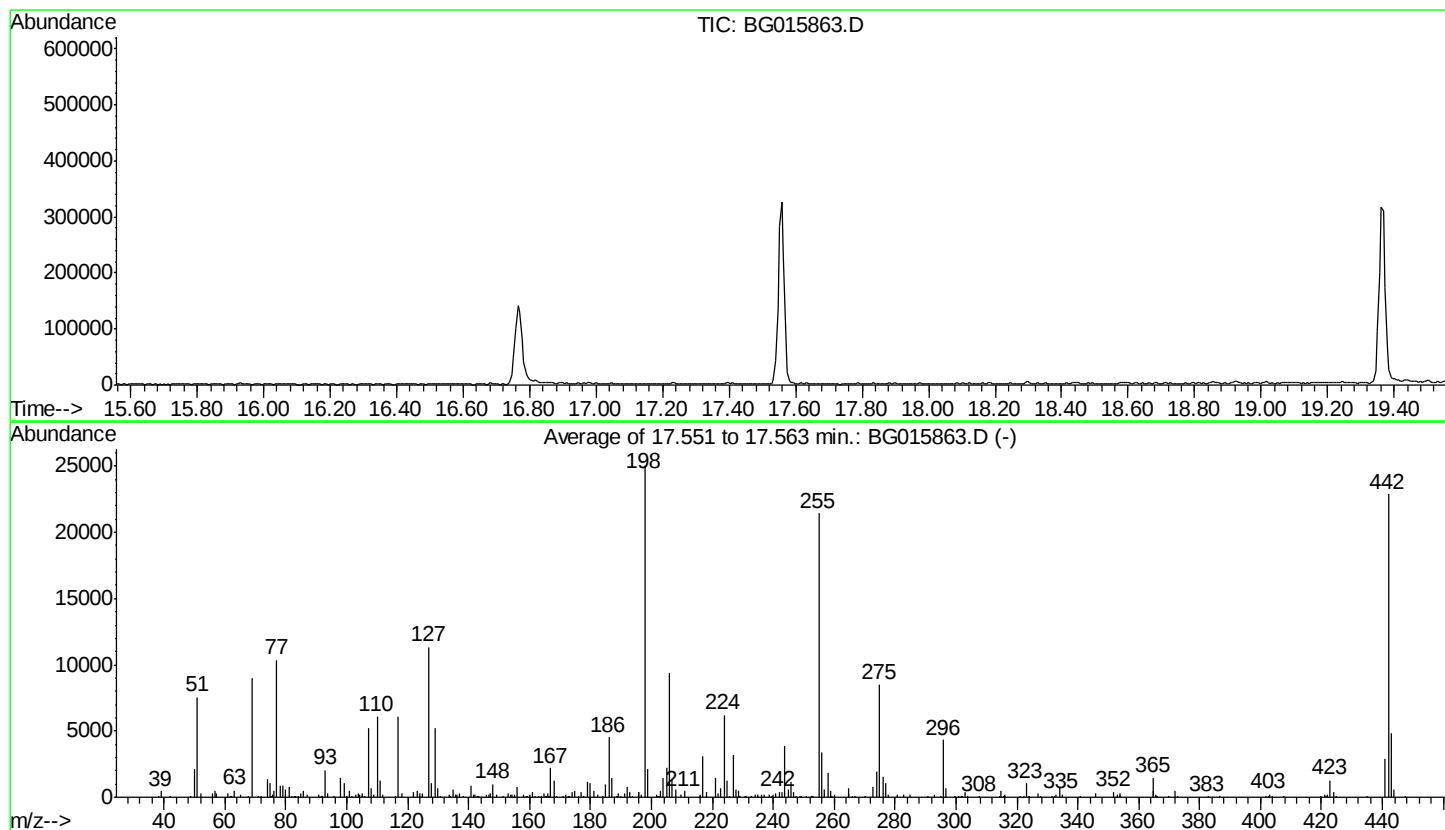

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	7567	PASS
68	69	0.00	2	0.9	82	PASS
69	198	0.00	100	36.1	9031	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.3	11352	PASS
197	198	0.00	2	0.8	188	PASS
198	198	100	100	100.0	25032	PASS
199	198	5	9	8.6	2163	PASS
275	198	10	60	34.0	8501	PASS
365	198	1	100	5.9	1479	PASS
441	442	0.01	24	12.8	2933	PASS
442	198	50	100	91.5	22896	PASS
443	442	15	24	21.2	4844	PASS