
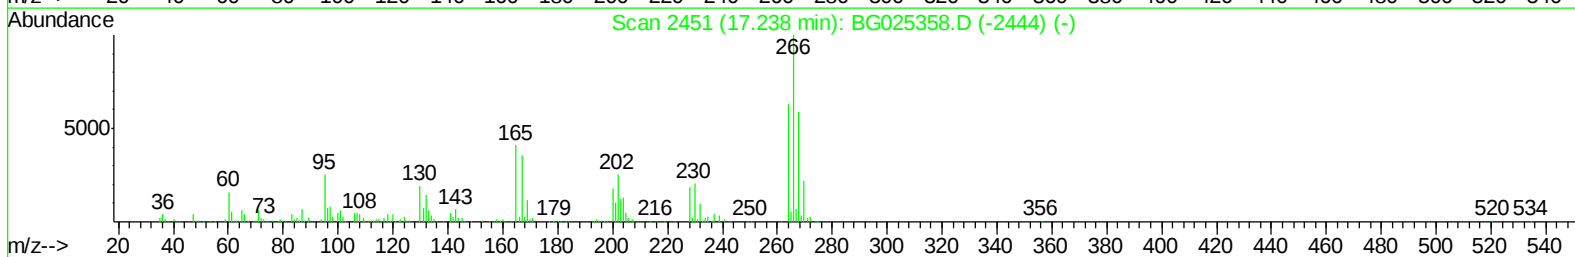
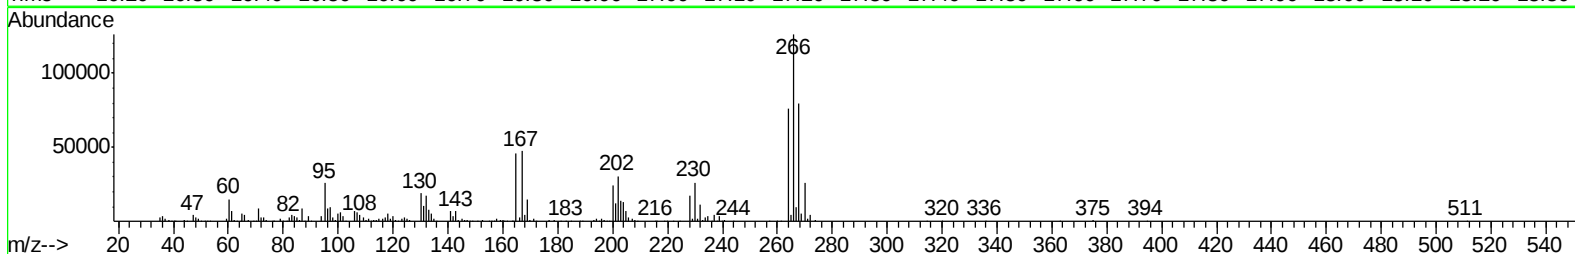


Data Path : Z:\HPCHEM1\BNA_G\Data\BG010917\
Data File : BG025432.D
Acq On : 9 Jan 2017 16:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 07:59:00 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 18:42:01 2016
Response via : Initial Calibration

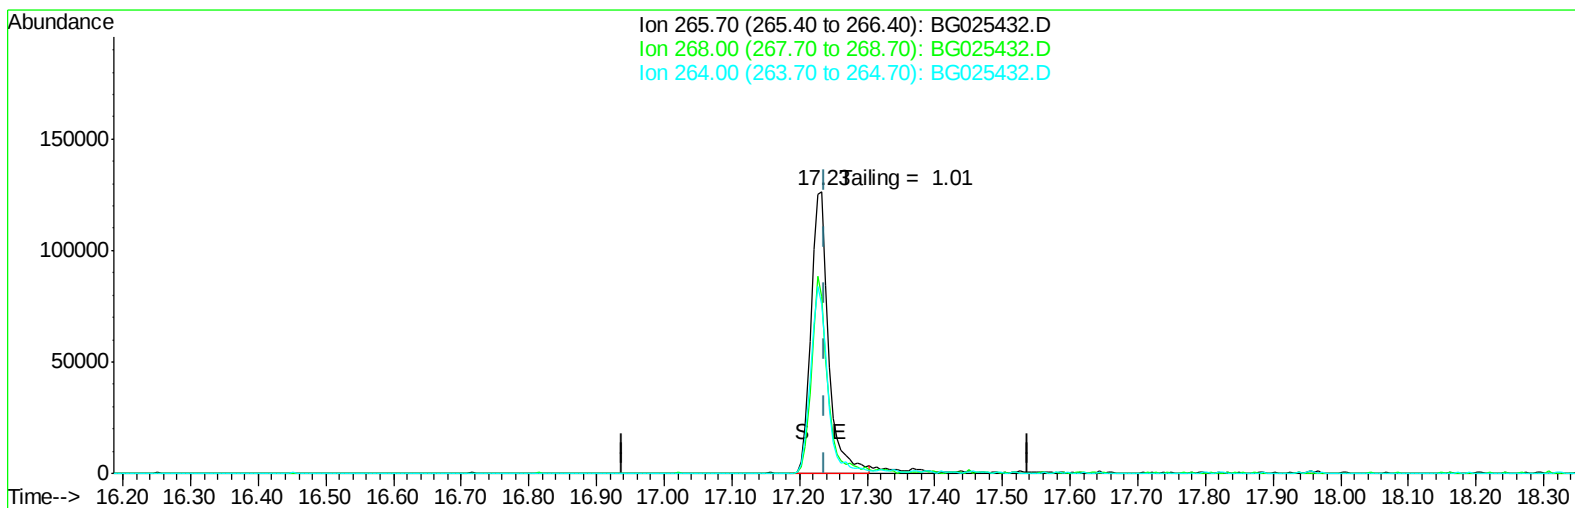

TIC: BG025432.D

(69) Pentachlorophenol (C)

17.232min (-0.006) 97966.70ng

response 236553

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.85
264.00	62.60	60.15
0.00	0.00	0.00

