


Data Path : Z:\HPCHEM1\BNA G\DATA\BG010917\
 Data File : BG025432.D
 Acq On : 9 Jan 2017 16:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 18:42:01 2016

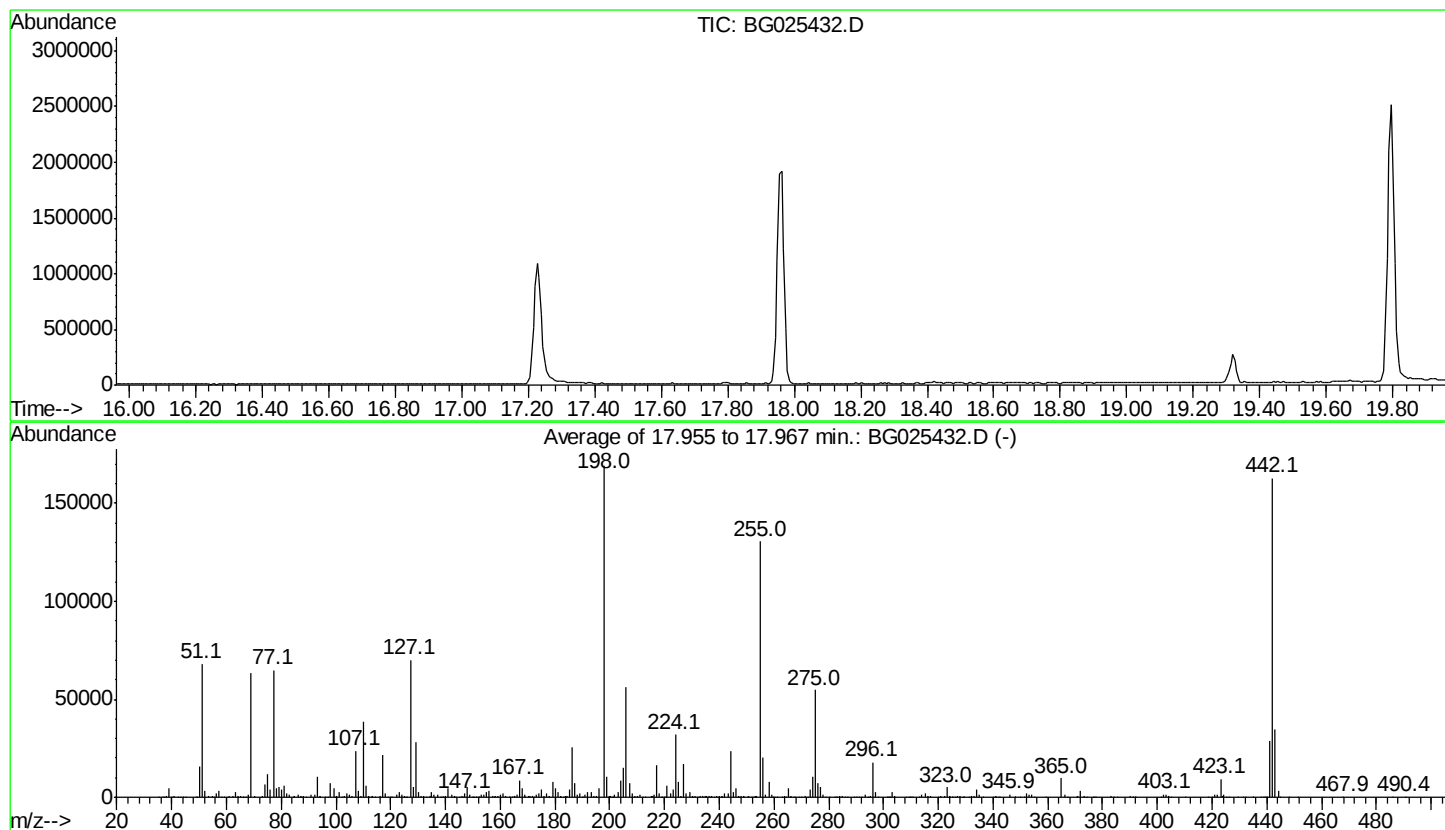

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	68096	PASS
68	69	0.00	2	1.8	1162	PASS
69	198	0.00	100	37.6	63685	PASS
70	69	0.00	2	1.0	646	PASS
127	198	10	80	41.4	70149	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	169250	PASS
199	198	5	9	6.4	10768	PASS
275	198	10	60	32.3	54672	PASS
365	198	1	100	5.7	9665	PASS
441	442	0.01	24	17.5	28536	PASS
442	198	50	100	96.2	162858	PASS
443	442	15	24	21.1	34344	PASS