
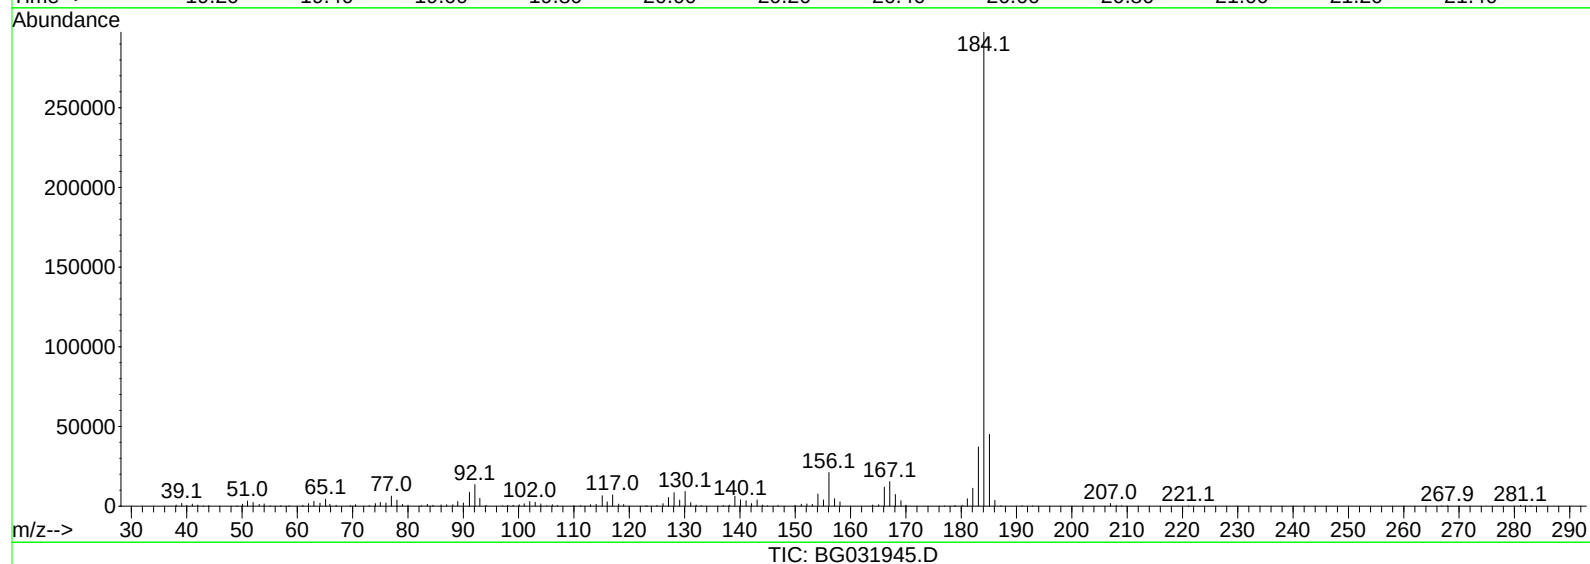


Data Path : Z:\HPCHEM1\BNA G\Data\BG010918\
Data File : BG031945.D
Acq On : 9 Jan 2018 13:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 06:22:03 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 05 15:31:34 2018
Response via : Initial Calibration

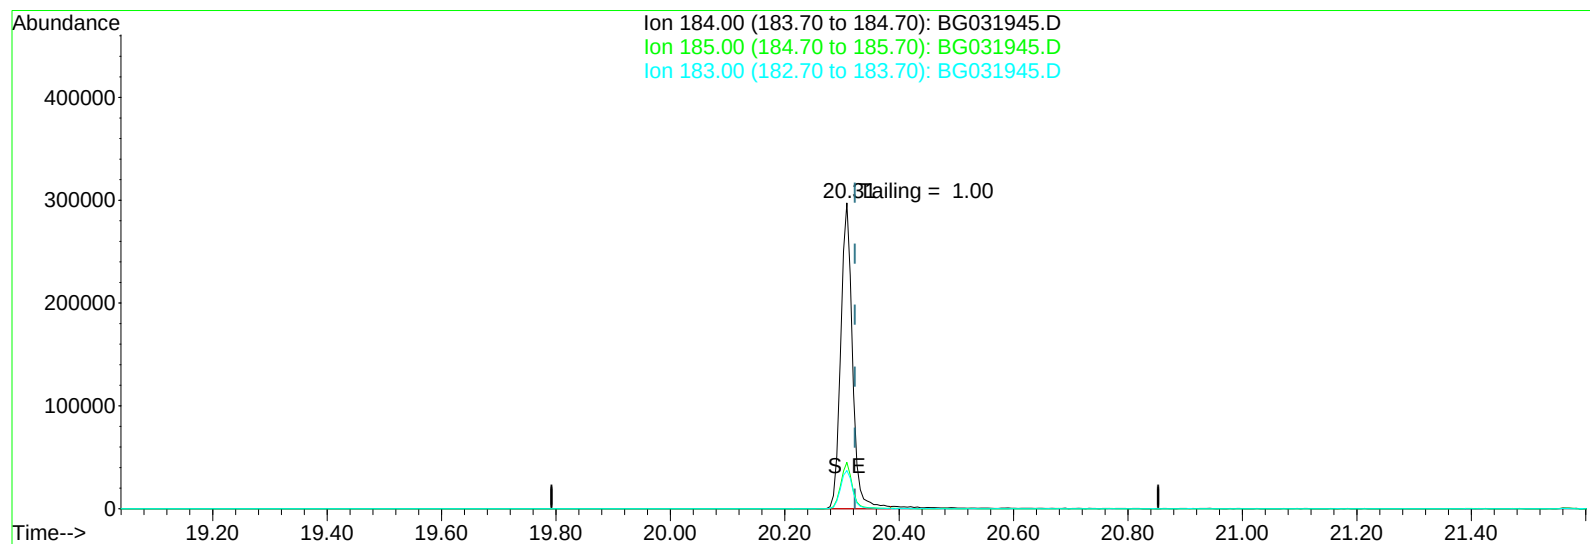

(76) Benzidine



20.309min (-0.014) 197013.12ng

response 425662

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.14
183.00	13.30	12.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG010918\
Data File : BG031945.D
Acq On : 9 Jan 2018 13:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 06:22:03 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 05 15:31:34 2018
Response via : Initial Calibration

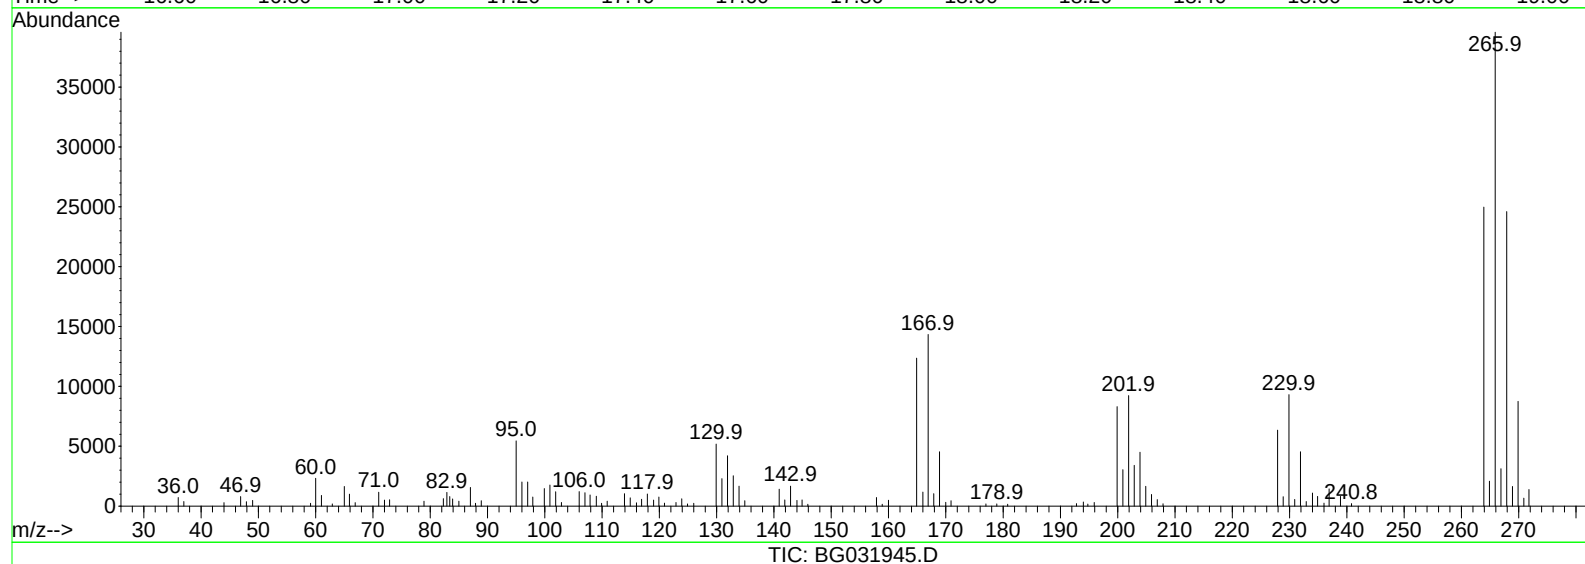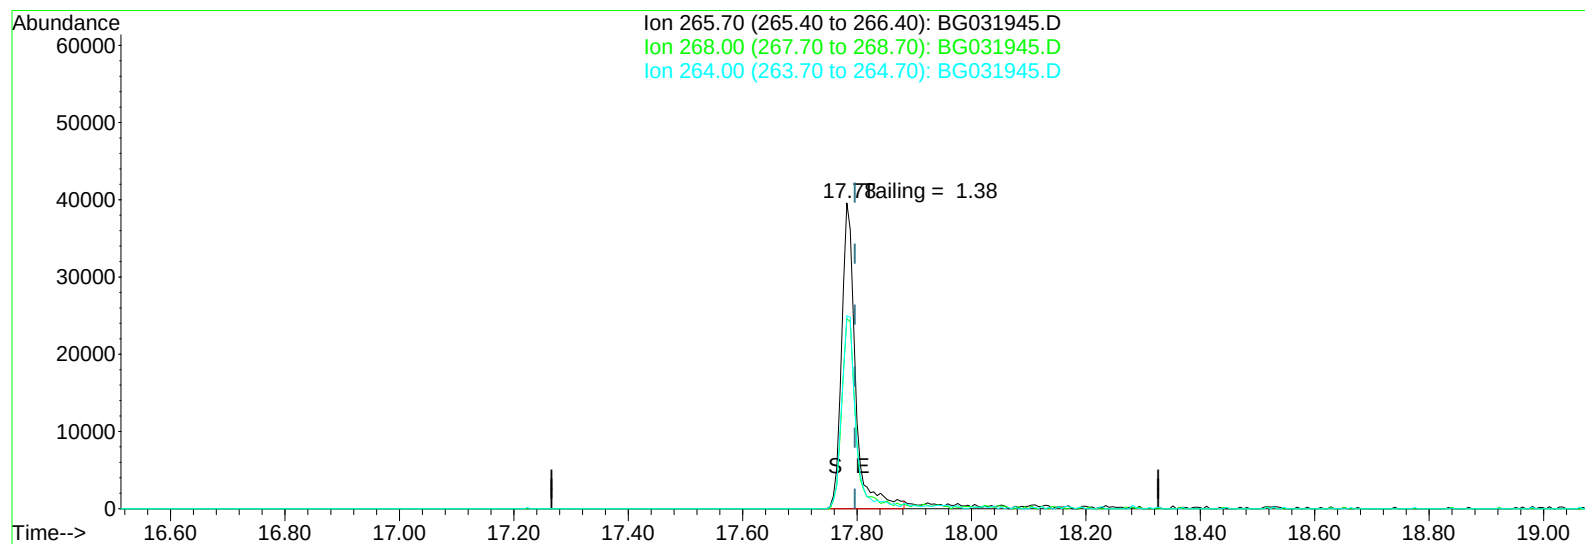

(69) Pentachlorophenol (C)

17.782min (-0.014) 37425.44ng

response 65832

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.15
264.00	62.00	63.08
0.00	0.00	0.00