
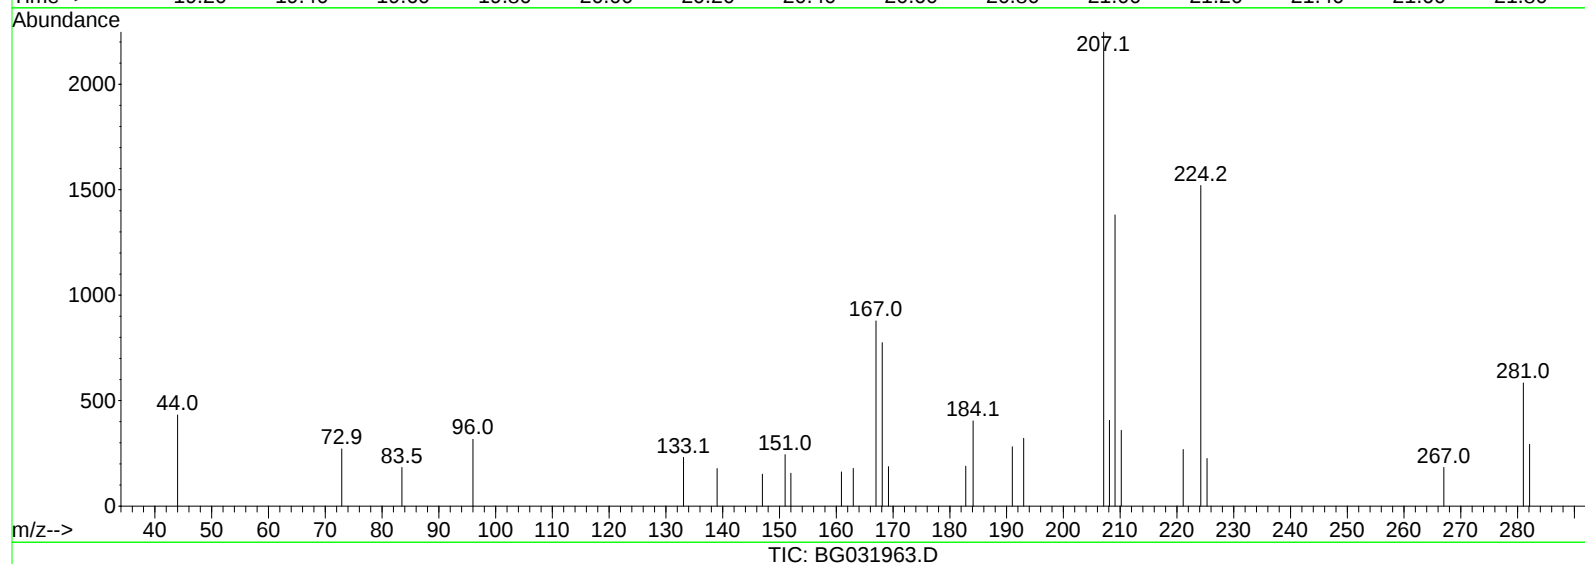


Data Path : Z:\HPCHEM1\BNA G\Data\BG010918\
Data File : BG031963.D
Acq On : 10 Jan 2018 2:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 06:27:03 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 05 15:31:34 2018
Response via : Initial Calibration

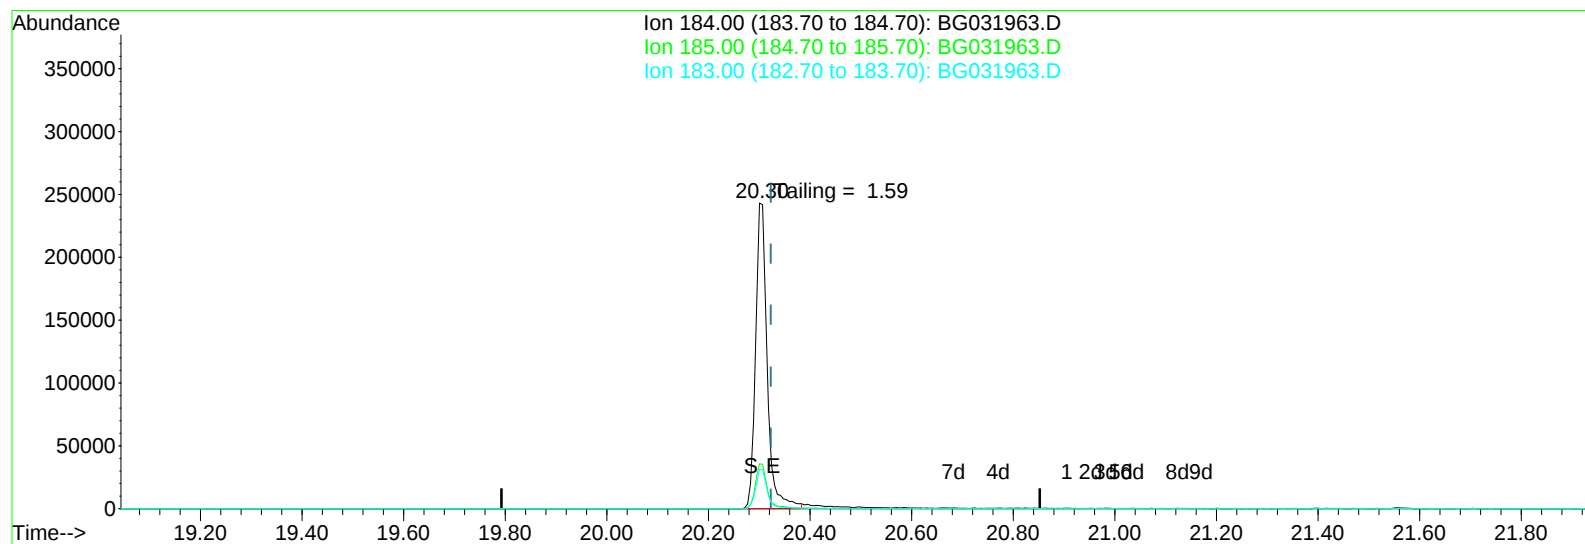

(76) Benzidine



20.906min (+0.583) 311.84ng

response 539

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	13.30	46.78#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG010918\
Data File : BG031963.D
Acq On : 10 Jan 2018 2:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 06:27:03 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 05 15:31:34 2018
Response via : Initial Calibration

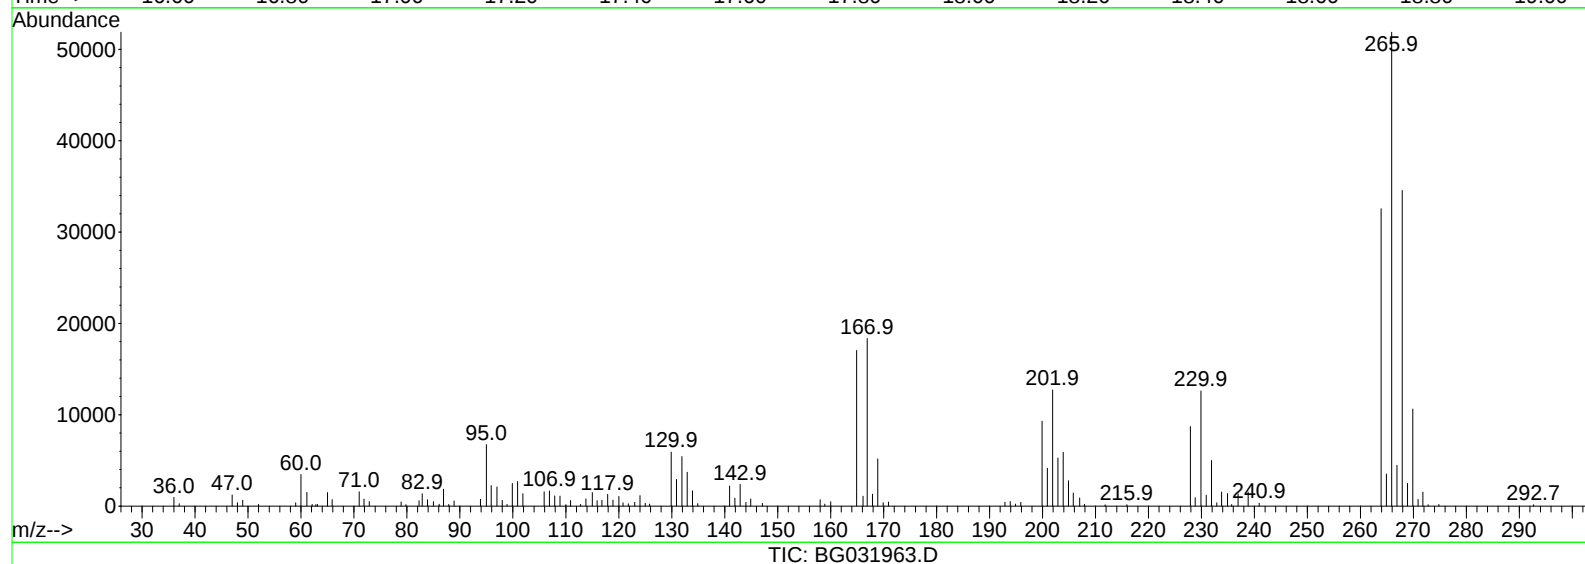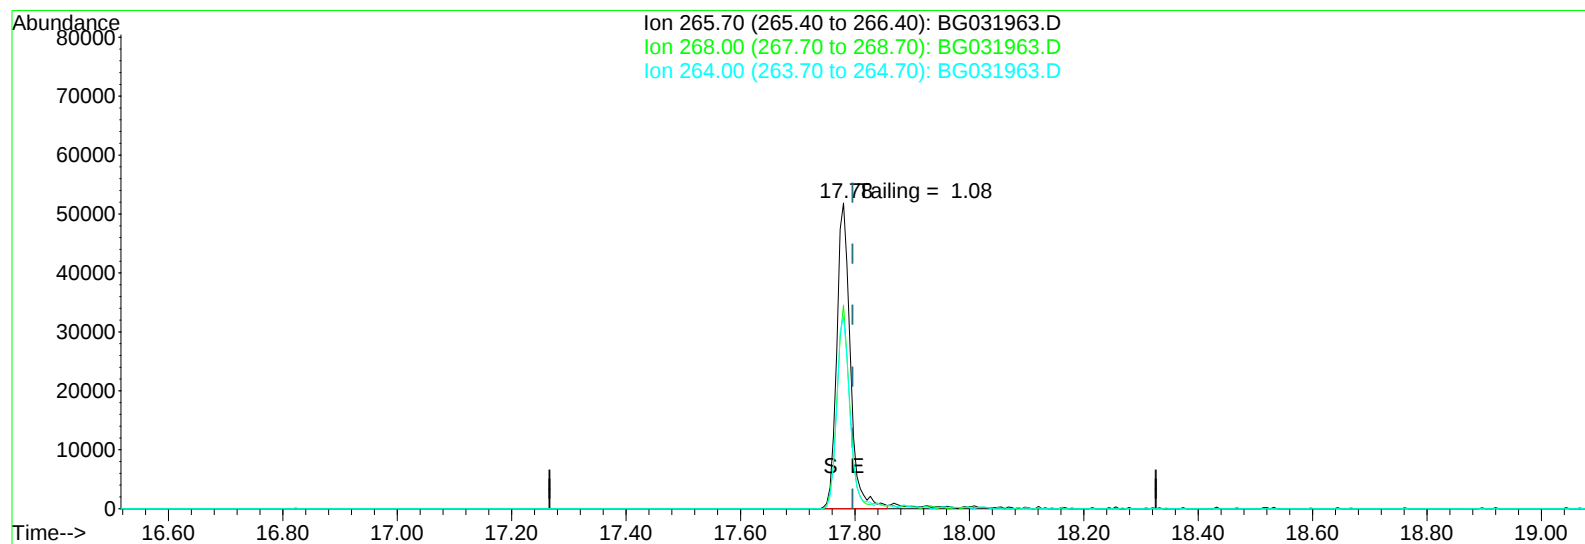

(69) Pentachlorophenol (C)

17.780min (-0.016) 19178.09ng

response 85409

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.60
264.00	62.00	62.74
0.00	0.00	0.00