

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG010918\
 Data File : BG031975.D
 Acq On : 10 Jan 2018 10:40
 Operator : SJ/JU
 Sample : PB105532TB
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB105532TB

Quant Time: Jan 10 11:14:17 2018
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 05 15:31:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.79	152	67096	20.00	ng	0.00
21) Naphthalene-d8	11.67	136	277687	20.00	ng	0.00
38) Acenaphthene-d10	15.42	164	189518	20.00	ng	-0.01
63) Phenanthrene-d10	18.14	188	477441	20.00	ng	-0.02
75) Chrysene-d12	22.48	240	530066	20.00	ng	-0.04
86) Perylene-d12	26.21	264	526594	20.00	ng	-0.09
System Monitoring Compounds						
5) 2-Fluorophenol	6.21	112	469436	127.43	ng	0.00
7) Phenol-d6	7.89	99	594924	124.39	ng	0.00
23) Nitrobenzene-d5	9.99	82	328429	89.31	ng	0.00
41) 2,4,6-Tribromophenol	16.88	330	344277	119.05	ng	-0.02
44) 2-Fluorobiphenyl	14.05	172	1187936	78.67	ng	0.00
78) Terphenyl-d14	20.67	244	1899124	81.85	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG010918\
Data File : BG031975.D
Acq On : 10 Jan 2018 10:40
Operator : SJ/JU
Sample : PB105532TB
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB105532TB

Quant Time: Jan 10 11:14:17 2018
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 05 15:31:34 2018
Response via : Initial Calibration

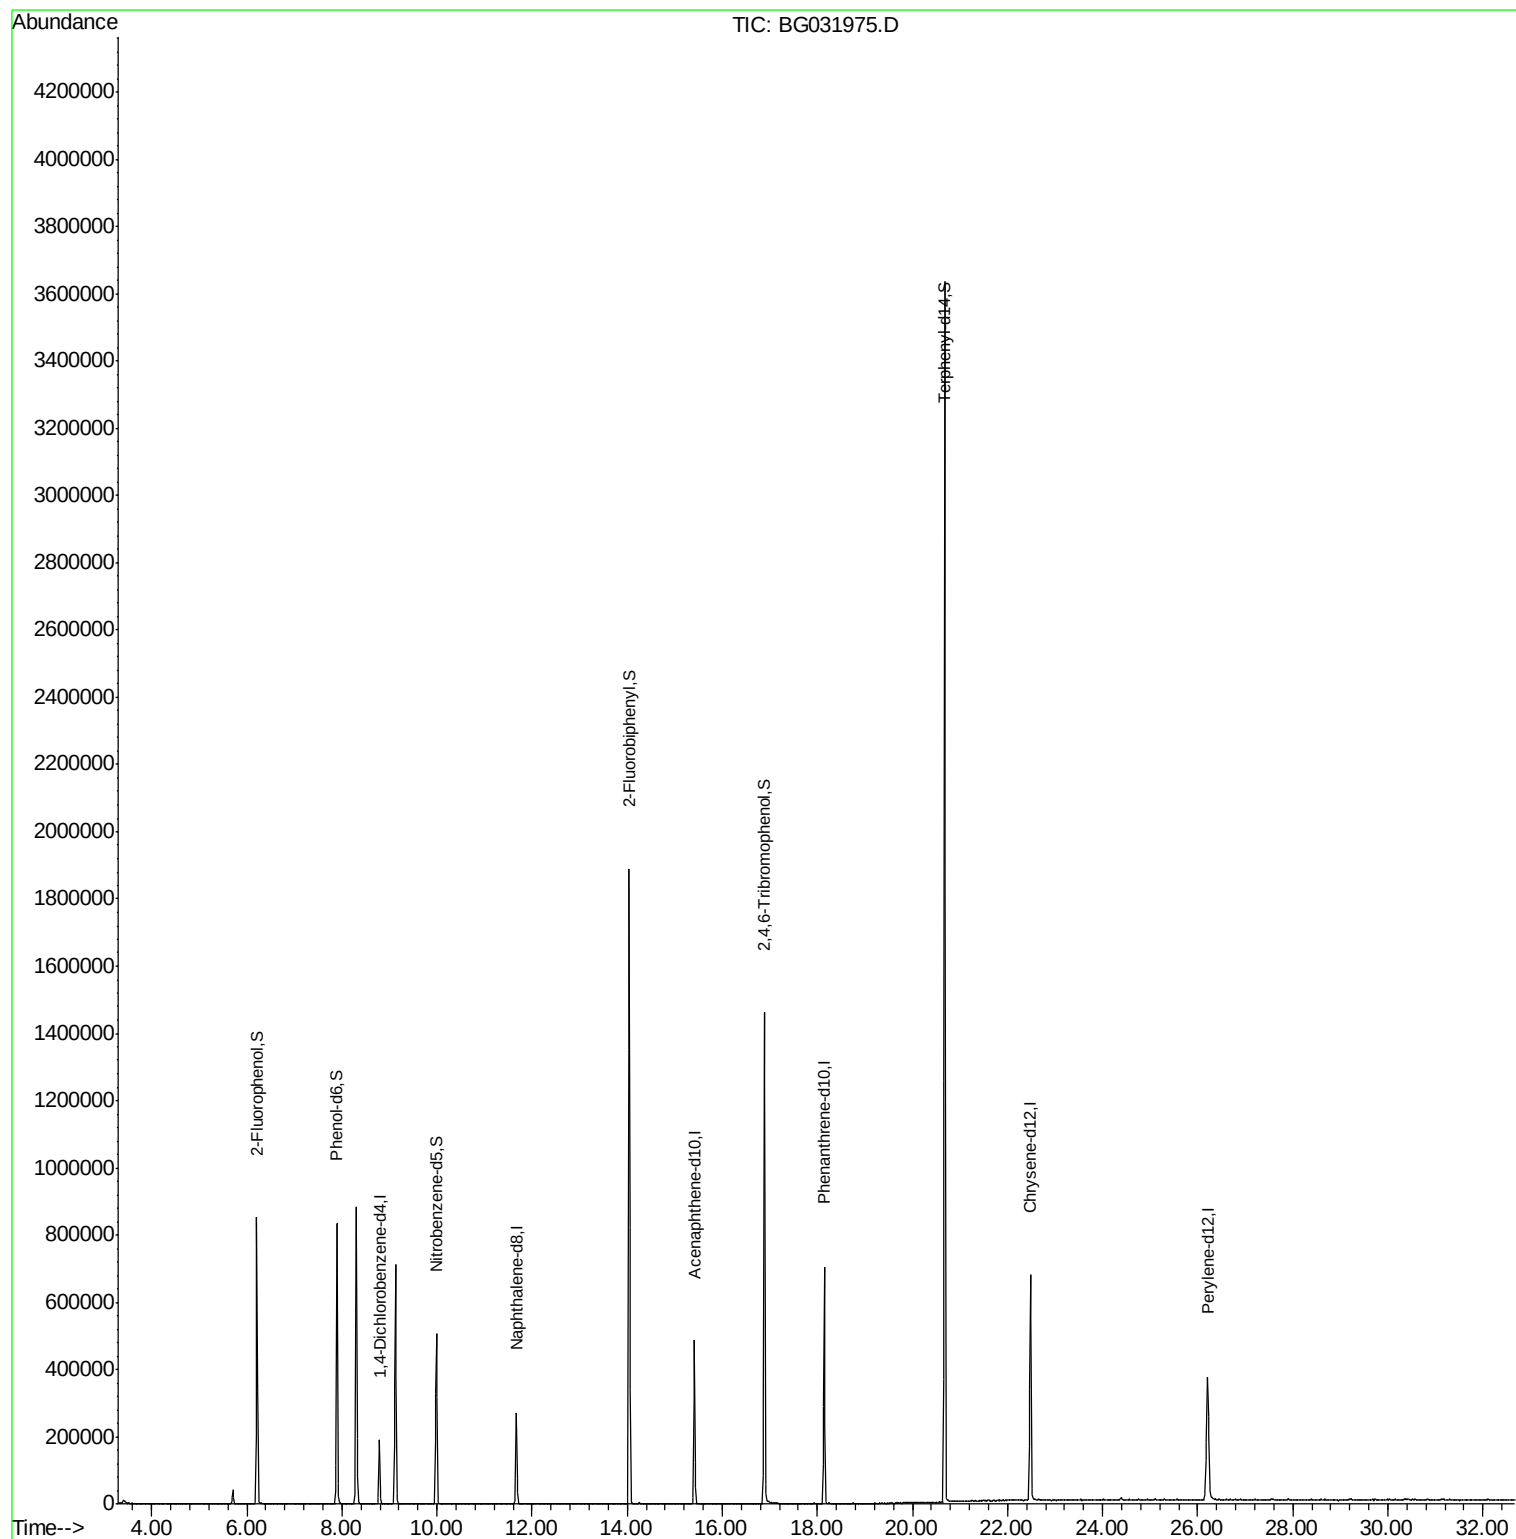

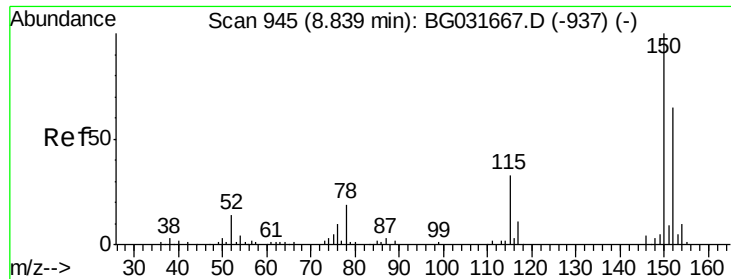


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.79 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: BG031975.D
 Acq: 10 Jan 2018 10:40

Instrument :
 BNA_G
 ClientSampleId :
 PB105532TB

Tgt Ion:152 Resp: 67096
 Ion Ratio Lower Upper
 152 100
 150 147.5 126.6 189.8
 115 52.1 53.0 79.4#

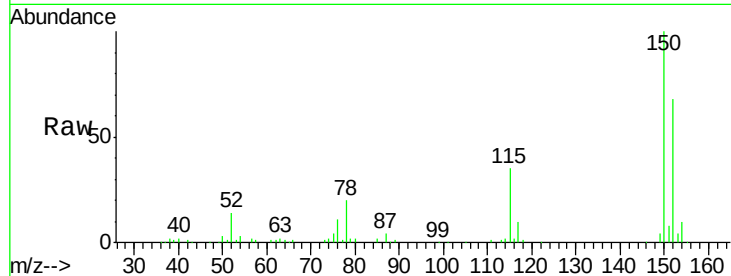


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

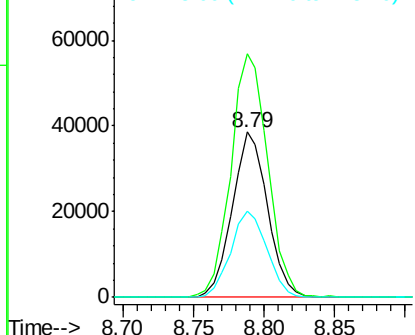



#5


2-Fluorophenol
 Concen: 127.433 ng
 RT: 6.21 min Scan# 498
 Delta R.T. 0.00 min
 Lab File: BG031975.D
 Acq: 10 Jan 2018 10:40

Tgt Ion:112 Resp: 469436
 Ion Ratio Lower Upper
 112 100
 64 50.0 56.3 84.5#
 63 26.9 30.1 45.1#



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

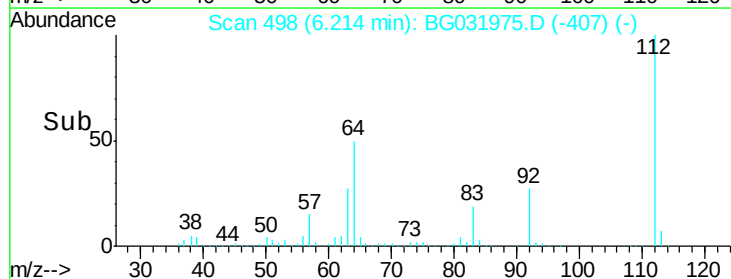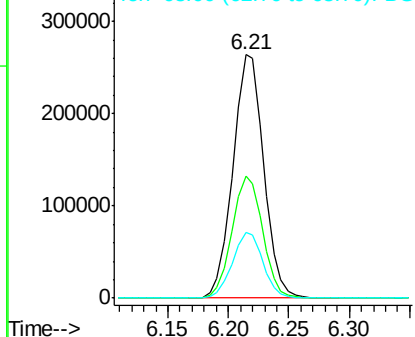



#7

Phenol-d6

Concen: 124.389 ng

RT: 7.89 min Scan# 784

Delta R.T. 0.00 min

Lab File: BG031975.D

Acq: 10 Jan 2018 10:40

Instrument :

BNA_G

ClientSampleId :

PB105532TB


Tgt Ion: 99 Resp: 594924

Ion Ratio Lower Upper




99 100

42 13.7 14.1 21.1#

71 35.4 26.1 39.1

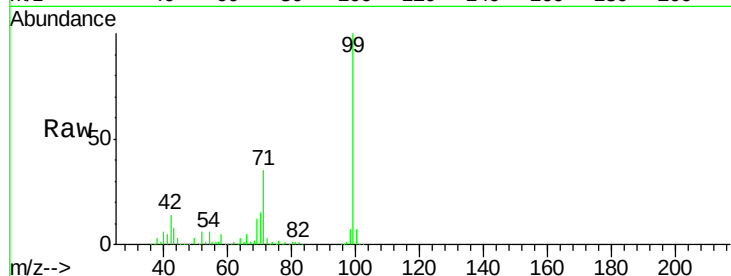

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

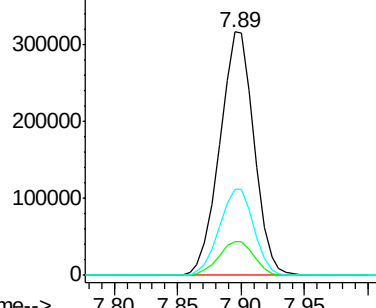

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.67 min Scan# 1427

Delta R.T. -0.00 min

Lab File: BG031975.D

Acq: 10 Jan 2018 10:40

Tgt Ion: 136 Resp: 277687


Ion Ratio Lower Upper

136 100



137 10.2 9.2 13.8


54 5.3 10.3 15.5#

68 3.5 4.5 6.7#



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

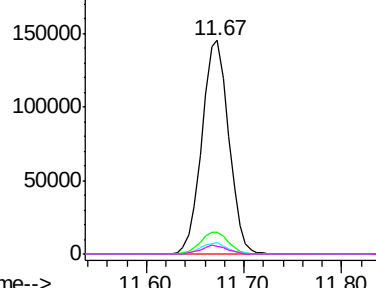







#23
 Nitrobenzene-d5
 Concen: 89.311 ng
 RT: 9.99 min Scan# 1140
 Delta R.T. -0.00 min
 Lab File: BG031975.D
 Acq: 10 Jan 2018 10:40

Instrument :
 BNA_G
 ClientSampleId :
 PB105532TB

Tgt Ion: 82 Resp: 328429
 Ion Ratio Lower Upper
 82 100
 128 50.5 29.7 44.5#
 54 44.3 43.1 64.7

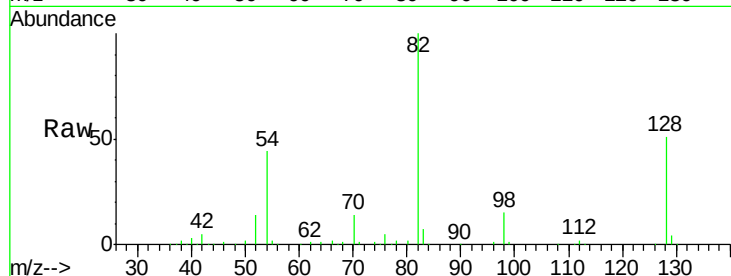


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC


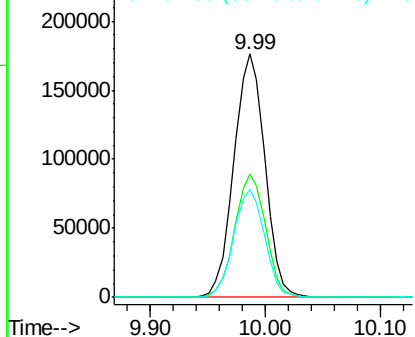



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.42 min Scan# 2064
 Delta R.T. -0.01 min
 Lab File: BG031975.D
 Acq: 10 Jan 2018 10:40

Tgt Ion: 164 Resp: 189518
 Ion Ratio Lower Upper
 164 100
 162 108.0 78.8 118.2
 160 44.8 35.4 53.0



Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

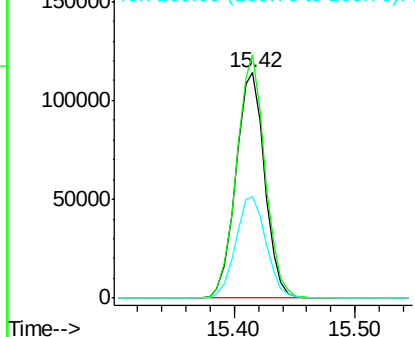


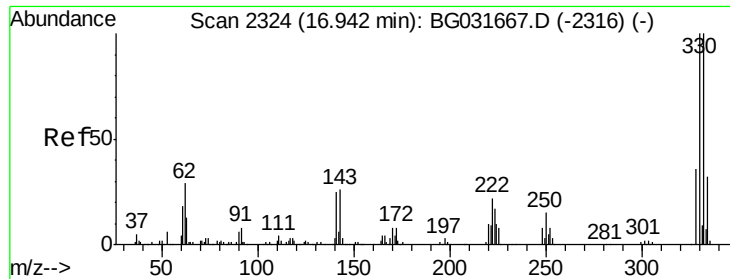




#41
 2,4,6-Tribromophenol
 Concen: 119.054 ng
 RT: 16.88 min Scan# 2314
 Delta R.T. -0.02 min
 Lab File: BG031975.D
 Acq: 10 Jan 2018 10:40

Instrument :
 BNA_G
 ClientSampleId :
 PB105532TB

Tgt Ion:330 Resp: 344277
 Ion Ratio Lower Upper
 330 100
 332 96.7 77.0 115.6
 141 27.1 25.2 37.8

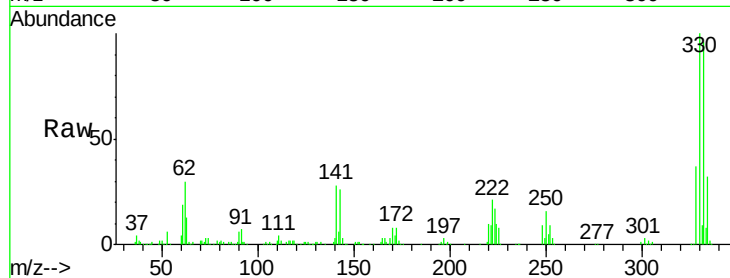


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

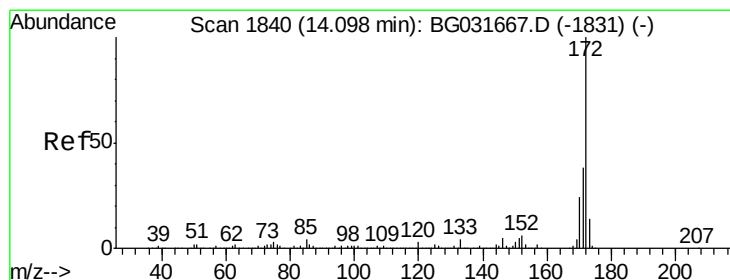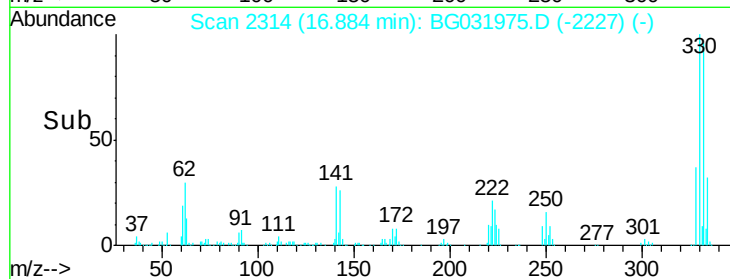
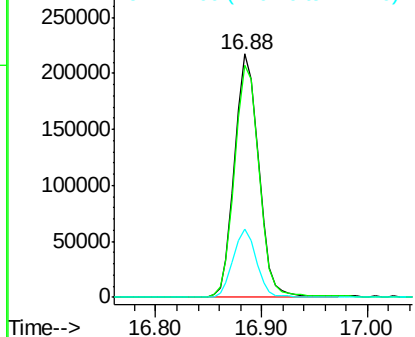



#44
 2-Fluorobiphenyl
 Concen: 78.674 ng
 RT: 14.05 min Scan# 1831
 Delta R.T. -0.01 min
 Lab File: BG031975.D
 Acq: 10 Jan 2018 10:40

Tgt Ion:172 Resp: 1187936
 Ion Ratio Lower Upper
 172 100
 171 38.0 30.0 45.0
 170 23.8 19.5 29.3

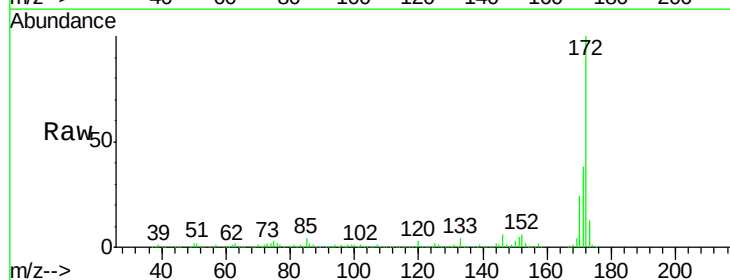

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



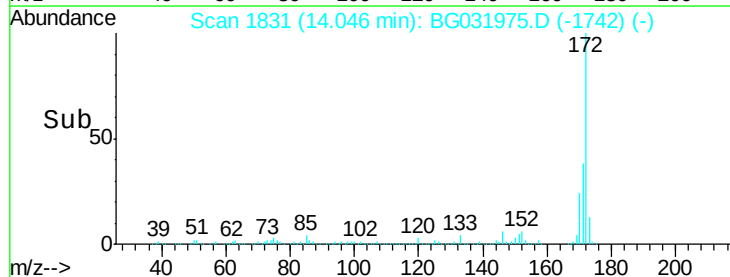
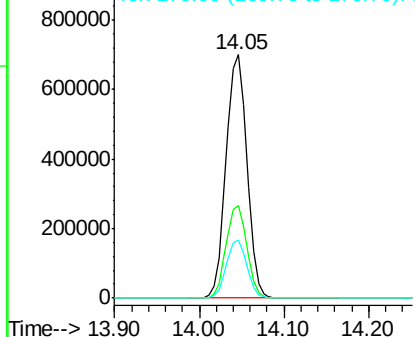




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.14 min Scan# 2528
Delta R.T. -0.02 min
Lab File: BG031975.D
Acq: 10 Jan 2018 10:40




Instrument :
BNA_G
ClientSampleId :
PB105532TB


Tgt Ion:188 Resp: 477441
Ion Ratio Lower Upper
188 100
94 5.3 6.9 10.3#
80 6.2 7.7 11.5#

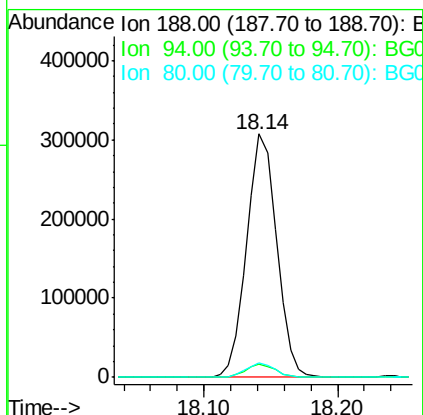

#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.48 min Scan# 3267
Delta R.T. -0.04 min
Lab File: BG031975.D
Acq: 10 Jan 2018 10:40

Tgt Ion:240 Resp: 530066
Ion Ratio Lower Upper
240 100
120 5.5 6.8 10.2#
236 25.1 20.9 31.3

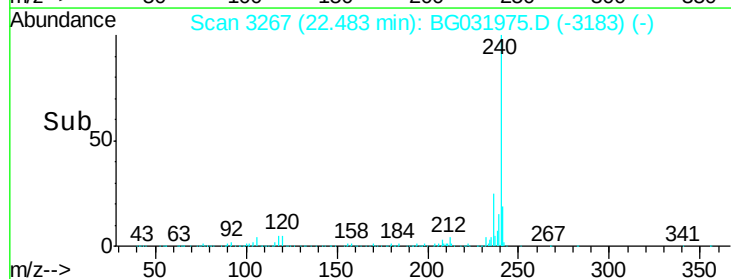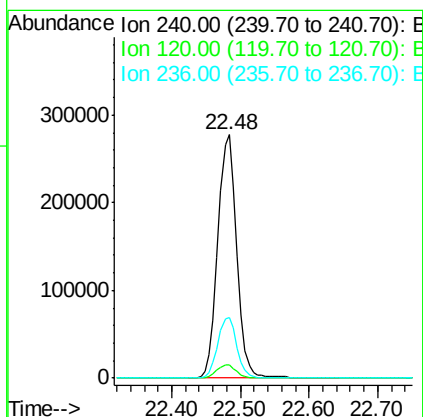

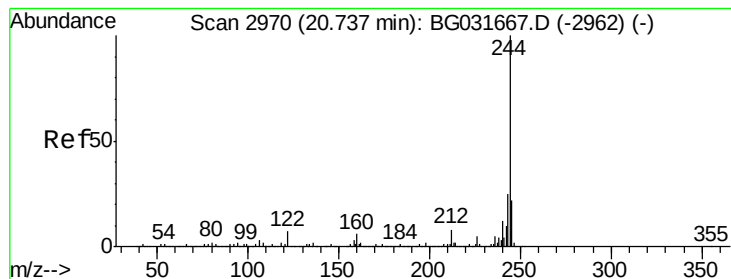

#78

Terphenyl-d14

Concen: 81.855 ng

RT: 20.67 min Scan# 2959

Delta R.T. -0.02 min

Lab File: BG031975.D

Acq: 10 Jan 2018 10:40

Instrument :

BNA_G

ClientSampleId :

PB105532TB


Tgt Ion:244 Resp: 1899124

Ion Ratio Lower Upper

244 100

212 8.0 5.8 8.8




122 7.3 7.0 10.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

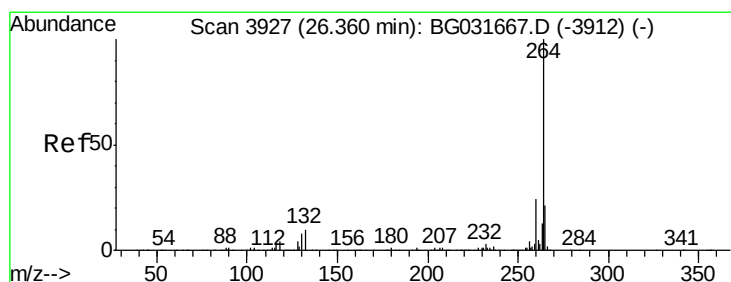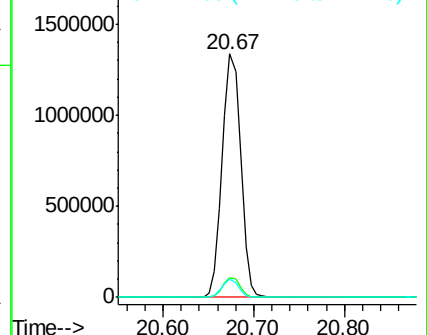

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.21 min Scan# 3901

Delta R.T. -0.09 min

Lab File: BG031975.D

Acq: 10 Jan 2018 10:40


Tgt Ion:264 Resp: 526594

Ion Ratio Lower Upper

264 100

260 23.4 17.4 26.0

265 20.6 17.7 26.5



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

