


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG010918\
 Data File : BG031963.D
 Acq On : 10 Jan 2018 2:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 05 15:31:34 2018

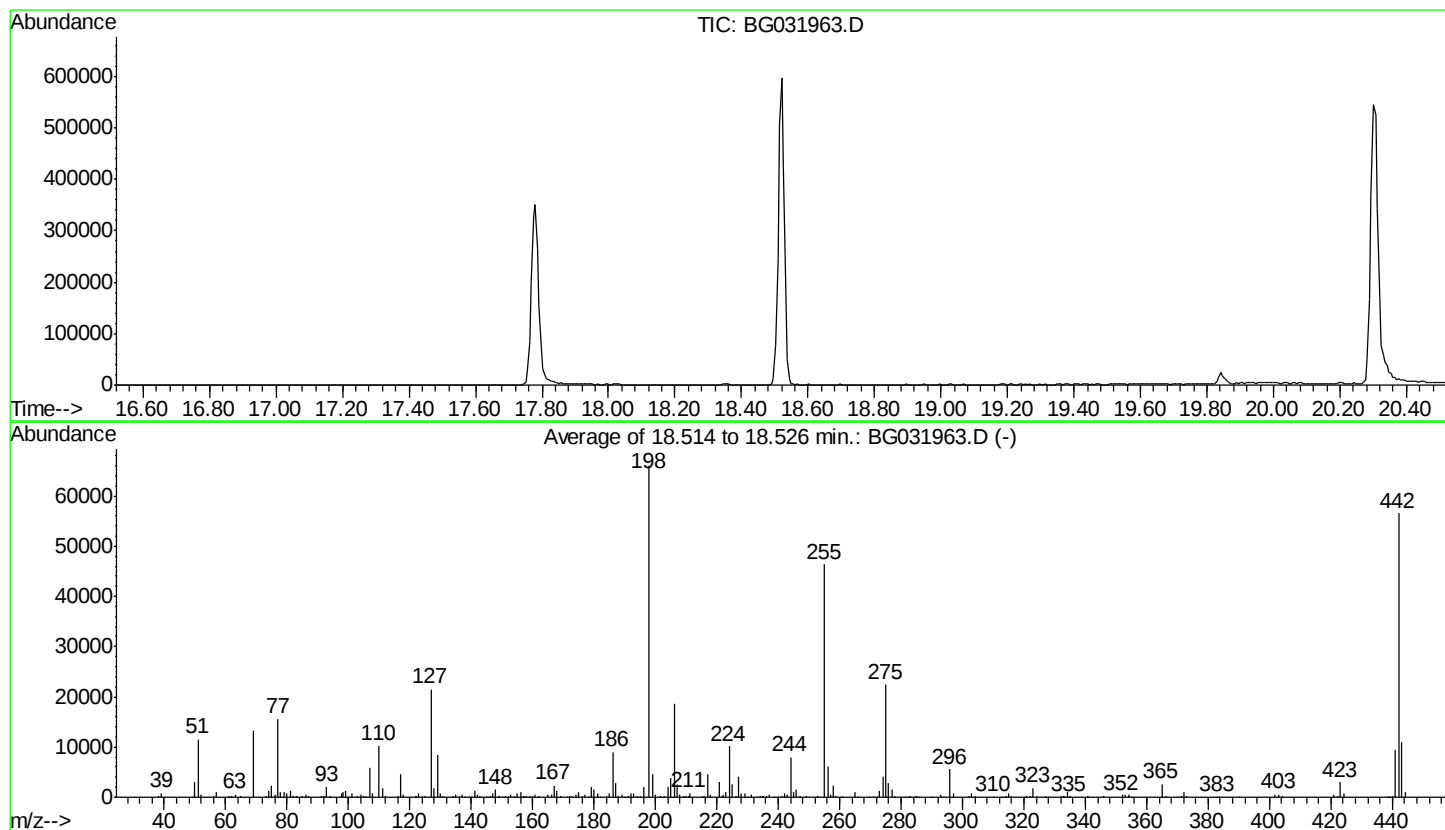

AutoFind: Scans 2591, 2592, 2593; Background Corrected with Scan 2584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.5	11557	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	20.0	13205	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.5	21437	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66037	PASS
199	198	5	9	6.9	4524	PASS
275	198	10	60	33.8	22344	PASS
365	198	1	100	4.0	2631	PASS
441	442	0.01	24	16.8	9476	PASS
442	198	50	100	85.5	56474	PASS
443	442	15	24	19.6	11066	PASS