

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010923\
 Data File : BG056228.D
 Acq On : 9 Jan 2023 9:59
 Operator : CG/JU
 Sample : PB150058BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056228.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.355	7	11	18	rVB	19731	27974	1.68%	0.188%
2	3.631	54	58	64	rBV	8309	13542	0.81%	0.091%
3	4.066	129	132	144	rBV	107623	181956	10.93%	1.223%
4	4.148	144	146	149	rVB	1677	1669	0.10%	0.011%
5	4.418	188	192	198	rVB3	2426	4580	0.28%	0.031%
6	7.462	702	710	724	rVB	149487	263885	15.86%	1.773%
7	7.638	733	740	749	rVB	125354	209272	12.57%	1.406%
8	7.856	770	777	785	rBV	153362	267513	16.07%	1.798%
9	8.332	851	858	866	rBV	145587	242788	14.59%	1.631%
10	9.019	968	975	985	rBV	212987	370327	22.25%	2.488%
11	9.501	1048	1057	1068	rBB	143208	257603	15.48%	1.731%
12	10.229	1174	1181	1189	rBV	129605	229828	13.81%	1.544%
13	10.770	1266	1273	1289	rVB	234529	408784	24.56%	2.747%
14	11.163	1332	1340	1348	rBV	204100	363493	21.84%	2.442%
15	11.287	1353	1361	1371	rVV	212556	367174	22.06%	2.467%
16	12.720	1601	1605	1611	rVB2	4342	7386	0.44%	0.050%
17	14.330	1871	1879	1886	rBV	503473	712713	42.82%	4.789%
18	14.642	1925	1932	1941	rVB	531615	859725	51.66%	5.777%
19	14.941	1976	1983	1991	rVB	410984	637046	38.28%	4.281%
20	15.106	2004	2011	2025	rBV	162579	266050	15.99%	1.788%
21	15.923	2143	2150	2159	rVB	758715	1175651	70.64%	7.900%
22	16.028	2161	2168	2177	rVV	177581	262066	15.75%	1.761%
23	16.163	2186	2191	2196	rVB	2915	4680	0.28%	0.031%
24	16.974	2325	2329	2334	rVB	1142	1695	0.10%	0.011%
25	17.679	2442	2449	2458	rVV	594136	876647	52.67%	5.890%
26	17.779	2458	2466	2476	rVB	868795	1335891	80.27%	8.976%
27	18.044	2508	2511	2514	rVB3	1590	1789	0.11%	0.012%
28	18.755	2628	2632	2635	rBV4	1425	1929	0.12%	0.013%
29	19.442	2748	2749	2754	rBV3	2508	2430	0.15%	0.016%
30	19.612	2773	2778	2782	rBV3	13177	16740	1.01%	0.112%
31	19.677	2785	2789	2793	rBV	14493	20196	1.21%	0.136%
32	19.748	2799	2801	2803	rVB3	3032	2565	0.15%	0.017%
33	19.783	2803	2807	2810	rBV4	2045	3680	0.22%	0.025%
34	19.924	2830	2831	2835	rVB4	1945	1703	0.10%	0.011%
35	20.041	2844	2851	2858	rBV	1182717	1664334	100.00%	11.183%
36	20.153	2868	2870	2873	rVB4	2273	1867	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010923\
 Data File : BG056228.D
 Acq On : 9 Jan 2023 9:59
 Operator : CG/JU
 Sample : PB150058BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
 Title : SVOA CALIBRATION

37	20.494	2927	2928	2929	rBV	3364	1753	0.11%	0.012%
38	20.629	2949	2951	2953	rBV3	4319	2860	0.17%	0.019%
39	20.646	2953	2954	2956	rBV2	3422	2917	0.18%	0.020%
40	21.064	3024	3025	3028	rBV4	4608	4295	0.26%	0.029%
41	21.475	3093	3095	3099	rVB5	4505	4865	0.29%	0.033%
42	21.669	3126	3128	3132	rBV4	3451	3959	0.24%	0.027%
43	21.974	3173	3180	3188	rVB2	587765	996088	59.85%	6.693%
44	22.726	3303	3308	3312	rBV8	6652	13925	0.84%	0.094%
45	23.525	3441	3444	3449	rVB6	8570	13334	0.80%	0.090%
46	23.649	3463	3465	3466	rBV	5086	4234	0.25%	0.028%
47	23.749	3480	3482	3485	rBV4	3521	3164	0.19%	0.021%
48	24.090	3538	3540	3541	rBV2	4065	2564	0.15%	0.017%
49	24.659	3635	3637	3638	rVB2	4326	2179	0.13%	0.015%
50	25.200	3716	3729	3743	rVV2	546526	1629267	97.89%	10.948%
51	25.306	3746	3747	3750	rVB3	4433	3391	0.20%	0.023%
52	25.435	3758	3769	3781	rVB	335597	1013372	60.89%	6.809%
53	26.158	3888	3892	3893	rBV4	10057	12029	0.72%	0.081%
54	26.645	3969	3975	3983	rVB9	19337	53885	3.24%	0.362%
55	26.733	3988	3990	3991	rBV2	3752	2752	0.17%	0.018%
56	27.192	4066	4068	4069	rBV2	3739	3011	0.18%	0.020%
57	27.533	4124	4126	4130	rBV4	4218	6500	0.39%	0.044%
58	27.679	4149	4151	4152	rBV2	3687	2601	0.16%	0.017%
59	28.978	4370	4372	4373	rBV2	4570	2702	0.16%	0.018%
60	29.101	4391	4393	4396	rBV4	4786	2966	0.18%	0.020%
61	29.372	4437	4439	4441	rBV3	3809	2375	0.14%	0.016%
62	30.365	4606	4608	4610	rBV2	3669	1996	0.12%	0.013%
63	30.934	4703	4705	4707	rBV3	3583	2997	0.18%	0.020%
64	31.281	4762	4764	4767	rBV4	3493	3278	0.20%	0.022%
65	31.434	4788	4790	4791	rBV2	3953	2524	0.15%	0.017%
66	32.016	4886	4889	4890	rBV3	7629	7855	0.47%	0.053%
67	32.591	4984	4987	4990	rBV5	5712	5594	0.34%	0.038%




Sum of corrected areas: 14882403

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010923\
Data File : BG056228.D
Acq On : 9 Jan 2023 9:59
Operator : CG/JU
Sample : PB150058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

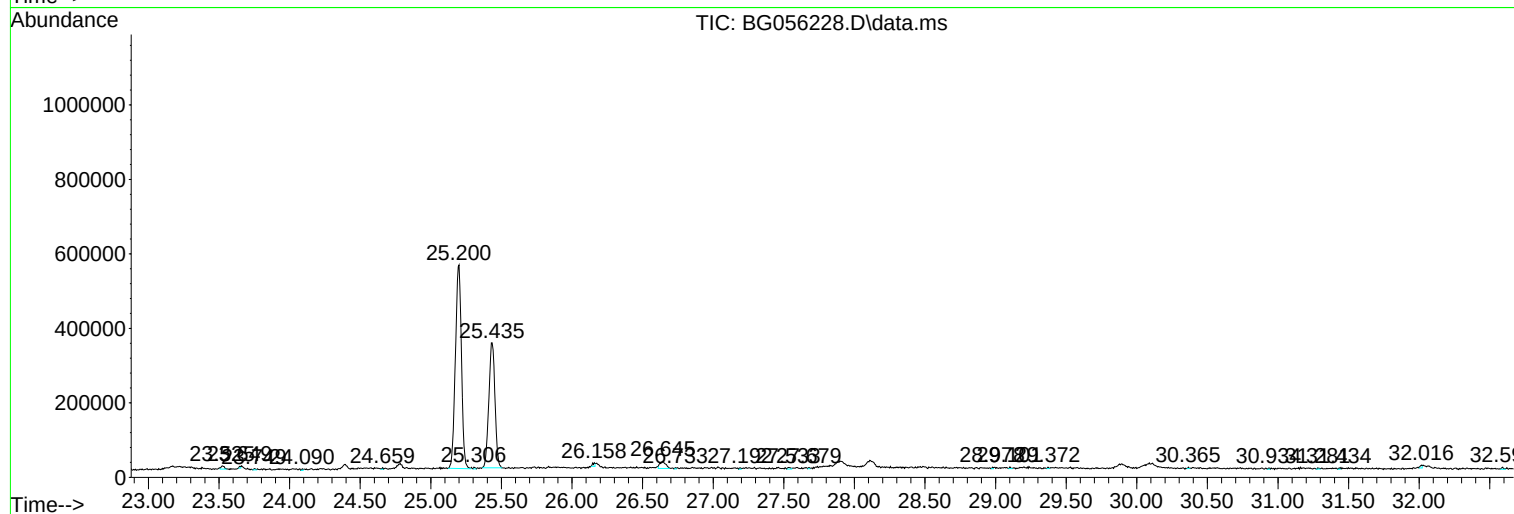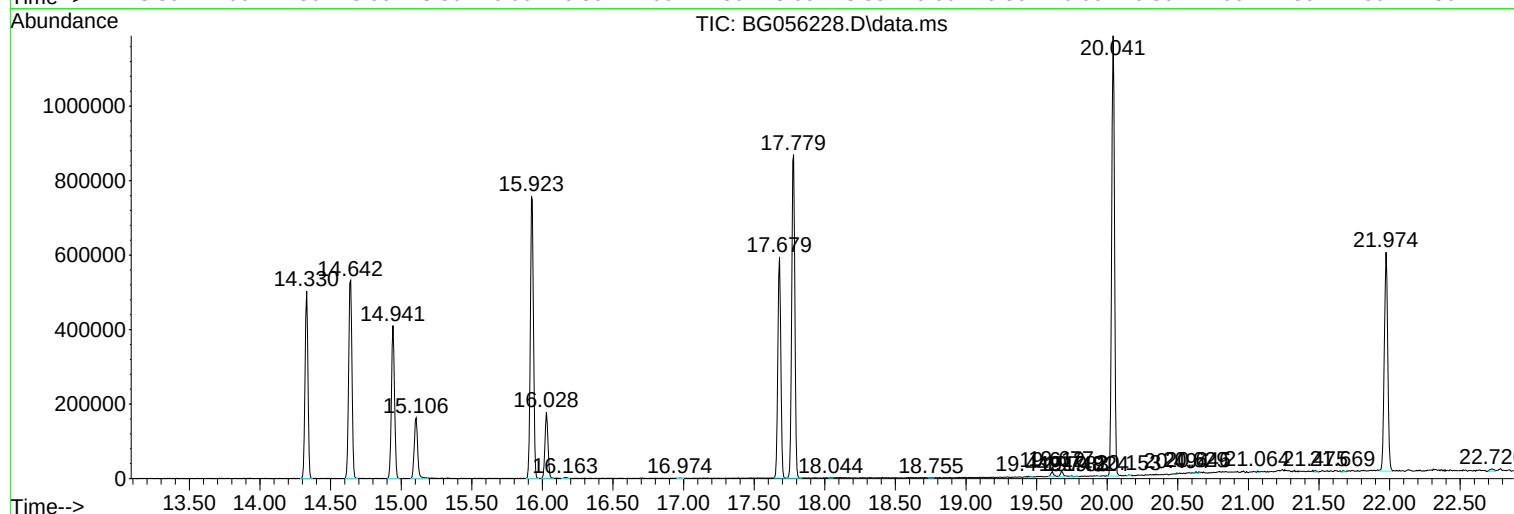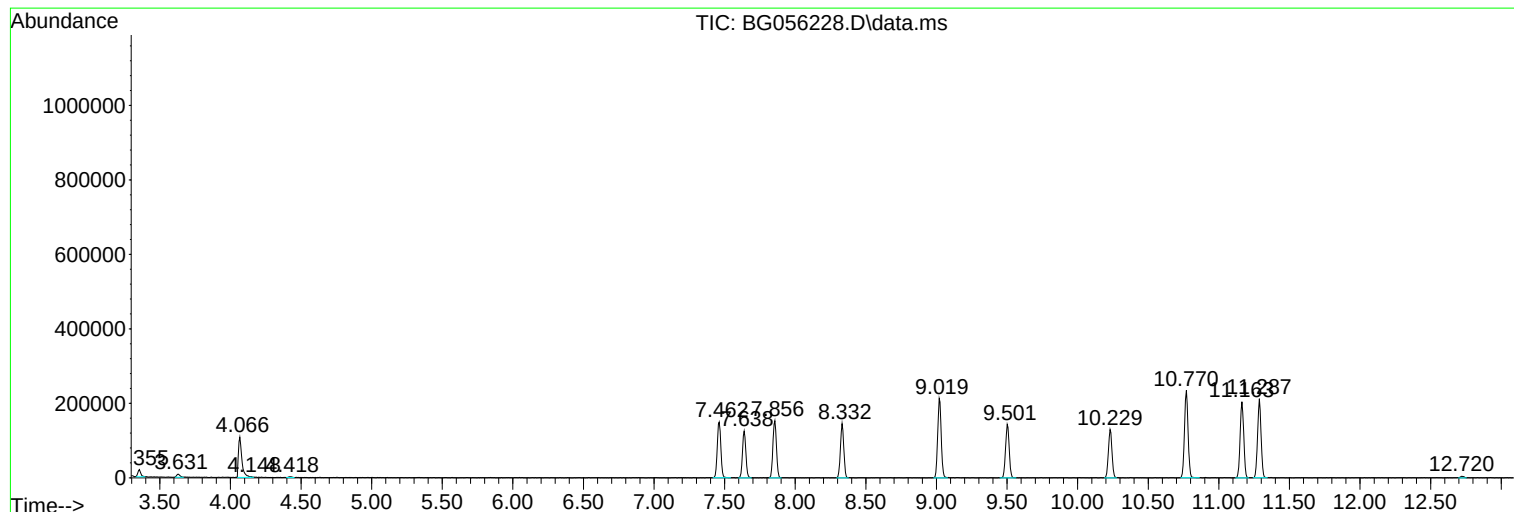

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010923\
Data File : BG056228.D
Acq On : 9 Jan 2023 9:59
Operator : CG/JU
Sample : PB150058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK058










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.355	2.30 ng/ul	27974	1,4-Dichlorobenzene-d4	8.332

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	45
2			1,3-Dioxolane, 2-(1-methylethyl)-	116	C6H12O2	000822-83-3	17
3			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	17
4			Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9
5			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9

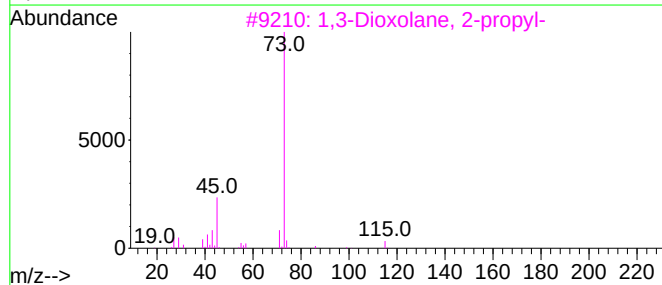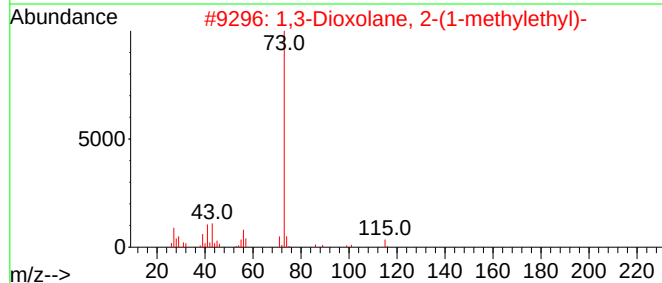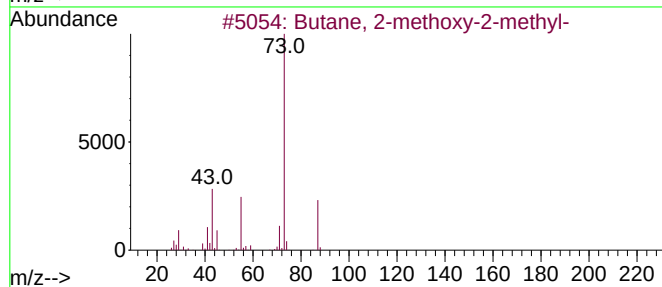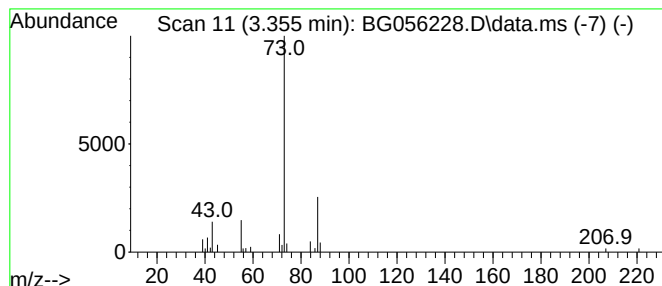

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010923\
Data File : BG056228.D
Acq On : 9 Jan 2023 9:59
Operator : CG/JU
Sample : PB150058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.355	2.3	ng/u1	27974	1	8.332	242788	20.0