

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010923\
 Data File : BG056232.D
 Acq On : 9 Jan 2023 13:48
 Operator : CG/JU
 Sample : PB150061BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	6	11	20	rVV	22329	35946	2.16%	0.221%
2	3.423	20	23	26	rVB2	1334	2142	0.13%	0.013%
3	3.628	54	58	65	rVB	10099	15404	0.93%	0.095%
4	4.057	127	131	144	rBV	125171	211269	12.71%	1.301%
5	4.139	144	145	148	rVB	2189	1755	0.11%	0.011%
6	4.416	187	192	200	rBV	9808	16756	1.01%	0.103%
7	7.459	703	710	723	rBV	178914	310554	18.68%	1.913%
8	7.635	730	740	750	rBV	150238	246621	14.84%	1.519%
9	7.853	769	777	787	rVB	185116	313773	18.87%	1.933%
10	8.329	850	858	865	rBB	174251	291829	17.55%	1.798%
11	9.016	968	975	985	rBV	245586	428431	25.77%	2.639%
12	9.498	1049	1057	1066	rBB	165475	295737	17.79%	1.822%
13	10.226	1174	1181	1189	rBV	148849	271740	16.35%	1.674%
14	10.767	1265	1273	1282	rBV	264139	472821	28.44%	2.913%
15	11.161	1332	1340	1348	rBV	243713	428927	25.80%	2.642%
16	11.284	1354	1361	1374	rVB	226302	418508	25.17%	2.578%
17	12.724	1601	1606	1613	rBV2	4785	8088	0.49%	0.050%
18	14.328	1872	1879	1886	rBV	532287	771932	46.43%	4.755%
19	14.639	1925	1932	1940	rVB	611995	962519	57.90%	5.929%
20	14.944	1976	1984	1993	rVB	463899	729998	43.91%	4.497%
21	15.103	2005	2011	2019	rBV	170900	281795	16.95%	1.736%
22	15.332	2047	2050	2057	rVB	1569	1872	0.11%	0.012%
23	15.926	2144	2151	2159	rBV	854911	1281779	77.10%	7.896%
24	16.031	2163	2169	2178	rBV	191999	287300	17.28%	1.770%
25	16.161	2188	2191	2199	rVB3	3814	5300	0.32%	0.033%
26	17.471	2410	2414	2418	rVB2	1231	2149	0.13%	0.013%
27	17.677	2443	2449	2459	rVB	588530	933041	56.13%	5.747%
28	17.776	2459	2466	2476	rBV	912370	1380310	83.03%	8.503%
29	18.053	2510	2513	2515	rBV3	1615	1762	0.11%	0.011%
30	18.899	2653	2657	2661	rVB	1007	1676	0.10%	0.010%
31	19.175	2699	2704	2708	rBV3	981	2005	0.12%	0.012%
32	19.615	2772	2779	2785	rVB3	14032	21846	1.31%	0.135%
33	19.680	2785	2790	2796	rBV	12019	22270	1.34%	0.137%
34	19.927	2830	2832	2834	rVB2	3235	2733	0.16%	0.017%
35	19.986	2839	2842	2843	rBV3	2215	2384	0.14%	0.015%
36	20.044	2846	2852	2860	rVB	1214717	1662423	100.00%	10.240%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010923\
 Data File : BG056232.D
 Acq On : 9 Jan 2023 13:48
 Operator : CG/JU
 Sample : PB150061BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
 Title : SVOA CALIBRATION

37	20.473	2923	2925	2928	rBV3	2573	3177	0.19%	0.020%
38	20.538	2934	2936	2938	rBV3	2193	1718	0.10%	0.011%
39	20.732	2967	2969	2971	rBV2	2558	2615	0.16%	0.016%
40	20.961	3006	3008	3012	rVB5	5354	4506	0.27%	0.028%
41	21.167	3041	3043	3044	rBV2	3180	2084	0.13%	0.013%
42	21.977	3173	3181	3188	rVB	610862	1035167	62.27%	6.377%
43	22.788	3315	3319	3320	rBV4	7168	8593	0.52%	0.053%
44	22.953	3345	3347	3350	rVB3	3635	3141	0.19%	0.019%
45	23.528	3441	3445	3451	rVB7	15172	29383	1.77%	0.181%
46	23.740	3479	3481	3482	rBV2	4682	3291	0.20%	0.020%
47	24.398	3588	3593	3599	rVB7	20430	39713	2.39%	0.245%
48	24.774	3653	3657	3658	rBV3	5994	8959	0.54%	0.055%
49	25.080	3708	3709	3711	rBV2	3370	2721	0.16%	0.017%
50	25.197	3718	3729	3742	rBV2	555022	1642891	98.83%	10.120%
51	25.438	3758	3770	3783	rBV2	359155	1109411	66.73%	6.834%
52	26.049	3872	3874	3876	rBV3	3410	3236	0.19%	0.020%
53	26.642	3966	3975	3985	rBV5	30472	97329	5.85%	0.600%
54	26.742	3991	3992	3994	rBV2	3764	2268	0.14%	0.014%
55	27.306	4086	4088	4089	rBV2	3455	2546	0.15%	0.016%
56	28.117	4218	4226	4227	rBV8	26758	50339	3.03%	0.310%
57	28.241	4245	4247	4248	rBV2	3480	1909	0.11%	0.012%
58	28.905	4359	4360	4362	rBV2	4052	3656	0.22%	0.023%
59	29.439	4449	4451	4453	rBV3	4313	3847	0.23%	0.024%
60	29.633	4482	4484	4487	rBV4	4704	6290	0.38%	0.039%
61	29.786	4508	4510	4513	rBV4	4112	4942	0.30%	0.030%
62	30.902	4698	4700	4701	rVB2	5021	2647	0.16%	0.016%
63	30.973	4710	4712	4713	rBV2	3757	2898	0.17%	0.018%
64	31.384	4780	4782	4785	rVB4	4989	3960	0.24%	0.024%
65	31.413	4785	4787	4794	rBV6	3730	8180	0.49%	0.050%
66	31.784	4848	4850	4851	rBV2	3593	2313	0.14%	0.014%
67	32.019	4889	4890	4891	rBV	6313	3742	0.23%	0.023%
68	32.042	4891	4894	4895	rVV3	7629	7715	0.46%	0.048%
69	32.630	4992	4994	4996	rBV3	3450	3482	0.21%	0.021%




Sum of corrected areas: 16234064

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010923\
Data File : BG056232.D
Acq On : 9 Jan 2023 13:48
Operator : CG/JU
Sample : PB150061BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

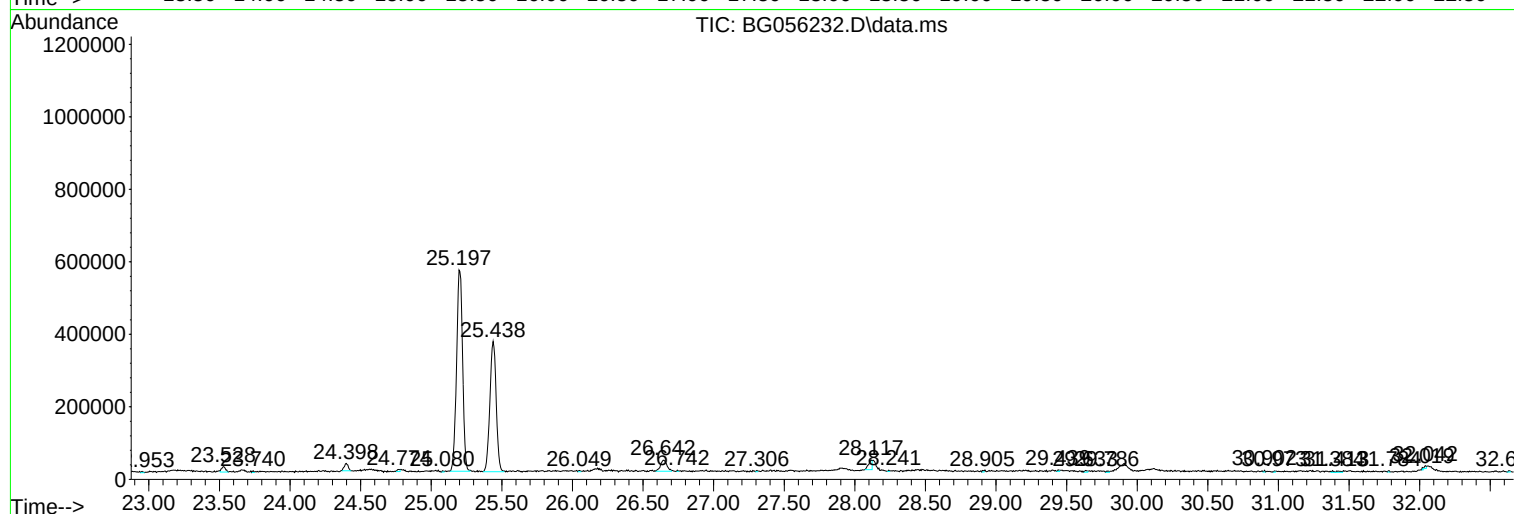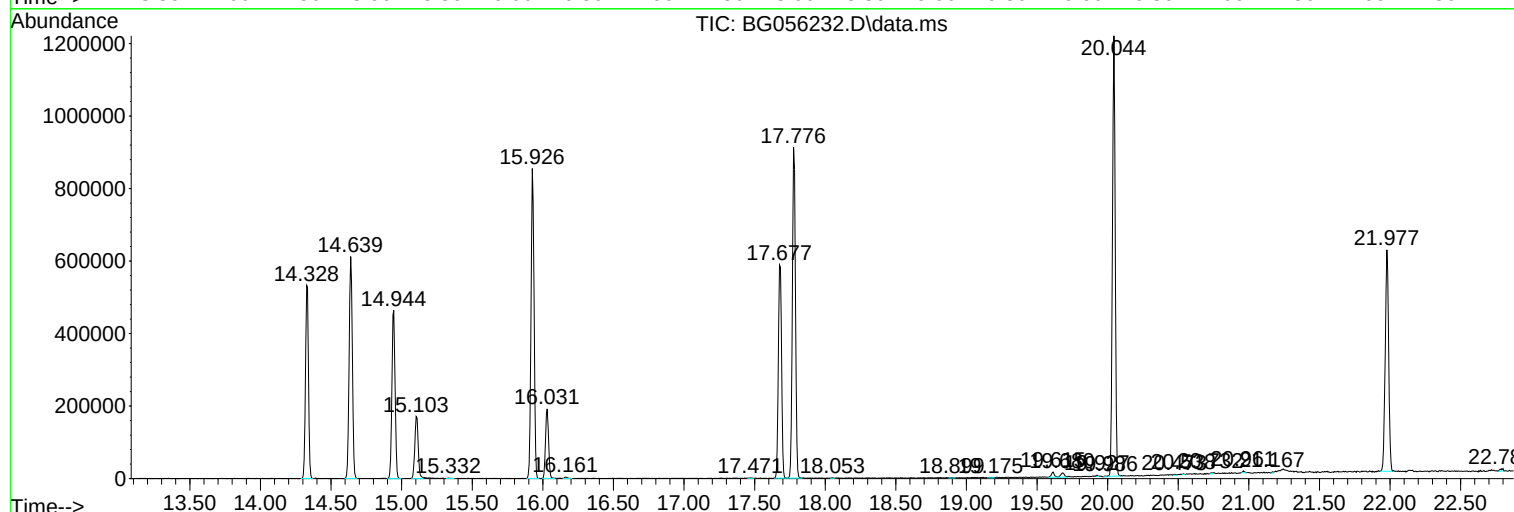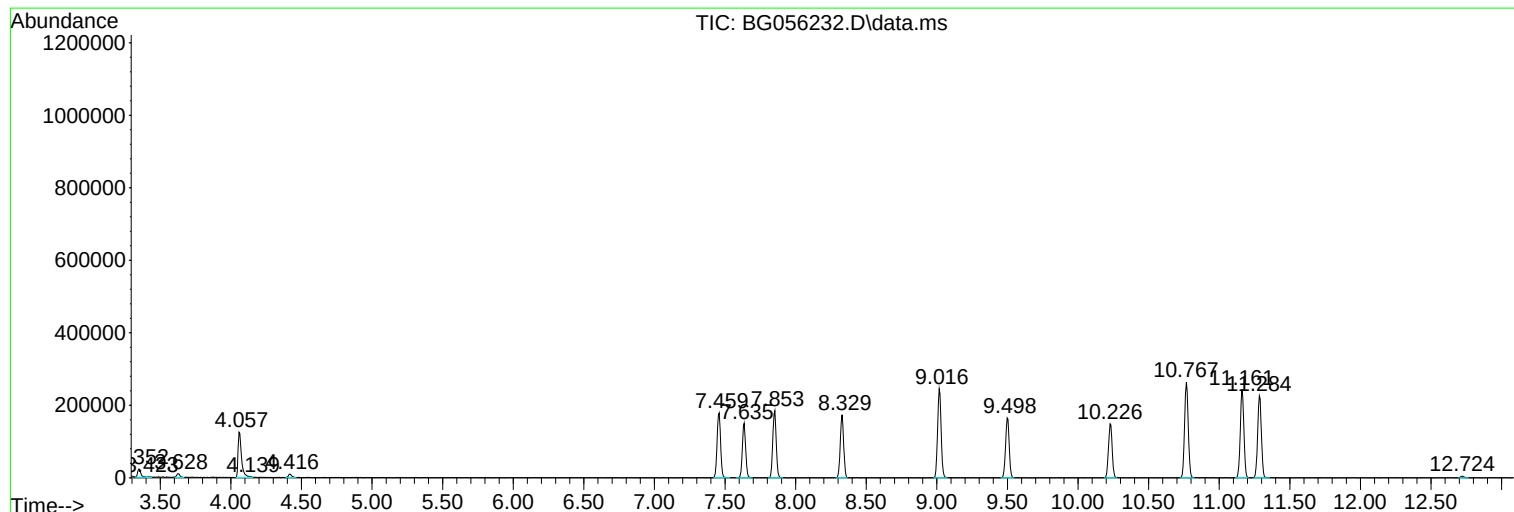

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010923\
Data File : BG056232.D
Acq On : 9 Jan 2023 13:48
Operator : CG/JU
Sample : PB150061BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK061










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.352	2.46 ng/ul	35946	1,4-Dichlorobenzene-d4	8.329

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
2			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
3			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9
4			N-Ethylformamide	73	C3H7NO	000627-45-2	7
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	7

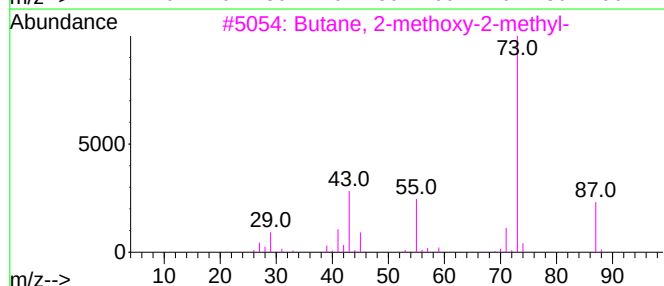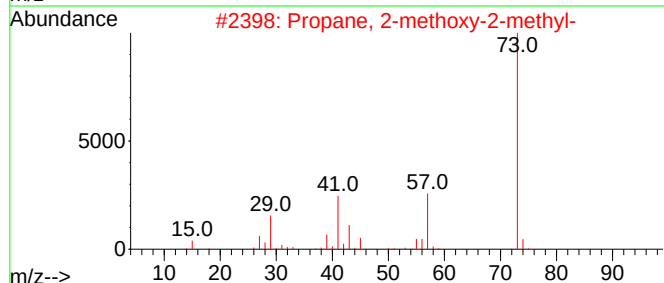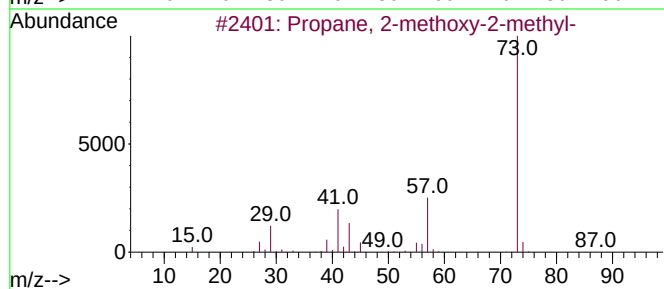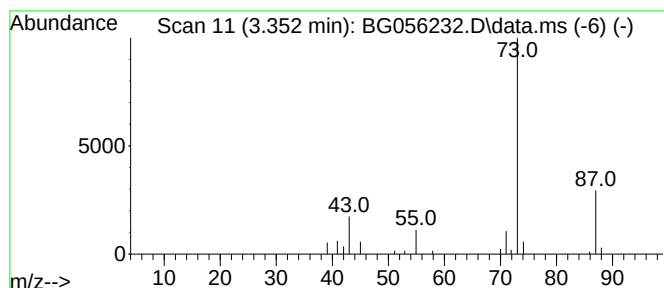

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010923\
Data File : BG056232.D
Acq On : 9 Jan 2023 13:48
Operator : CG/JU
Sample : PB150061BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.352	2.5	ng/u1	35946	1	8.329	291829	20.0