

Data Path : Z:\HPCHEM1\BNA G\DATA\BG011017\
 Data File : BG025452.D
 Acq On : 10 Jan 2017 11:13
 Operator : UM/SJ
 Sample : I1064-11RE
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP5-6-COMP11

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.184	54	59	64	rBV4	44440	89634	1.42%	0.310%
2	3.577	122	126	136	rVB2	63474	95203	1.51%	0.329%
3	4.018	196	201	210	rVB	210626	320099	5.08%	1.106%
4	4.641	300	307	318	rBV	1544404	2385228	37.86%	8.242%
5	4.741	318	324	333	rVV4	44853	107087	1.70%	0.370%
6	5.740	487	494	507	rBV	1161723	2048092	32.51%	7.077%
7	7.250	744	751	759	rBV2	92596	205935	3.27%	0.712%
8	7.361	762	770	785	rVV2	674638	1323730	21.01%	4.574%
9	7.731	825	833	843	rBV	1258101	2287541	36.31%	7.904%
10	8.201	906	913	924	rVB	234798	432425	6.86%	1.494%
11	8.525	958	968	975	rBV	944016	1744552	27.69%	6.028%
12	8.765	1002	1009	1019	rBV2	138646	268563	4.26%	0.928%
13	9.130	1066	1071	1077	rBV	96033	143101	2.27%	0.494%
14	9.382	1106	1114	1125	rBV	817089	1597495	25.35%	5.520%
15	11.028	1386	1394	1407	rBV2	286801	614212	9.75%	2.122%
16	12.890	1702	1711	1720	rBV8	34289	94736	1.50%	0.327%
17	13.448	1797	1806	1814	rBV	2182006	3491489	55.42%	12.064%
18	14.829	2034	2041	2051	rVB2	230665	406937	6.46%	1.406%
19	16.315	2287	2294	2307	rBV2	1984756	3340626	53.02%	11.543%
20	17.573	2501	2508	2520	rBV2	581300	1010021	16.03%	3.490%
21	20.152	2941	2947	2955	rBV	4743836	6300598	100.00%	21.770%
22	21.868	3232	3239	3249	rBV2	306871	634127	10.06%	2.191%




Sum of corrected areas: 28941431

Data Path : Z:\HPCHEM1\BNA G\DATA\BG011017\
Data File : BG025452.D
Acq On : 10 Jan 2017 11:13
Operator : UM/SJ
Sample : I1064-11RE
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP5-6-COMP11

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

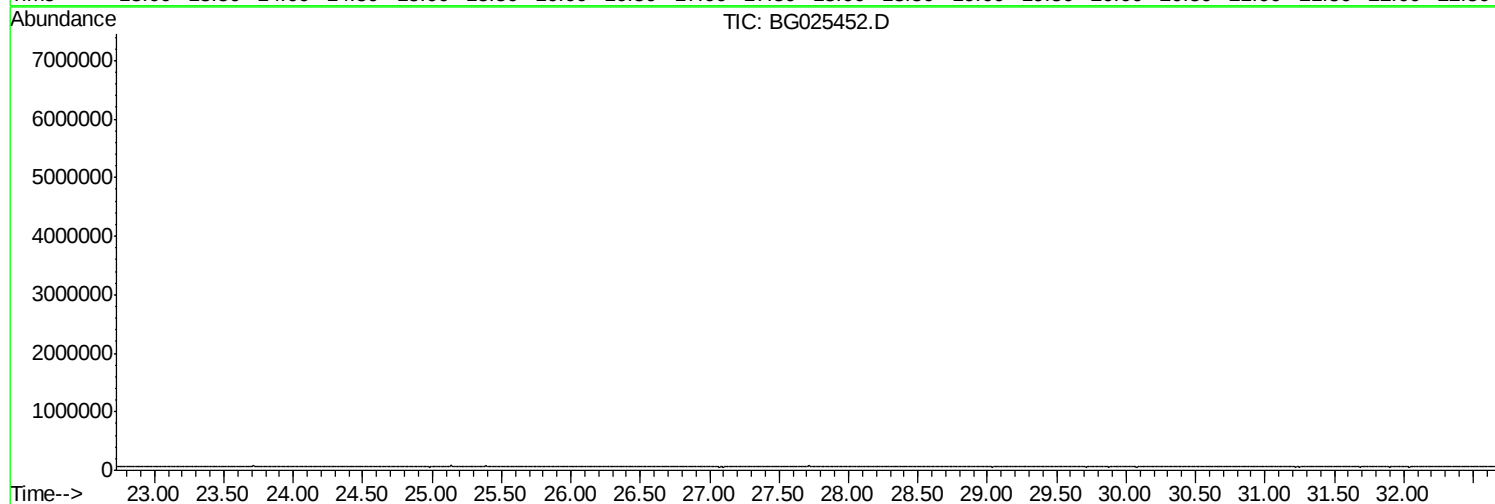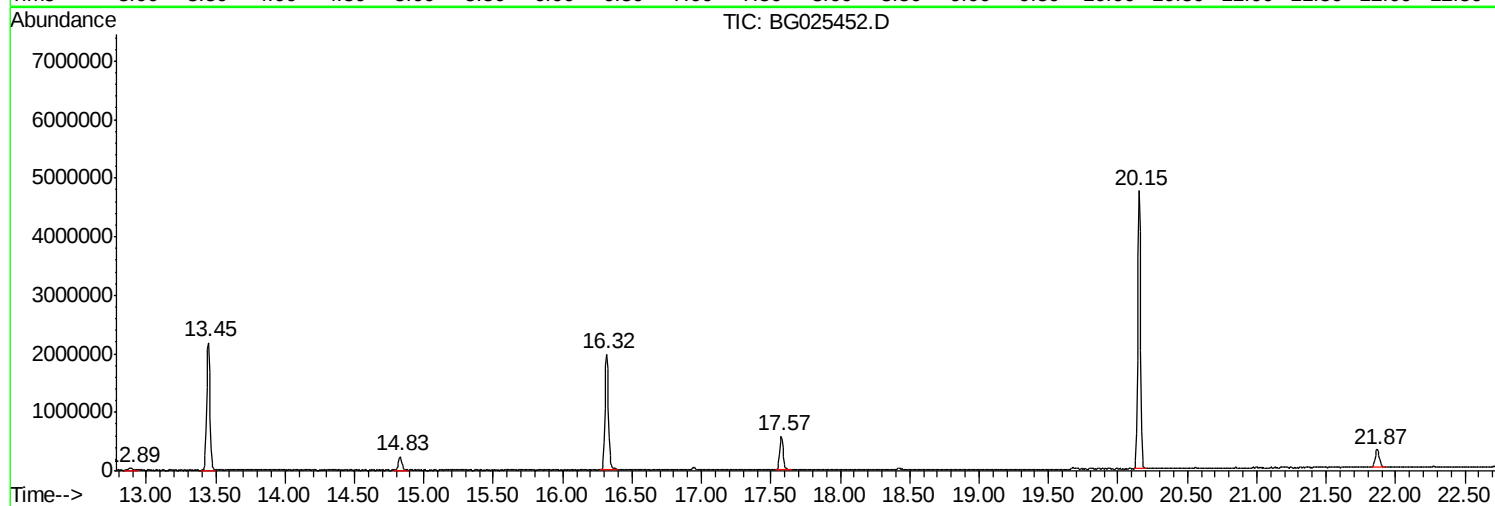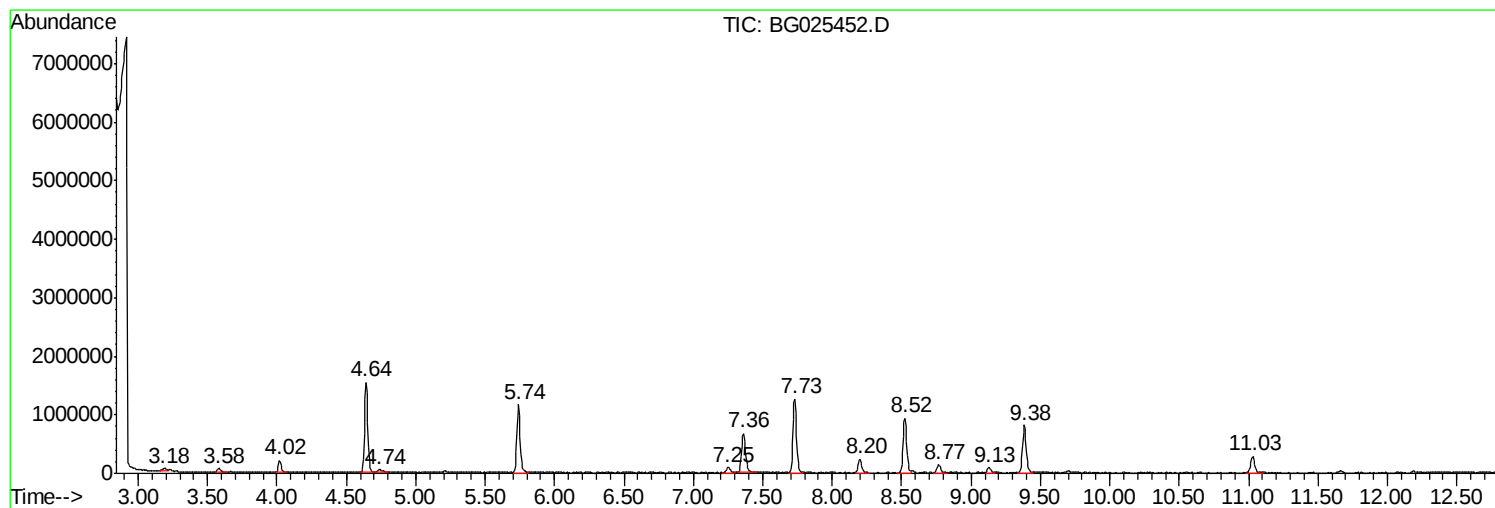

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG011017\
Data_File : BG025452.D
Acq_On : 10 Jan 2017 11:133
Operator : UM/SJJ
Sample : I1064-11REE
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
TP5-6-COMP11

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
