


Data Path : Z:\HPCHEM1\BNA G\DATA\BG011017\
 Data File : BG025450.D
 Acq On : 10 Jan 2017 9:56
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 10 11:26:22 2017

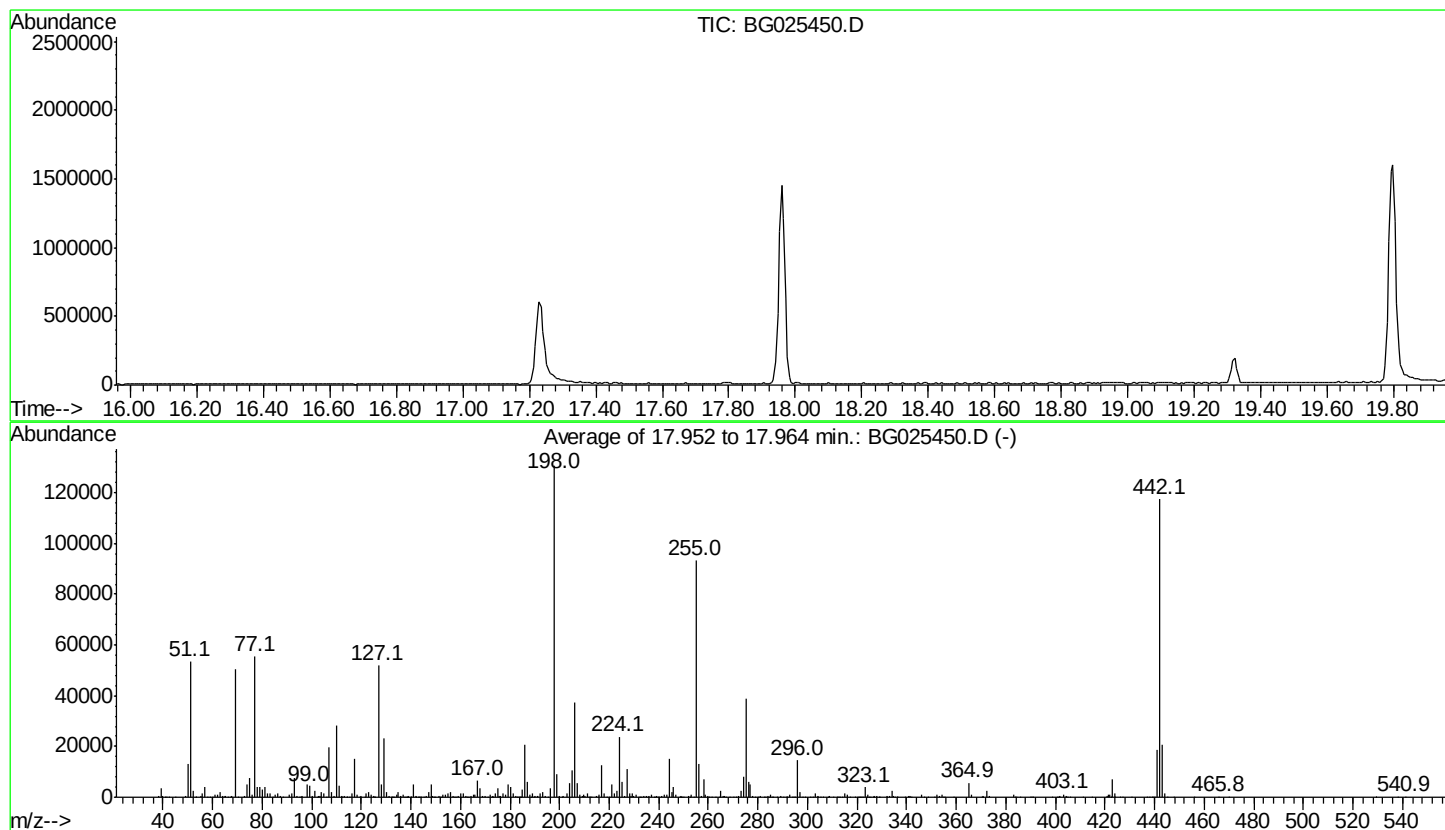

AutoFind: Scans 2572, 2573, 2574; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	53448	PASS
68	69	0.00	2	1.1	535	PASS
69	198	0.00	100	38.5	50277	PASS
70	69	0.00	2	0.5	265	PASS
127	198	10	80	39.6	51741	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	130677	PASS
199	198	5	9	7.1	9216	PASS
275	198	10	60	29.8	39005	PASS
365	198	1	100	4.3	5623	PASS
441	442	0.01	24	15.8	18619	PASS
442	198	50	100	89.9	117496	PASS
443	442	15	24	17.8	20888	PASS