
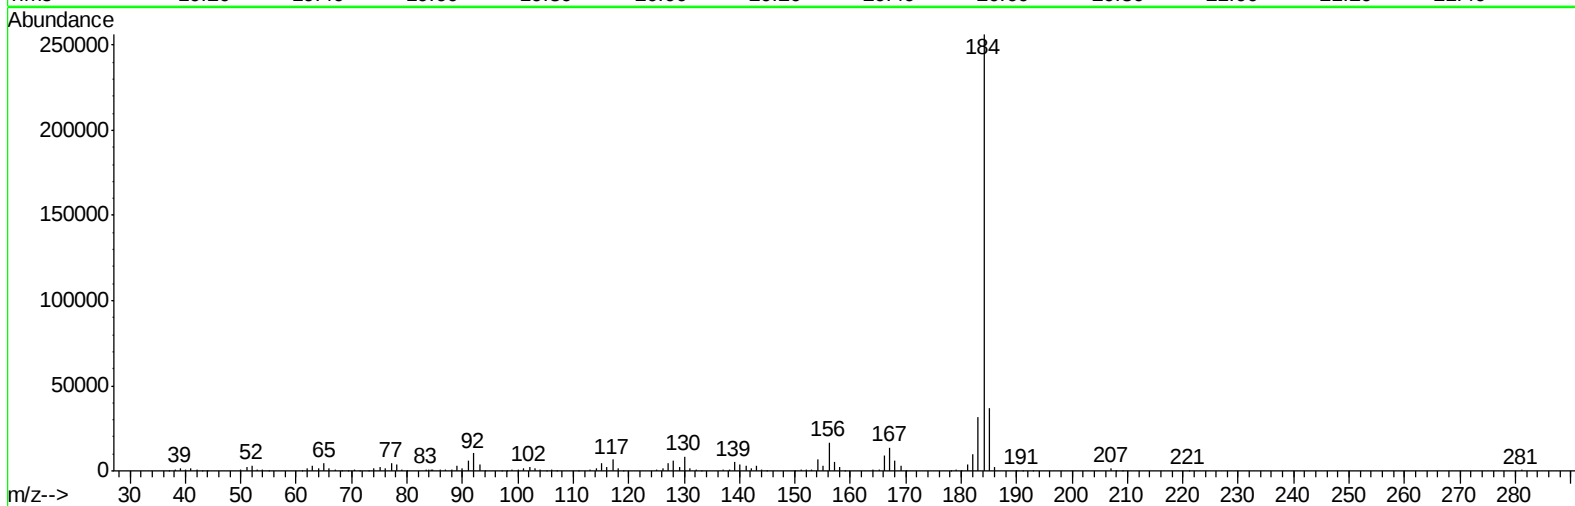


Data Path : Z:\HPCHEM1\BNA G\DATA\BG011018\
Data File : BG031977.D
Acq On : 10 Jan 2018 14:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 01:18:58 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 05 15:31:34 2018
Response via : Initial Calibration

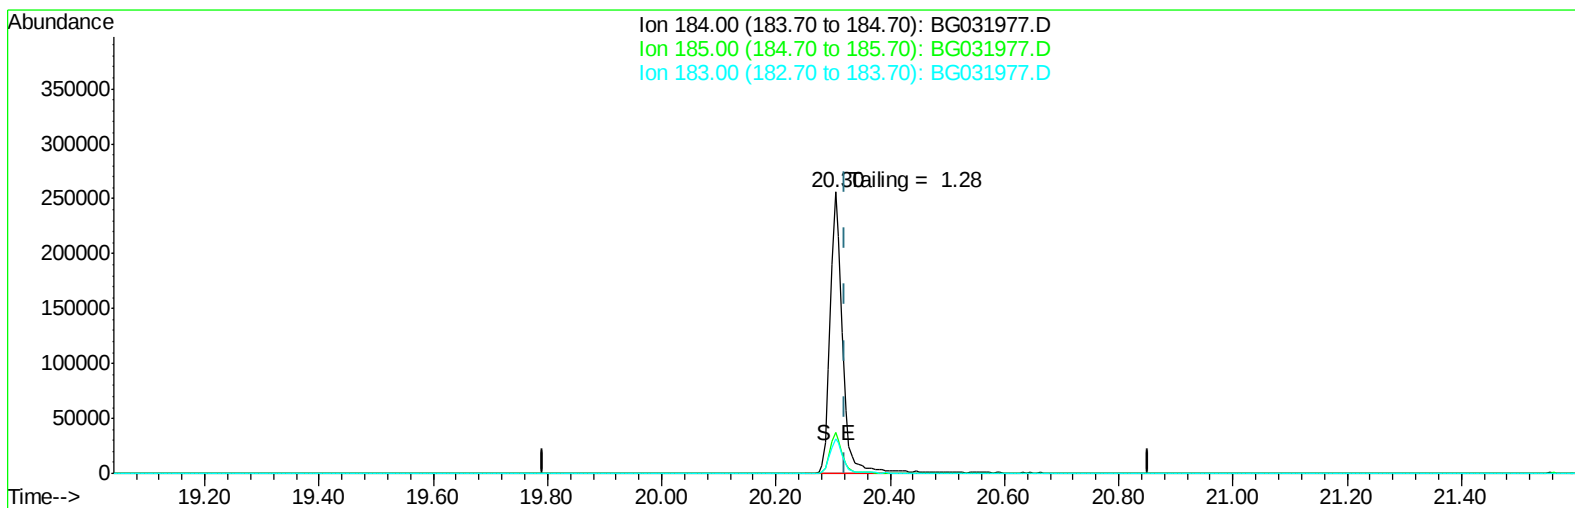

TIC: BG031977.D

(76) Benzidine



20.304min (-0.019) 0.00ng

response 380899

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.36
183.00	13.30	12.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG011018\
Data File : BG031977.D
Acq On : 10 Jan 2018 14:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 01:18:58 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 05 15:31:34 2018
Response via : Initial Calibration

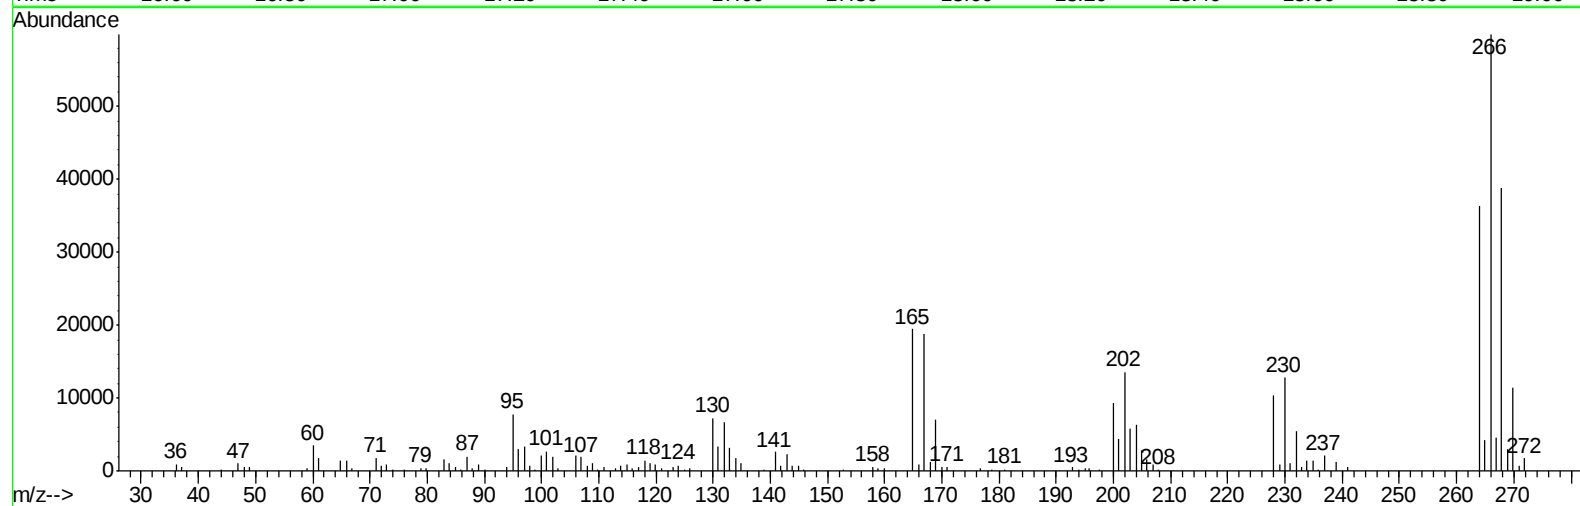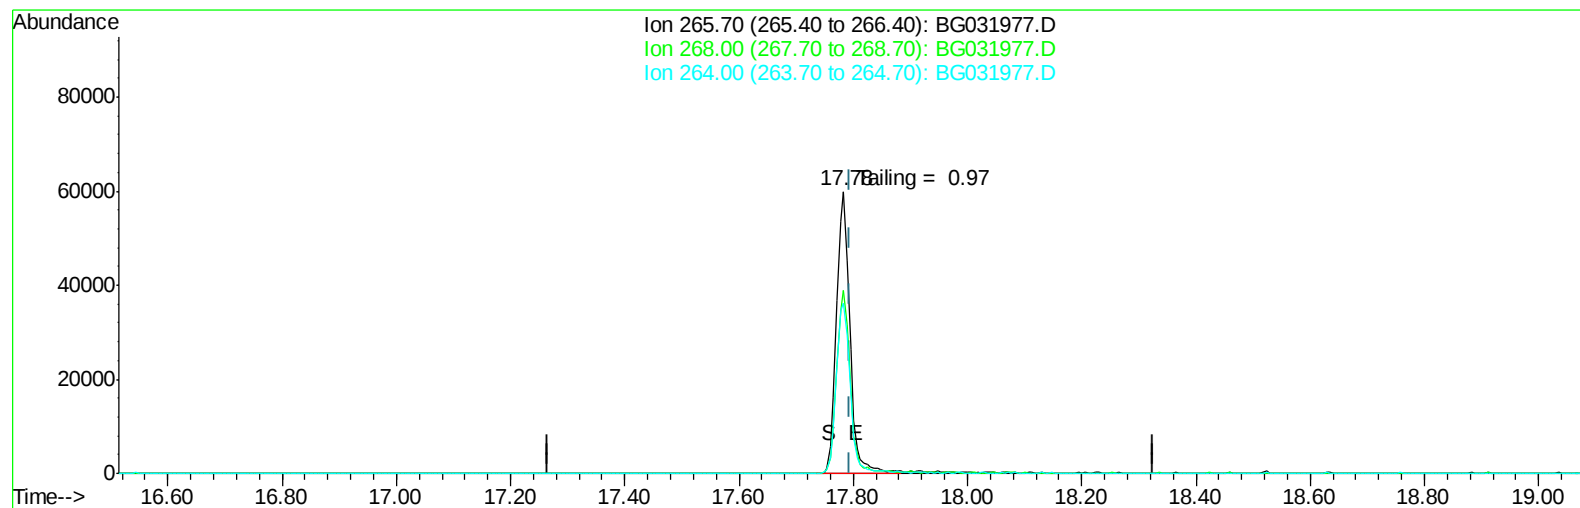

TIC: BG031977.D

(69) Pentachlorophenol (C)

17.783min (-0.013) 18927.72ng

response 96226

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.95
264.00	62.00	60.69
0.00	0.00	0.00