

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011022\
 Data File : BG051932.D
 Acq On : 10 Jan 2022 16:16
 Operator : CG/JU
 Sample : PB141942BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK942

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.576	10	15	21	rVV3	8836	12407	1.24%	0.141%
2	3.629	21	24	28	rVB2	1263	1519	0.15%	0.017%
3	4.005	84	88	99	rBV	99290	169082	16.86%	1.925%
4	4.357	144	148	152	rVV	4173	6132	0.61%	0.070%
5	5.197	290	291	295	rBV	770	1026	0.10%	0.012%
6	6.507	511	514	517	rVB2	848	1138	0.11%	0.013%
7	6.795	558	563	566	rBV2	691	1289	0.13%	0.015%
8	7.059	602	608	609	rVB2	778	1164	0.12%	0.013%
9	7.177	624	628	631	rBV2	809	1530	0.15%	0.017%
10	7.394	656	665	674	rBV	122092	206118	20.56%	2.347%
11	7.565	687	694	703	rVB	81567	138773	13.84%	1.580%
12	7.782	725	731	739	rBV	109223	181648	18.12%	2.068%
13	8.258	805	812	820	rVB	82756	141091	14.07%	1.606%
14	8.957	925	931	940	rVB	135031	237430	23.68%	2.703%
15	9.427	1004	1011	1020	rBV2	107317	199698	19.92%	2.274%
16	10.161	1128	1136	1143	rBV	92402	162288	16.19%	1.848%
17	10.707	1221	1229	1237	rVV	134126	237210	23.66%	2.701%
18	10.760	1237	1238	1242	rVB	977	1098	0.11%	0.013%
19	11.095	1288	1295	1303	rVB	114789	202432	20.19%	2.305%
20	11.218	1309	1316	1325	rBV	139462	251503	25.08%	2.863%
21	12.646	1554	1559	1560	rBV2	810	1054	0.11%	0.012%
22	12.669	1560	1563	1569	rVB3	2389	3392	0.34%	0.039%
23	14.285	1831	1838	1845	rBV	310230	442392	44.12%	5.037%
24	14.590	1882	1890	1896	rBV	301078	471204	47.00%	5.365%
25	14.896	1933	1942	1948	rBV	210941	315451	31.46%	3.591%
26	15.066	1965	1971	1979	rBV	132395	220629	22.01%	2.512%
27	15.883	2102	2110	2117	rBV	416848	614021	61.24%	6.990%
28	15.988	2122	2128	2135	rVV	101694	157487	15.71%	1.793%
29	16.464	2204	2209	2213	rBV2	722	1461	0.15%	0.017%
30	16.558	2224	2225	2230	rBV3	540	1048	0.10%	0.012%
31	16.711	2246	2251	2253	rBV2	664	1071	0.11%	0.012%
32	17.281	2345	2348	2351	rVB2	973	1166	0.12%	0.013%
33	17.434	2369	2374	2376	rBV3	1271	1298	0.13%	0.015%
34	17.645	2403	2410	2417	rVB	297814	462709	46.15%	5.268%
35	17.739	2419	2426	2436	rBV2	507775	787501	78.54%	8.966%
36	18.068	2480	2482	2486	rBV2	699	1187	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011022\
 Data File : BG051932.D
 Acq On : 10 Jan 2022 16:16
 Operator : CG/JU
 Sample : PB141942BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK942

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	18.197	2501	2504	2507	rVB2	1028	1357	0.14%	0.015%
38	18.391	2533	2537	2542	rVB3	1136	1668	0.17%	0.019%
39	18.697	2588	2589	2592	rBV2	1191	1112	0.11%	0.013%
40	18.796	2602	2606	2608	rBV3	1107	1442	0.14%	0.016%
41	18.973	2635	2636	2639	rVB3	1420	1133	0.11%	0.013%
42	19.073	2651	2653	2654	rBV	1306	1056	0.11%	0.012%
43	19.114	2658	2660	2664	rVV3	1440	1736	0.17%	0.020%
44	19.278	2683	2688	2689	rBV3	765	1356	0.14%	0.015%
45	19.331	2695	2697	2700	rBV2	1110	1340	0.13%	0.015%
46	19.484	2721	2723	2726	rVB3	1377	1410	0.14%	0.016%
47	19.519	2727	2729	2732	rVV3	1494	1307	0.13%	0.015%
48	19.584	2738	2740	2745	rVV4	7352	10060	1.00%	0.115%
49	19.654	2747	2752	2757	rBV	6602	10286	1.03%	0.117%
50	19.819	2778	2780	2782	rBV2	1595	1483	0.15%	0.017%
51	19.866	2786	2788	2792	rVB4	1600	1817	0.18%	0.021%
52	20.018	2808	2814	2822	rVB	699441	1002621	100.00%	11.415%
53	20.077	2822	2824	2826	rBV2	1619	1258	0.13%	0.014%
54	20.341	2865	2869	2870	rBV3	1738	1982	0.20%	0.023%
55	20.435	2882	2885	2886	rBV2	1806	2228	0.22%	0.025%
56	20.471	2889	2891	2893	rBV2	1869	1700	0.17%	0.019%
57	20.570	2906	2908	2909	rVB2	1943	1037	0.10%	0.012%
58	20.588	2909	2911	2913	rBV3	3165	2684	0.27%	0.031%
59	20.817	2949	2950	2952	rBV2	3224	2906	0.29%	0.033%
60	20.970	2973	2976	2977	rBV3	2208	2346	0.23%	0.027%
61	21.452	3056	3058	3060	rBV3	2771	1413	0.14%	0.016%
62	21.510	3066	3068	3071	rBV4	2312	2230	0.22%	0.025%
63	21.863	3127	3128	3130	rBV2	5452	3192	0.32%	0.036%
64	21.880	3130	3131	3132	rVV	3309	1384	0.14%	0.016%
65	21.963	3137	3145	3153	rVV	306515	555678	55.42%	6.326%
66	22.139	3173	3175	3176	rVB2	3192	1452	0.14%	0.017%
67	22.157	3176	3178	3181	rVB3	2600	1601	0.16%	0.018%
68	22.368	3212	3214	3215	rBV2	2635	1501	0.15%	0.017%
69	22.644	3259	3261	3263	rVB2	2807	1606	0.16%	0.018%
70	23.049	3328	3330	3332	rVB3	2539	1184	0.12%	0.013%
71	23.449	3396	3398	3401	rBV4	4065	3681	0.37%	0.042%
72	23.966	3482	3486	3487	rBV4	2753	3058	0.31%	0.035%
73	24.060	3501	3502	3505	rBV3	3406	3748	0.37%	0.043%
74	24.730	3614	3616	3618	rBV3	2879	2809	0.28%	0.032%
75	25.059	3671	3672	3674	rVB2	3980	2804	0.28%	0.032%
76	25.211	3685	3698	3709	rVB2	305472	916088	91.37%	10.429%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011022\
 Data File : BG051932.D
 Acq On : 10 Jan 2022 16:16
 Operator : CG/JU
 Sample : PB141942BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK942

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	25.452	3727	3739	3752	rBV2	169809	538780	53.74%	6.134%
78	26.016	3833	3835	3836	rVB2	3359	1758	0.18%	0.020%
79	26.621	3936	3938	3940	rVB3	2421	1340	0.13%	0.015%
80	27.244	4042	4044	4046	rBV2	2986	2419	0.24%	0.028%
81	27.267	4046	4048	4049	rBV2	3758	2483	0.25%	0.028%
82	27.784	4132	4136	4137	rBV4	3281	3541	0.35%	0.040%
83	27.908	4155	4157	4160	rBV4	3328	3870	0.39%	0.044%
84	27.996	4170	4172	4173	rBV2	2664	1990	0.20%	0.023%
85	28.712	4292	4294	4295	rVB2	2523	1687	0.17%	0.019%
86	28.977	4337	4339	4341	rBV3	3466	2927	0.29%	0.033%
87	29.036	4347	4349	4350	rBV2	3299	2259	0.23%	0.026%
88	29.071	4354	4355	4356	rBV	3369	1848	0.18%	0.021%
89	29.605	4444	4446	4447	rBV2	2178	1021	0.10%	0.012%
90	29.646	4451	4453	4454	rBV2	3002	1841	0.18%	0.021%
91	29.782	4474	4476	4479	rBV3	3185	3233	0.32%	0.037%
92	29.817	4480	4482	4483	rVV2	2727	1512	0.15%	0.017%
93	30.181	4543	4544	4546	rBV2	3305	2285	0.23%	0.026%
94	30.375	4576	4577	4579	rBV2	2929	2415	0.24%	0.027%
95	30.545	4604	4606	4608	rBV3	2329	1337	0.13%	0.015%
96	31.332	4739	4740	4742	rBV2	3518	2807	0.28%	0.032%
97	31.538	4773	4775	4777	rBV3	3094	2517	0.25%	0.029%
98	31.720	4804	4806	4807	rBV2	2527	1405	0.14%	0.016%




Sum of corrected areas: 8783676

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011022\
Data File : BG051932.D
Acq On : 10 Jan 2022 16:16
Operator : CG/JU
Sample : PB141942BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK942

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

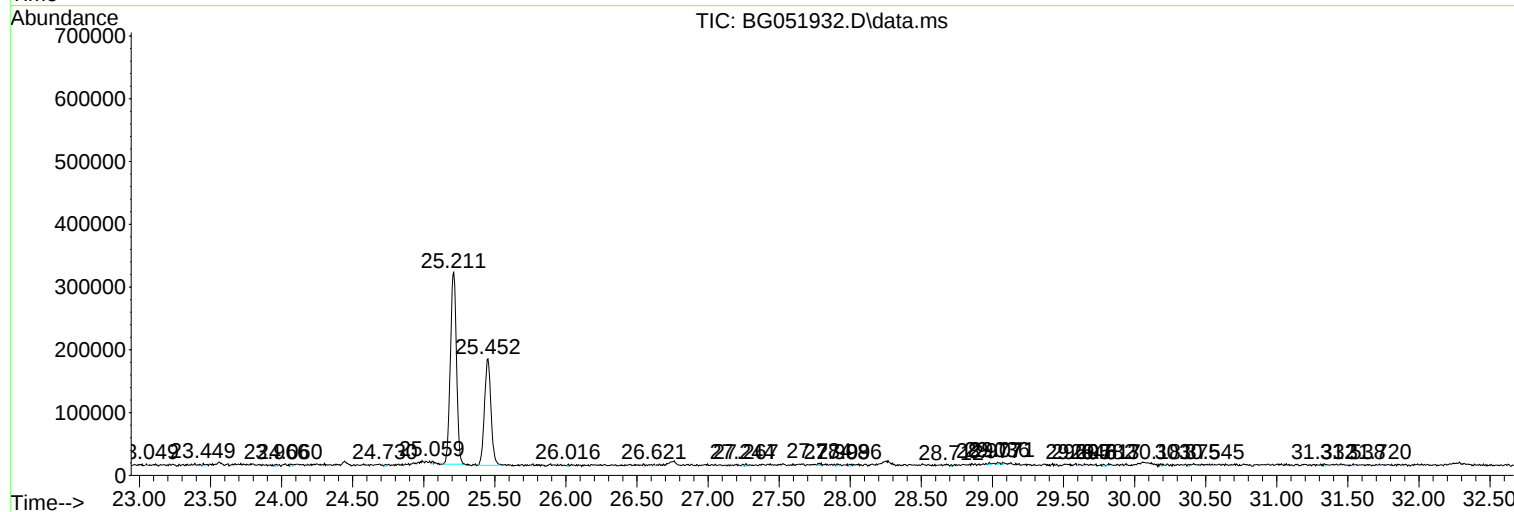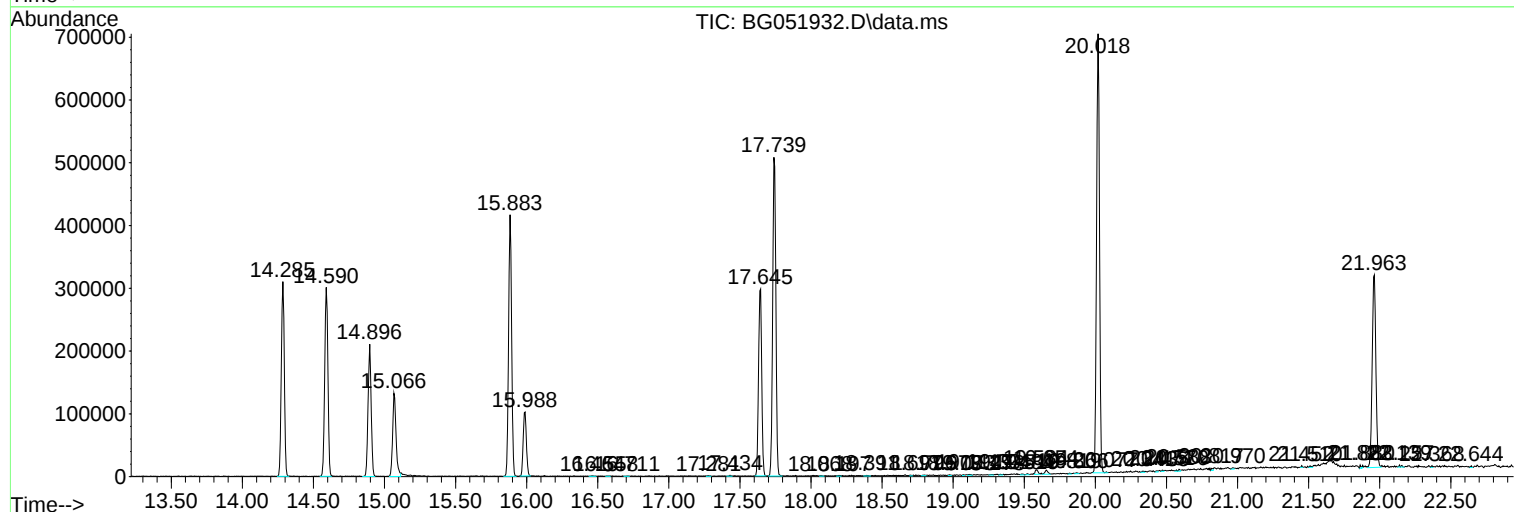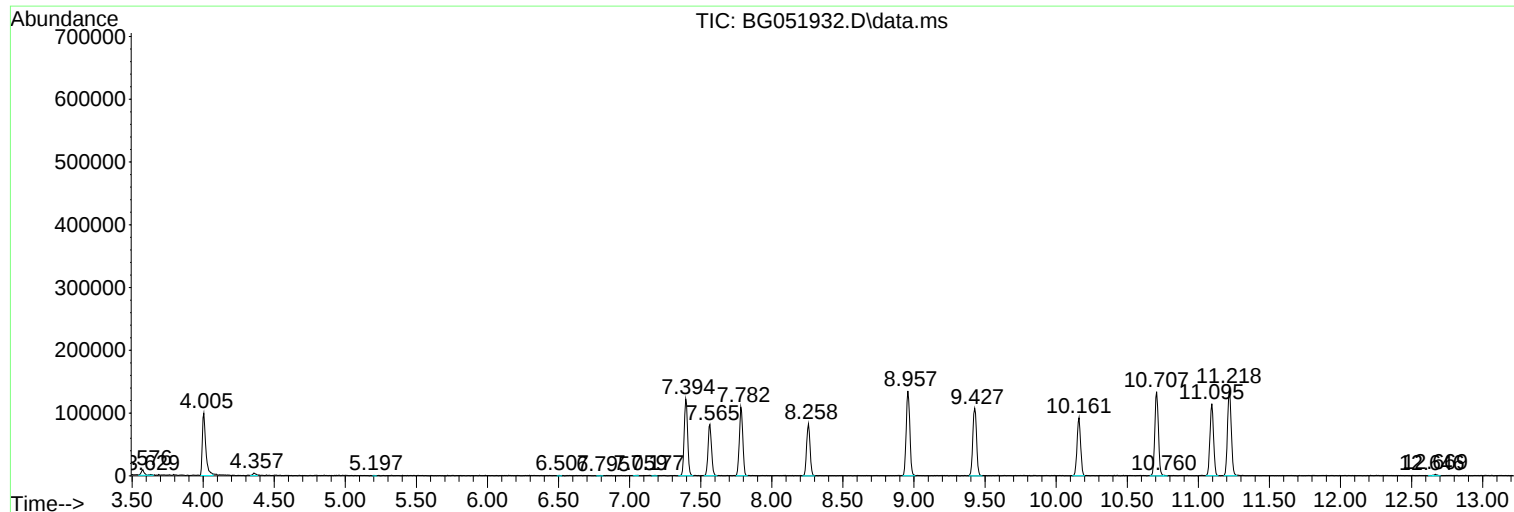

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011022\
Data File : BG051932.D
Acq On : 10 Jan 2022 16:16
Operator : CG/JU
Sample : PB141942BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK942

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011022\
Data File : BG051932.D
Acq On : 10 Jan 2022 16:16
Operator : CG/JU
Sample : PB141942BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK942

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------